INCH-POUND

A-A-51961A
21 August 1992
SUPERSEDING
A-A-0051961(DM)
29 MAY 1987

COMMERCIAL ITEM DESCRIPTION

TUBE, STOMACH, SURGICAL (Levin)

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-T-36612(2) which is cancelled.

This commercial item description covers three sizes of reusable Levin stomach tubes suitable for aspirating, tube feeding or irrigating.

Salient characteristics:

Classification. Tubes covered by this specification shall be of the following sizes as specified in Notes.

Size
12 Fr
16 Fr
18 Fr

General. Shall be non-sterile, reusable, single-lumen stomach tubes of the Levin design as shown in Figure 1; as an alternate, the proximal end shall be provided with an integral or attached funnel type connector.

Style and design. The stomach tubes shall be a continuous tube and shall comply with Figure 1 and the requirements specified herein.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Two pairs of diametrically opposed, oval-shaped "eyes" shall be located as shown on the drawing. As an alternate, the tube may have five oval eyes. One eye shall sever the radiopaque line at a point beginning 2 inches (5.08 cm) from the distal end. Two pairs of eyes shall be present distal to the eye on the radiopaque line. Each eye of a pair shall oppose the other and shall be 90° away from the radiopaque line. Oval eyes shall have well rounded, smoothly beveled edges.

The cross-sectional area of each eye shall be no less than 85 percent of each tube's cross-sectional area, nor greater than 115 percent of each tube's cross-sectional area. By definition, the cross-sectional area of each tube shall be based on the tube's inside diameter.

Each eye shall be chamfered and rounded.

The distal edge of each tube shall be rounded.

The tube shall be supplied clean and shall be capable of sterilization by commercially prepared cold sterilization solutions and by steam autoclaving. The tube shall be unaffected by oil base lubricants.

Materials. All stomach tubes covered by this document shall be fabricated from clear PVC (Polyvinylchloride). Samples of this material shall be subjected to the test method specified for each requirement and shall meet with the values specified as follows:

Material Requirements

Requirement	Value	Test Method
Elastic Modulus:	10,000 psi, Maximum	ASTM D638
Water Absorption:	0.5 percent, Maximum	ASTM D570*
Shore Hardness:	A50-A100	ASTM D2240
Toxicity:	Non-Toxic	ASTM F895

* Perform the 24-hour water absorption test.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Marking. Each tube covered by this document shall be permanently and legibly marked with depth graduation at 18, 22, 26, & 30 inches from its distal end. Tolerance on these measurements shall be ±1/4 inch; chain tolerancing shall not be used. Tube shall also be permanently and legibly marked with the manufacturer's name or registered trade mark and the French size.

Radiopacity. Each tube covered by this document shall have a radiopaque stripe spanning its entire length. This stripe shall have a minimum relative attenuation coefficient of 95 percent. Sample stomach tubes shall be tested for radiopacity in accordance with Method B of ASTM F640.

Pyrogens and biological tests. The tube shall meet the requirements of the United States Pharmacopeia (USP) for pyrogens and Type II biocompatibility tests.

Certificate of biocompatibility. A certificate of compliance, stipulating that offered items meet the biocompatibility test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there has been no changes to material, formulation and the method of processing since actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and National Stock Number (NSN), a statement certifying that material processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

Workmanship. Each tube covered by this document shall be free from blooming, blisters, fish-eyes, frosting, pits, pimples, shorts, warpage, wrinkles, and any other defects that detract from their appearance or impair their serviceability.

Definitions of defects listed above shall be in accordance with ASTM D883, "Standard of Definitions of Terms Relating to Plastics". Stomach tubes shall be supplied clean.

Unit. Package (PG). One package containing fifty individually packaged, clean stomach tubes of one French size as specified, constitutes one unit. Each tube shall be individually packaged in a transparent peel-open container.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Physical properties testing. Tubes after autoclaving for 20 minutes at 250°F and 15 psi shall be tested for breaking strength. The test method shall be American Society for Testing and Materials Standard D412. Any break which is shown to have been caused by the gripping actions of the jaws of the testing machine may be disregarded and another tube tested. Breaking strength shall be 12 pounds for 12 French, 17.5 pounds for 16 French and 25 pounds for 18 French tubes. As an alternate, dumbell specimens which have been sterilized as above may be tested. If dumbell specimens are used, the specimens shall have a tensile strength of 1400 psi minimum.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Adapter test. A molded adapter shall be secured to the proximal end of each tube. The adapter-to-tube connection shall withstand a 15-pound tensile load. As an alternate, an integral adapter may be used in lieu of molded adapter.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at level S-2, Acceptable Quality Level (AQL) 0.65 percent. Acquisition of samples from raw material lots shall be conducted in accordance with section 12.2 of ASTM D1899.

Sampling for inspection of the end-item shall be conducted in accordance with MIL-STD-105 at Level S-2, AQL 1.0 percent. The unit of product for purposes of end-item inspection shall be one stomach tube as specified herein.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-225-9719	TUBE, STOMACH, SURGICAL, Plastic, Radiopaque, Levin, 16 Fr, 50s
6515-00-935-4063	TUBE, STOMACH, SURGICAL, Plastic, Radiopaque, Levin, 12 Fr, 50s
6515-00-935-4065	TUBE, STOMACH, SURGICAL, Plastic, Radiopaque, Levin, 18 Fr, 50s

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-4565
Location: AA51961A/S11

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

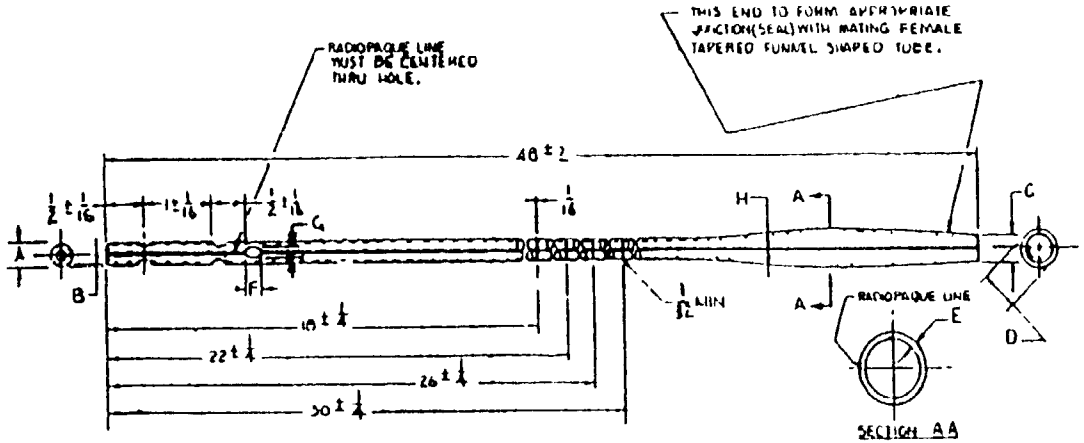


NSN	SIZE	A OD	B WALL THICKNESS	C BUBBLE AT CUTOFF	D BUBBLE OD	E BUBBLE WALL	F EYE WIDTH	G EYE HEIGHT	H WIDTH OF RADIOPAQUE LINE
6515 00 935 4063	12 Fr	.156	.020	.259	.341	.048	.140	.050	.035 .060
6515-00 225-9719	16Fr	.209	.025	.269	.341	.048	.185	.085	.035 .060
6515-00-935-4065	18Fr	.234	.027	.259	.341	.048	.212	.095	.035 .060
TOLERANCES			±.015	MIN	±.020	±.020	±.010	REF.	REF.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ON
FRACTIONS ±1/64 DECIMALS = ANGLES =

GENERAL NOTES.

1 TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.

ALTERNATE TIP DESIGN				
NSN	SIZE	F	G	J
6515-00 935-4063	12 FR	.140	060	406
6515 00 225-9719	16 FR	250	125	531
6515-00-935-4065	18 FR	250	.125	343
TOLERANCES		REF	REF	±1/16

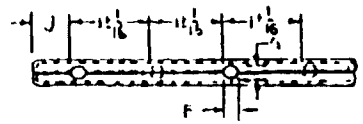

NOTE.
ALL FEATURES AND DIMENSIONS SAME AS ABOVE EXCEPT AS SHOWN.

A-A-51961A

FIGURE 1 TUBE, STOMACH, SURGICAL, PLASTIC, RADIOPAQUE, LEVIN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:03Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-51961A	21 August 1992

3 DOCUMENT TITLE
TUBE, STOMACH, SURGICAL (Levin)

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)*

5 REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial 215-737-2870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil downloaded 2010-26T09:03Z
Check the source to verify that this is the current version before use.