INCH-POUND

A-A-51992/1
19 March 1993

COMMERCIAL ITEM DESCRIPTION SHEET

HOLDER, SUTURE NEEDLE, Castroviejo

The General Services Administration has authorized the use of this Commercial Item Description Sheet.

The complete requirements for procuring suture needle holders shall consist of this document and the issue in effect of Commercial Item Description A-A-51992B.

Salient characteristics:

Style, design and dimensions. This specification covers the following style of ophthalmic and plastic surgery suture needle holders:

Style I - Delicate jaws

Class 1 - Straight, 5-1/2 inches
Class 2 - Curved, 5-1/2 inches

The suture needle holders shall be in accordance with Figure 1.

Notes:

1. Intended use: Suture needle holders of the Castroviejo design covered in this Commercial Item Description Sheet are intended for aiding in ophthalmic and plastic surgery procedures on the eye.

2. Copies of Commercial Item Description A-A-51992B may be obtained by writing the Defense Printing Service Detachment Office; Bldg. 4D; DoD-SSP; 700 Robbins Avenue; Philadelphia, PA; 19222-5094

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution in unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:04Z
Check the source to verify that this is the current version before use.

3. National Stock Numbers, Item Identifications and Classes.

NATIONAL STOCK NUMBER	Item Identification	Class
6515-01-120-5013	HOLDER, SUTURE NEEDLE, Castroviejo, Curved, 5-1/2 inches	2
6515-01-120-5014	HOLDER, SUTURE NEEDLE, Castroviejo, Straight, 5-1/2 inches	1

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5354
Location: genhold\S17

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:04Z
Check the source to verify that this is the currentversion before use.

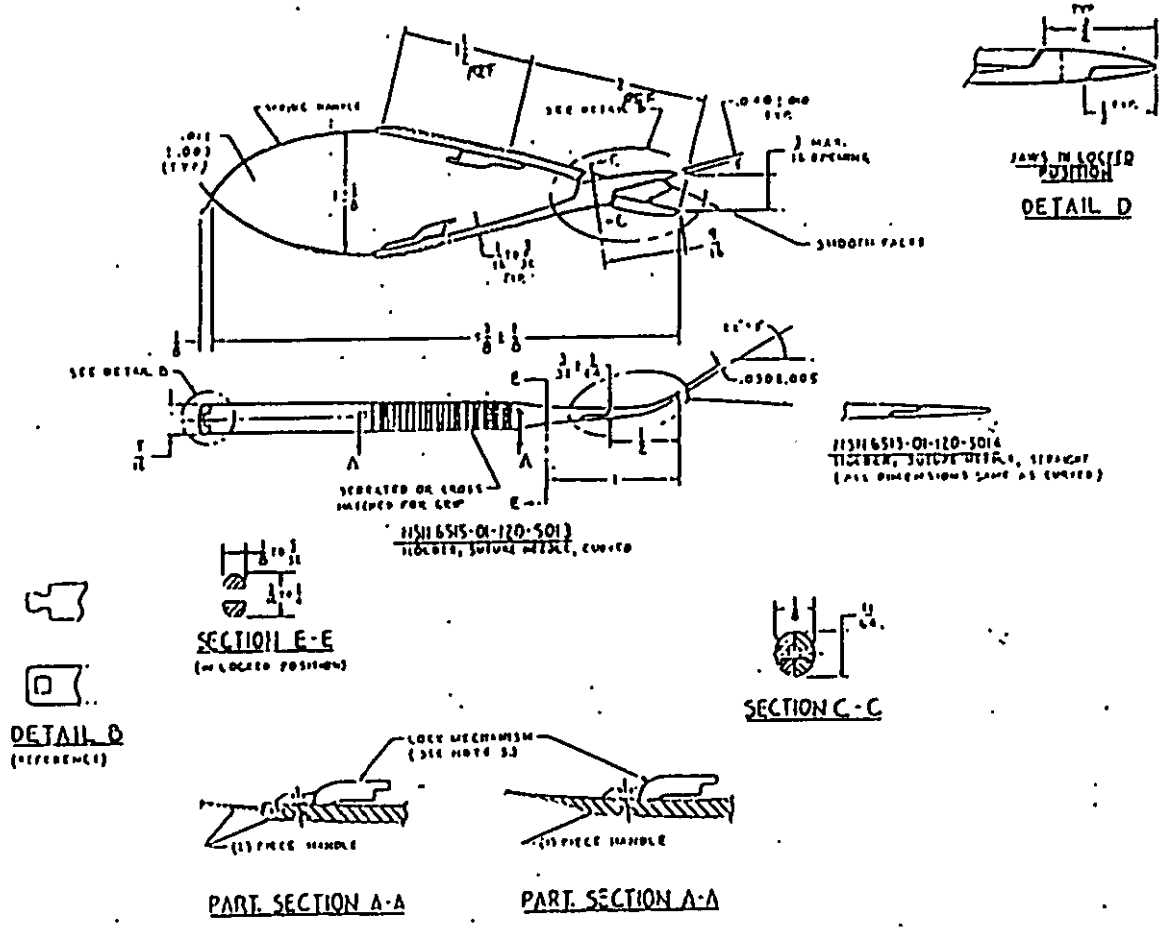

NOTES:

1. TOLERANCES INDICATED ARE INTENDED TO PERMIT VARIATION IN DESIGN AND ARE NOT INTENDED TO PERMIT VARIANCES WITHIN A SAMPLE INSTRUMENT WHICH WOULD SACRIFICE QUALITY, FUNCTION OR WORKMANSHIP.
2. FORCEPS BLADE EDGES AND INSIDE FACES SHALL BE UNIFORM AND MATCH EXACTLY WITHIN A SINGLE INSTRUMENT.
3. LOCK MECHANISM TO ENGAGE BY SLIGHT PRESSURE AT SERRATED PORTIONS OF HANDLES TO DISENGAGE BY ADDITIONAL SLIGHT PRESSURE IN SAME PLANE.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	±	±

A-A-51952/1

FIGURE 1 HOLDER, SUTURE NEEDLE, CASTROVIEJO

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:04Z
Check the source to verify that this is the current version before use.