INCH-POUND

MIL-T-26963D(USAF)
30 APRIL 1992
SUPERSEDING
MIL-T-26963C(USAF)
30 December 1982

MILITARY SPECIFICATION

TESTER, PRESSURE GAGE, HYDRAULIC, PORTABLE TYPE MP-1

This specification is approved for use by the Department of the Air Force and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of portable hydraulic pressure gage tester, designated type MP-1.

2. APPLICABLE DOCUMENTS

* 2.1 Government documents.

2.1.1 Specifications standards and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATIONS

FEDERAL

PPP-B-601	Box, Wood, Cleated-Plywood
PPP-B-636	Box, Shipping Fiberboard

MILITARY

MIL-P-116	Preservation, Methods of
DOD-D-1000	Drawing, Engineering and Associated List
MIL-L-5020	Liquid, Compass, Aircraft
MIL-C-5541	Chemical, Conversion Coatings on Aluminum and Aluminum Alloys
MIL-S-7742	Screw Threads, Standard, Optimum Selected Series, General Specification for
MIL-A-8625	Anodic Coatings, For Aluminum and Aluminum Alloys

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: The Technology & Industrial Services Division, SA-ALC/TIRDM, Kelly AFB, TX 78241-5609 by using the Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC/NA FSC 6685

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 20261O-20T10:33Z
Check the source to verify that this is the current version before use.

STANDARDS

FEDERAL

FED-STD-595	Colors used in Government Procurement

MILITARY

MIL-STD-129	Marking for Shipment and Storage
MIL-STD-130	Identification Marking of US Military Property
MIL-STD-810	Environmental Test Methods and Engineering Guidelines
MIL-STD-831	Test Reports, Preparation of
MIL-STD-970	Standards and Specifications, Order of Preference for the Selection of
MIL-STD-1186	Cushioning, Anchoring, Bracing, Blocking and Waterproofing, with Appropriate Test Methods

(Unless otherwise indicated, copies of federal and military specifications, standards, and handbooks are available from the Naval Publications Standardization Documents Order Desk, Bldg 4D, 700 Robbins Avenue, Philadelphia PA 19111-5094.)

2.2 Non-Government publications. The following document(s) form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DOD adopted are those listed in the issue of the DODISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DODISS are the issues of the documents cited in the solicitation (se 6.2).

Official Classification Committee

Uniform Freight Classification Rules

(Application for copies should be addressed to the Official Classification Committee, Room 202, Union Station, 516 West Jackson Boulevard, Chicago, IL 60606.)

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM B633 Zinc on Iron and Steel, Electro-deposited Coating of

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103-1137.)

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this document and the references cited herein, the text of this document takes precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

* 3.1 First article. The tester furnished under this specification shall be a product which has been tested and has passed the first article tests specified herein.

3.2 Component parts. The tester shall consist of a hand operated piston type pump, accessories, and gages contained in a steel carrying case.

3.3 Selection of specification and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected according to MIL-STD-970 except as provided in 3.3.1 and 3.3.2.

3.3.1 Commercial parts. Commercial parts having suitable properties may be used where on the date of invitation for bids, there are no suitable standard parts. In any case, commercial pins, having suitable properties may be used provided:

a. They can be replaced by the standard parts (MS or AN) without alteration.

b. The corresponding standard part numbers are referenced in the parts list and, if practical, on the contractor,s drawings.

3.3.2 Standard parts. With the exception in 3.3, MS and AN standard parts shall be used where they suit the purpose. They shall be identified on the drawings by their part number.

3.4 Materials. Materials shall conform to the applicable specifications as specified herein. When materials are used which are not specifically designated, they shall be entirely suitable for the purpose.

3.4.1 Fungus-proof materials. Materials that are nutrients for fungi shall not be used where it is practical to avoid them. Where used and not hermetically sealed, they shall be treated with a fungicidal agent acceptable to the procuring activity. However, if they will be used in a hermetically sealed enclosure, fungicidal treatment will not be necessary.

3.4.2 Protective treatment. When materials are used in the construction of the tester that are subject to deterioration when exposed to climatic and environmental conditions likely to occur during service usage, they shall be protected against such deterioration in such a manner that will in no way prevent compliance with the performance requirements of this specifications. The use of any protective coating that will crack, chip, or scale with age or extremes of climatic and environmental conditions shall be avoided.

3.4.3, Metals. Metals shall be of the corrosion-resistant type or treated to resist corrosion due to fuels, salt spray, or atmospheric conditions likely to be met in storage or normal service.

* 3.4.4 Reclaimed materials. The use of reclaimed materials shall be encouraged to the maximum extent possible.

3.5 Design and construction.

3.5.1 Design. The tester shall consist of an integral unit, designed to provide accurate determination of pressures. The design shall provide for

Source: https://assist.dla.mil -- Downloaded: 202610-20T10:33Z
Check the source to verify that this is the current version before use.

comparison tests wherein an aircraft pressure gage under test, is compared with one of the master gages provided with the tester.

3.5.2 The detailed mechanical design of the tester shall be accomplished by the contractor subject to the requirements of this specification, these requirements being detailed only to the extent considered necessary to obtain the desired mechanical characteristics, performance, and permanence in accuracy of indication. The design, layout, and assembly of the tester and its component parts shall be such as to facilitate quantity production and ease of maintenance.

* 3.5.3 The tester shall be designed for operation on light and medium weight oils.

3.5.4 Construction. The tester shall be constructed similar to Figure 1 and provided herein, with minor alterations as to component parts provided the revisions do not interfere with or alter their intended function. A combination filler and vent plug may be incorporated atop the body.

3.6 Performance. The tester shall be capable of meeting the test requirements specified in Section 4 when subjected to the following conditions:

a. Temperature. Temperature ranging from -54° Centigrade (C) to +71°C.

b. Humidity. Relative humidity up to 95 percent.

* 3.7 Interchangeability. All parts having the same manufacturer's part number shall be directly and completely interchangeable with each other with respect to installation and performance. Changes in manufacturer's part numbers shall be governed by the drawing number requirements of DOD-D-1000.

3.8 Pump. The pump shall conform substantially to Figure 1 as to size and format. It shall consist of the body, reservoir, and drip pan.

* 3.8.1 Body. The body shall be cast of heat treated aluminum alloy. It shall contain the piston, which is operated by a hand lever, a vent plug, two vertical outlets and one horizontal outlet, a valve to gradually relieve pressure back to the reservoir and a precision pressure adjustment valve which can be used to increase or decrease pressure reading. These valves will be provided with stops to prevent accidental removal during operation. The needles and seats of the valves shall be of stainless steel. The outlet shall have 0.5000-UNF3B threads in accordance with MIL-S-7742 and shall contain plugs for shipping purposes.

3.8.2 Reservoir. The reservoir shall be constructed of stainless steel or aluminum alloy and designed to contain a minimum of 1-1/2 pints of liquid. If a combination filler and vent plug is not used, a filler plug shall be provided on the end of the reservoir. A washer shall be provided for the plug to prevent seepage of liquid.

3.8.3 Drip pan. The drip pan shall be cast of heat treated aluminum alloy and shall be 20-3/4 inches in length, 5 inches in width and 1 inch in depth. A tolerance of ±1/8 inch shall apply for the dimensions. The body of the pump shall be bolted to the drip pan.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

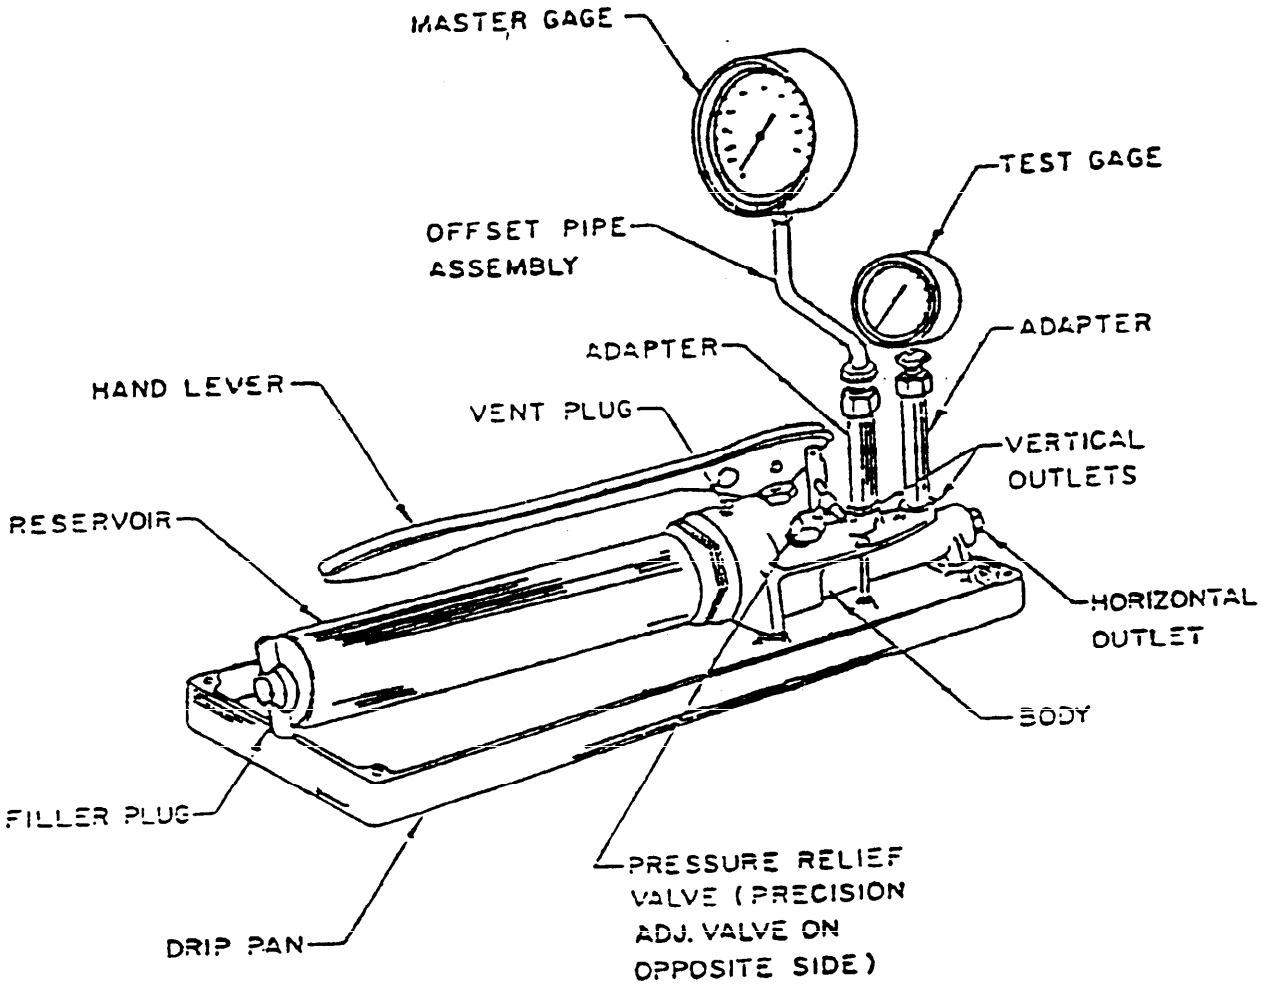


FIGURE I. Tester

Source: https://assist.dla.mil -- Downloaded: 20260-20T10:33Z
Check the source to verify that this is the current version before use.

3.9 Gages. Four master gages shall be supplied with the tester. The case for each gage shall be fabricated from brass, steel or aluminum and shall employ a 4-1/2 inch size dial. Each gage shall be provided with a calibration adjustment located on the face of the dial for facilitating recalibration of the instrument. The gages shall be provided with fittings for connecting to either the adapters or the offset pipe assembly. The cases for the gages shall be sealed so that the gages are capable of resisting deterioration when subjected to the environmental conditions specified in Section 4. The pressure outlet of each gage shall be provided with a plug so as to completely seal the gage while stored in the case. The plugs shall be removed during use. The basic gage design shall incorporate features for preventing breaking of the cover glass in the event the internal component parts fail when pressure over the respective operating range is applied. The range, accuracy, and calibration of the gages shall be as specified below:

a. Gage No. 1: Range 0 to 160 pounds per square inch (psi) having an accuracy of 1/4 of 1 percent of full scale. Dial calibrated in maximum increments of 1.0 psi and numbered at maximum intervals of 10 psi starting with zero.

b. Gage No. 2: Range 0 to 600 psi having an accuracy of 1/4 of 1 percent of full scale. Dial calibrated in maximum increments of 2 psi and numbered at maximum increments of 50 psi starting with zero.

c. Gage No. 3: Range 0 to 5000 psi having an accuracy of 1/4 of 1 percent of full scale. Dial calibrated in mximum increments of 20 psi and numbered at maximum increments of 500 psi starting with zero.

* d. Gage No. 4: Range 0 to 10,000 psi having an accuracy of 1/4 of 1 percent of full scale. Dial calibration in maximum increments of 50 psi and numbered at maximum increments of 1000 psi starting with zero.

3.10 Accessories. The accessories consisting of at least one offset pipe assembly, two adapters, and tools shall be furnished with the tester.

* 3.10.1 Adapters. The adapters, with a length of 3 ± 1/4 inch after installation on the pump body, shall be provided as shown on Figure 1. One end of each adapter shall fit into either of the vertical outlets shown on Figure 1. The opposite end of each adapter shall provide means for interchangeable mounting of the gages, the offset assembly or a 1/2 inch national taper pipe thread (NPT) female fitting supplied with the adapters. It will be designed and constructed so that the pump could not become loose in the case during rough service conditions. A 1/2 inch NPT female fitting (provided with a 1/2 to 1/4 inch NPT reducer) shall be furnished for each adapter. One adapter may be eliminated if the offset pipe assembly incorporates the additional length of an adapter and still complies to the offset distance and interchangeable mounting as specified above. The gages will be protected by padding to prevent broken or scratched crystals and damage to the gages.

3.10.2 Offset pipe assembly. The pipe assembly shall be provided to offset a distance of 6 inches +1 inch, either the master gage being used or the instrument under test, so that the visibility of one instrument is not blocked by the other. One end of the assembly shall mount on one of the adapters and the opposite end of the assembly shall provide means for interchangeable mounting of either the 1/2 inch

Source: https://assist.dla.mil -- Downloaded: 20260-20T10:33Z
Check the source to verify that this is the current version before use.

NPT female fittings supplied with the adapters, or one of the master gages, as required. An offset pipe assembly for the back connection gage should also be supplied.

3.10.3 Tools. At least two open end wrenches shall be provided for making all external connections to the pump, gages, and accessories.

3.10.4 Case. The case shall conform substantially to Figure 2. The overall dimension shall not exceed 22 inches in length, 9-1/4 inches in width and 8-1/2 inches in depth. It shall employ welded construction and shall be fabricated of 0.046 inch thick sheet steel so as to withstand rough service usage without damage to the tester of its component parts. A handle shall be provided on the lid for carrying the case. Two suitcase latches shall be provided for fastening the lid.

3.10.4.1 The pump, accessories, and gages shall be individually mounted in the case so that one item may be easily removed without removing another item. The wrenches and pipe assembly, shall be mounted on the sides of the case in such a manner that when the lid is closed it will form a hold down for each of these items. The pump shall be mounted in the bottom of the case and secured by a method which allows quick and easy removal. This shall not be accomplished by screws, bolts, or nuts. The gages shall be mounted on the side of the case and may be secured in place by the lid or as shown in Figure 2.

3.10.4.2 Handle. A hinged metal handle shall be mounted on the outside surface of the lid and shall be located in the optimum position with respect to weight distribution. The handle shall provide a clearance from the case sufficient to pass a block 1-7/8 by 4-3/8 inches in cross section and having the edges rounded to 15/16 inch radius. The grip portion of the handle shall be of a nonmetallic material and shaped to fit the hand comfortably.

3.10.4.3 Operating instructions. Operating instruction entered on a chart shall be permanently attached to the inside surface of the case lid. The body of the chart shall be white and the markings black, shall withstand the effects of the tests specified in Section 4, and shall clearly define the set-up connections, and operation of the tester.

3.11 Weight. The weight of the tester, including the case and the component parts of the tester, shall not exceed 55 pounds.

3.12 Finish and protective coating.

3.12.1 Finish. The exterior and interior surfaces of the carrying case provided for the tester shall be finished in accordance with FED-STD-595, color No. 13538.

3.12.2 Aluminum alloy parts. Aluminum alloy parts shall be covered with an anodic film conforming to MIL-A-8625, except as follows:

3.12.2.1 Aluminum alloys which do not anodize satisfactorily shall be coated with a chemical film in accordance with MIL-C-5541.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

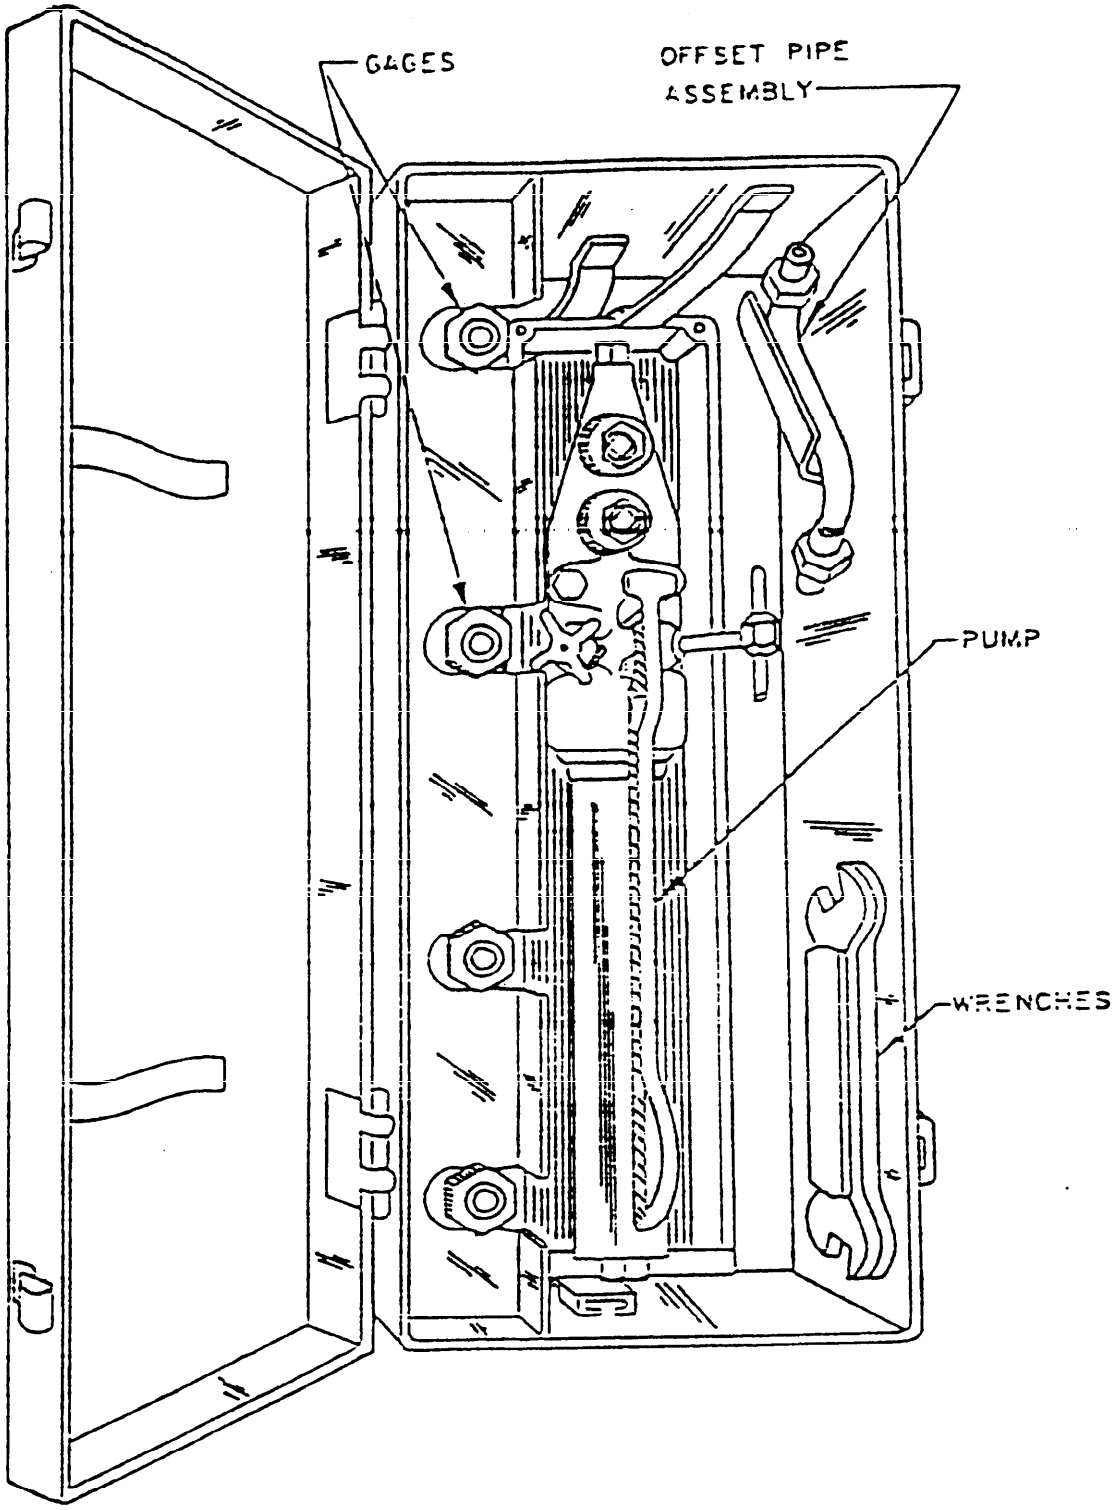


FIGURE II. Case

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

3.12.2.2 Where the primary purpose of the treatment is to afford a suitable paint base, chemical treatments in accordance with MIL-C-5541 may be used in lieu of anodizing.

3.12.2.3 Castings containing nonaluminum alloy integral inserts may be treated with a chemical film in accordance with MIL-C-5541 in lieu of anodizing.

* 3.12.3 Steel parts. Steel parts shall be zinc plated where practical in accordance with ASTM B633 Type II, with a thickness of 5 (micrometer) minimum.

3.13 Identification of product. Equipment, assemblies, and parts shall be marked for identification in accordance with MIL-STD-130.

3.14 Workmanship.

3.14.1 General. The tester, including all parts and accessories, shall be constructed in a thoroughly workmanlike manner. Particular attention shall be given to neatness, welding, machining, forming of parts, painting, and freedom of parts from burrs and sharp edges.

3.14.2 Dimensions. Dimensions and tolerances not specified shall be as close as is consistent with the best shop practices. Where dimensions and tolerances may affect the interchangeability, operation, or performance of the tester, they shall be held or limited accordingly.

3.14.3 Cleaning. The tester shall be thoroughly cleaned of metal chips and other foreign material after final assembly. Burrs and sharp edges shall be removed.

4. QUALITY ASSURANCE PROVISIONS

* 4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all tests and inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

* 4.2 Classification of tests. The inspection and testing of the tester shall be classified as follows:

a. First article tests

b. Quality conformance tests

4.3 Test conditions.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

4.3.1 Standard atmospheric conditions. Whenever the pressure and the temperature existing at the time of the test are not specified definitely, it is understood that the test is to be made at atmospheric pressure (approximately 29.92 inches mercury) and at room temperature (approximately +25°C). When tests are made with atmospheric pressure or room temperature differing materially from the above values, proper allowance shall be made for the difference from the specified condition.

4.3.2 Filling medium. For the low temperature test the pump shall be filled with compass liquid conforming to MIL-L-5020. For all other tests the pump shall be filled with a light or medium weight oil.

* 4.4 First article tests.

* 4.4.1 First article samples. Unless otherwise specified, as soon as practicable after the award of the contract or orders the contractor shall submit two testers to the tests as specified herein and in accordance with the contract or order.

* 4.4.2 First article tests. The first article tests shall consist of all tests specified under 4.6.

* 4.4.3 First article tests report. The contractor shall prepare a report of the first article tests in accordance with MIL-STD-831. Two copies shall be furnished to the procuring activity.

* 4.5 Quality conformance tests. Quality conformance tests shall consist of:

a. Individual tests

b. Sampling plans A and B

4.5.1 Individual tests. Each tester shall be subjected to the following tests as described under 4.6.

a. Examination of product

b. Gage calibration

c. Functional operation at room temperature

4.5.2 Sampling plans and tests.

4.5.2.1 Sampling plan A. One tester selected at random from each lot of 50 or less on the contract or order shall be subjected to the following tests as described under 4.6.

a. Individual tests

b. Low temperature

c. High temperature

Source: https://assist.dla.mil -- Downloaded: 20260-20T10:33Z
Check the source to verify that this is the current version before use.

4.5.2.1.1 Lot. A lot shall consist of testers manufactured under essentially the same condition and submitted for acceptance at substantially the same time.

4.5.2.1.2 Rejection and retest. When one or more items from a lot fail to meet the specification, acceptance of all items in the lot will be withheld until the extent and cause of failure are determined. After corrections have been made, all necessary tests shall be repeated.

4.5.2.1.2.1 Individual tests may continue. For production reasons, individual tests may be continued pending the investigation of a sampling test failure. Final acceptance of the entire lot shall not be made until it is determined that the lot meets all the requirements of the specification.

4.5.2.2 Sampling plan B. Unless otherwise specified, two testers selected at random from the first 10 items of the contract or order shall be subjected to the following tests as described under 4.6.

a. Sampling plan A tests

b. Humidity

4.5.2.2.1 Rejection and retest. When one item selected from a production run fails to meet the specification, no items still on hand or later produced shall be accepted until the extent and cause of failure are determined.

4.5.2.2.1.1 Individual tests may continue. For operational reasons, individual tests may be continued pending the investigation of a sampling test failure; but final acceptance of items on hand or later produced shall not be made until it is determined that items meet all the requirements of the specification.

4.5.3 Defects in items already accepted. The investigation of a test failure could indicate that defects may exist in items already accepted. If so, the contractor shall fully advise the procuring activity of all defects likely to be found and methods of correcting them.

4.6 Test methods.

4.6.1 Examination of product. Each tester shall be inspected to determine compliance with the requirements specified herein with respect to dimensions, material, workmanship, and marking.

4.6.2 Gage calibration. The four master gages called out in 3.9 and furnished with each tester shall be tested with approved standards. Each gage shall be checked as specified below:

Gage No.	Check Point	Tolerance at Each Check Point
1	Every 5 pounds from 0-160 psi	±0.4 psi
2	Every 30 pounds from 0-600 psi	±1.5 psi
3	Every 100 pounts from 0-5,000 psi	±12.5 psi
4	Every 250 pounds from 0-10,000 psi	±25.0 psi

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

4.6.3 Functional operation at room temperature. The reservoir of each tester shall be filled with lightweight oil. A test gage and the No. 4 master gage specified in 3.9 shall be attached to the tester. Testing shall be conducted to determine the following:

a. Pressure is readily developed when the pressure relief valve is closed, the vent plug opened, and the hand lever is operated.

b. Pressure to the master gage and the test gage can be varied smoothly and with a high degree of sensitivity by means of the precision adjustment valve.

c. Pressure readings registered by the master gage and the test gage are the same taking into consideration the accuracy tolerance of the gages being used. Reading shall be taken at each 1,000 psi increment over the range of 0 to 10,000 psi.

d. With pressure developed by means of the hand lever to 10,000 psi as evidenced by the reading of the No. 4 master gage, no change in indication of the master gage shall be visually detected during a check period of 30 seconds.

4.6.4 Low temperature. The tester shall be placed within a test chamber capable of maintaining an internal temperature of -55° ±2°C for a period of 24 hours. At the end of the 24-hour period, the temperature shall be changed to -40° ±2°C. At the end of an additional 2-hour period, with this temperature maintained the tester shall be subjected to the tests specified in 4.6.3 with the exception of the test specified therein under c.

4.6.4.1 The four master gages shall be placed within a test chamber capable of maintaining an internal temperature of -55° ±2° for a period of 24 hours. At the end of the 24-hour period, the temperature shall be changed to -40°±2°C. At the end of an additional 4-hour period, with this temperature maintained, each gage shall be tested as indicated below by means of the approved standards maintained at room temperature.

Gage No.	Check Point	Tolerance at Each Check Point
1	Every 20 pounds from 0-160 psi	±0.6 psi
2	Every 60 pounds from 0-600 psi	±2.25 psi
3	Every 500 pounds from 0-5,000 psi	±18.75 psi
4	Every 1,000 pounds from 0-10,000 psi	±75.00 psi

4.6.5 High temperature. The tester shall be placed within a test chamber capable of maintaining an internal temperature of +71° ±2°C for a period of 24 hours. At the end of the 24-hour period the temperature shall be changed to +55° ±2°C. At the end of an additional 2-hour period, with this temperature maintained, the tester shall be subjected to the tests specified in 4.6.3 with the exception of the test specified therein under c.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

4.6.5.1 The four master gages shall be placed within a test chamber capable of maintaining an internal temperature of +71° ±2°C for a period of 24 hours. At the end of the 24-hour period the temperature shall be changed to +55 ±2°C. At the end of an additional 2-hour period, with this temperature maintained, each gage shall be tested as specified under 4.6.4.1.

4.6.6 Humidity. This test shall be in accordance with MIL-STD-810, method 507.3, procedure I. Prior to the test, oil shall be drained from the reservoir and the tester and case shall be cleaned of oil film. The tester shall be contained in the case during the test period. The tester shall be examined 24 hours after the test to determine that no deterioration or corrosion of any internal or external components has occurred which would adversely affect subsequent operation. The tests specified in 4.6.3 shall be repeated.

4.7 Inspection of the preservation, packaging, packing and marking for shipment and storage. Sample items or packs and the inspection of the preservation, packaging packing and marking for shipment and storage shall be in accordance with the requirements of Section 5 or the documents specified therein.

* 5. PACKAGING

5.1 Preservation and packaging. Preservation and packaging shall be level A or C, as specified (see 6.2).

5.1.1 Level A. Unless otherwise specified in the contract or order, the testers shall be individually preserved and packaged in accordance with Method III of MIL-P-116. The tester within the case shall be overboxed in a unit container conforming to type CF, class Domestic, Variety SW, grade 275 of PPP-B-636.

5.1.2 Level C. The testers shall be individually preserved and packaged in a manner which will afford adequate protection against corrosion, deterioration and physical damage during shipment from supply source to the first receiving activity. This level may conform to the supplier's standard practice provided the latter meets the requirements of this level.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A. Each tester, preserved and packaged as specified in 5.1.1, shall be packed in overseas type shipping containers conforming to PPP-B-601, style A or B. Closure and strapping shall be in accordance with the appendix to PPP-B-601. Waterproofing shall be in accordance with MIL-STD-1186.

5.2.2 Level B. Each tester preserved and packaged as specified in 5.1.1 will not require overboxing. Unit containers will be shipping containers.

5.2.3 Level C. Packages that require overpacking for acceptance by the carrier shall be placed in exterior type shipping containers in a manner that will insure safe transportation at lowest rate to the point of delivery. Containers shall comply with Uniform Freight Classification Rules or Regulations of other carriers as applicable to the mode of transportation. This level may conform to the supplier's standard practice provided the latter meets the requirements of this level.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.

5.3 Physical protection. Cushioning, blocking and bracing shall be in accordance with MIL-STD-1186, except that for domestic shipments, waterproof ing requirements for cushioning materials and containers shall be waived. Drop tests of MIL-STD-1186 shall be waived when the item is preserved, packaged and packed for immediate use or when drop tests of MIL-P-116 are applicable.

5 4 Marking. Interior and exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The type MP-1 tester covered by this specification is intended for use in performing tests of aircraft pressure instruments on line and in the field.

6.2 Ordering data.

6.2.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number and date of this specification.

b. Accessories to be furnished, if different from 3.10.

c. Applicable levels of preservation, packaging, and packing required (see 5.1 and 5.2).

6.2.2 First article. (Page 52, MIL-STD-961C).

* 6.3 Subject term (key word) listing.

Gage, Pressure, Tester
Hydraulic Pressure Gage, Tester
Portable Pressure Gage, Tester
Pressure Gage Tester
Tester, Pressure Gage
Tester

6.4 Changes from previous issue. The margins of this specification are marked with asterisks to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodian:
Air Force - 99

Review activity:
DLA-GS

Preparing activity:
Air Force - 82

(Project No. 6685-F716

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T10:33Z
Check the source to verify that this is the current version before use.