INCH-POUND

A-A-54618
19 June 1992

COMMERCIAL ITEM DESCRIPTION

CURETTE, CHALAZION, MEYHOEFER

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-C-37017 which is cancelled.

This Commercial Item Description covers chalazion curettes suitable for use in surgical procedures on the human eyelid.

Salient characteristics:

General. The curettes shall be 5-1/4 inches in length, of the Meyhoefer design with a round cup shaped sharp edged blade, a straight rigid shank, and a hollow or solid handle. The curettes shall be of the following sizes and styles:

SIZE	DESCRIPTION
1	Medium
2	Small

Material. The curette shall be fabricated from class 4, martensitic corrosion-resistant steel in accordance with ASTM F899. As an alternate, the handle may be fabricated from class 3, austenitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The curette shall have a Rockwell Hardness (HRC) scale of 50 to 55 at the working edge when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Handles fabricated from class 3, austenitic corrosion-resistant steel shall have a Rockwell Hardness (HRB) scale of 75 to 90 when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The curette shall be in accordance with Figure 1 for style, design and dimensions.

Finish. The curette shall have a mirror or satin finish.

Passivation. The curette shall be properly passivated.

Corrosion resistance. The curette shall show no evidence of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM F1089.

Identification marking and labeling. The curette shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured curettes shall bear the name of the country of origin.

Workmanship. The curette shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One curette, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified herein. Unit of product for examination purposes shall be one curette. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one curette. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

NOTE: The following National Stock Numbers are covered by this document:

NSN	Item Identification	SIZE	STYLE
6515-00-321-9850	CURETTE, CHALAZION, Meyhoefer.	Medium	1
6515-00-321-9880	CURETTE, CHALAZION, Meyhoefer	Small	2

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T09:36Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB


Agent:

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS


Project No. 6515-5256

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

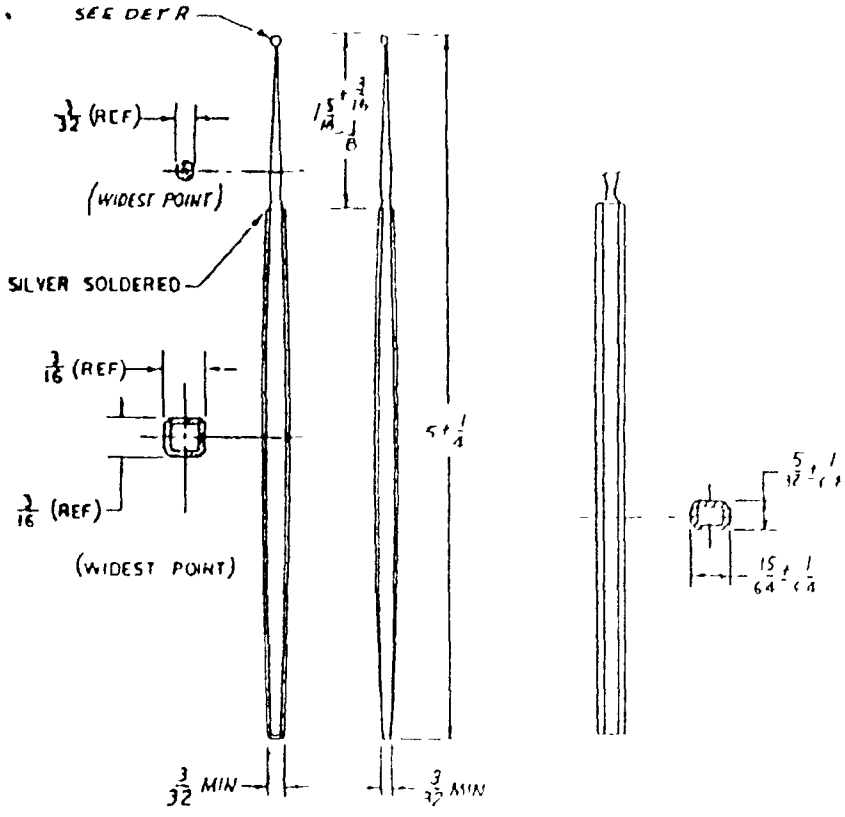

ALTERNATE DESIGN HANDLE

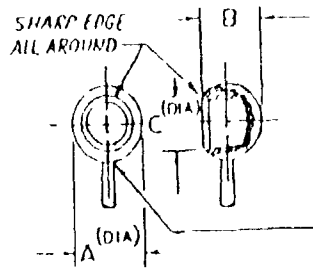

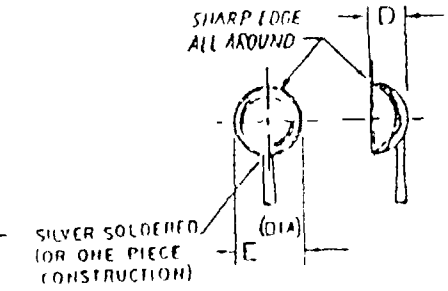

ALTERNATE DESIGN TIP

DETAIL R

NOTES:

1. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.
2. ALL DIMENSIONS ARE IN INCHES.
3. HANDLE NO HANDLE MAY BE SILVER SOLDERED IN ONE PIECE CONSTRUCTION.
4. HANDLE MAY BE HOLLOW OR SOLID.

DIMENSIONS

STOCK NO	SIZE	A(±.005)	B(±.1/64)	C(±.005)	D(±1/64)	E(±.005)
6515-00-321-9880 (SMALL)	2	.080	5/64	.070	3/64	.085
6515-00-321-9850 (MEDIUM)	1	.105	7/64	.095	3/64	.100

FIGURE 1. CURETTE, CHALAZION, MEIBOMIAN

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revisio letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification o requirements on current contracts Comments submitted on this form do not constitute or imply authorization t waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-54618	19 June 1992

3 DOCUMENT TITLE CURETTE, CHALAZION, MEYHOEFER

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: MSE	b TELEPHONE (Include Area Code) (1) Commercial (215)737-2870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) 2800 S. 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:36Z
Check the source to verify that this is the current version before use.