INCH-POUND

A-A-54624
17 April 1992

COMMERCIAL ITEM DESCRIPTION

Lamp, Incandescent

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a 100 watt quartz, tungsten halogen incandescent lamp suitable for use as the visible light source in a visible light dental curing system (see notes).

Salient characteristics:

The lamp shall be an incandescent quartz, tungsten halogen type. The lamp's reflector shall be a silicon dioxide coated mirror which is ellipsoidal in shape. The reflector shall be a white, cold light reflector which provides maximum reflection of white light in the 400 nm to 700 nm wavelength range. Style, design and dimensions of the lamp shall be in accordance with Figure 1.

The lamp shall be suitable for use in and dimensionally compatible with the visible light dental curing system (see notes).

The lamp shall have a focal length of 26mm and a minimum light output of 600 mW/cm^2.

The lamp shall require an input of 12 VAC. The lamp shall have a minimum power rating of 100 watts. The lamp shall meet all applicable requirements of United Laboratories (UL) 544. The average lamp life shall be rated at a minimum of 50 statistical hours at rated voltage (12 volts, nominal), or a minimum of 10,000 curing cycles at rated voltage (12 volts, nominal). One curing cycle shall be defined as the lamp being on for 18 consecutive seconds. Each curing cycle shall be followed by 18 consecutive seconds with the lamp off to allow cooling time between cycles.

Workmanship. The lamps shall be free from defects which may detract from their appearance or impair their serviceability.

AMSC N/A FSC 6240

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One lamp, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, at inspection level II, except dimensions shall be examined at inspection level S-2. The unit of product for examination purposes shall be one lamp, as specified.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, at Inspection Level S-2, and an acceptable number of zero for all sample sizes.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

order.

NOTE: The following National Stock Number is covered by this document.

National Stock Number	Item Identification
6240-01-315-3676	Lamp, Incandescent

NOTE 1: The following National Stock Number is referenced by this document.

National Stock Number	Item Identification
6520-01-296-5760	Curing System, Dental, Visible Light

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6240-1307
Location: DC Disk# 1
(LAMP)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

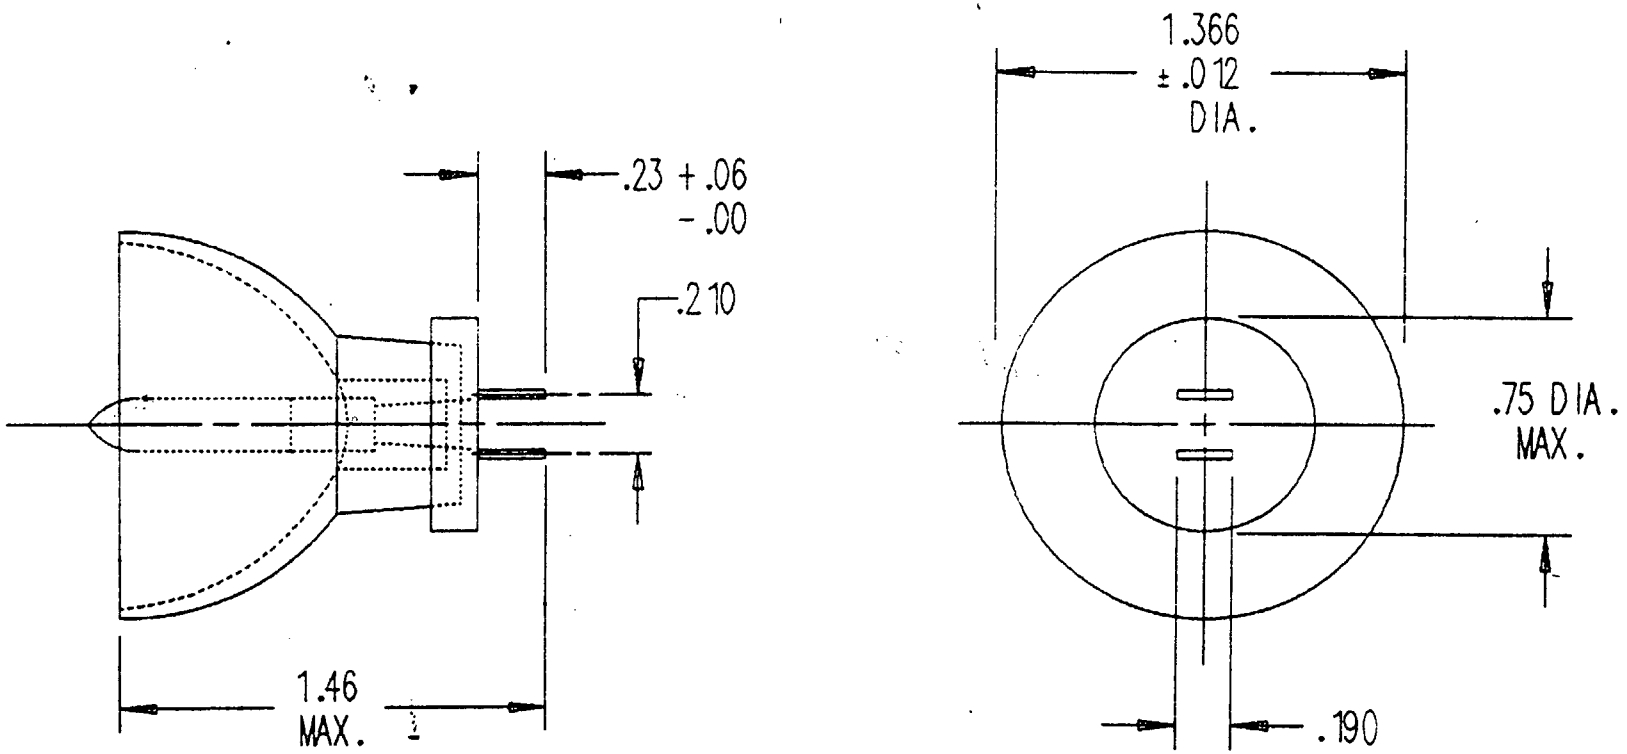

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES. TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
	± .005	

NSN 6240-01-315-3676

FIGURE 1 LAMP, INCANDESCENT

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER A-A-54624	2. DOCUMENT DATE (YYMMDD) 92-04-17

3. DOCUMENT TITLE
Lamp, Incandescent

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center	(215)737-2870	444-2870
c. ADDRESS (Include Zip Code) ATTN: DPSC-MSE 2800 S. 20th Street Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete — 90/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.