INCH-POUND

A-A-54633
30 May 1992

COMMERCIAL ITEM DESCRIPTION

CATHETERIZATION SET, CARDIOVASCULAR

The General Services Administrations has authorized the use of this commercial item description.

This commercial item description covers a 7 Fr, disposable, Multi-lumen, sterile cardiovascular catheterization set for use in placement of an in-dwelling central venous line.

Salient Characteristics:

General. The disposable cardiovascular catheterization set shall be a complete set of items required for placement of an in-dwelling central venous line.

Characteristics. The set shall consist of, as a minimum, the following disposable components:

Components	Qty
Catheter, radiopaque, multi-lumen, polyurethane central venous, 7 Fr by 12 inch, 16, 18, and 18 gauge lumen	1
Catheter, radiopaque, 16 gauge by 2-1/2, heavy wall fluorinated ethylene propylene over 20 gauge introducer needle	1
Caps, Luer lock injection	3
Clamp, catheter	1
Clamps, extension line	3
Dilator, vessel	1
Needle, 18 gauge by 2-1/2 inch	1

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Components	Qty
Spring wire guide, 0.035 inch diameter 26 inch long, straight soft tip on one end, and "J" curved tip on the other end.	1
Syringe, 5 ml	1

Material. The multi-lumen catheter shall be fabricated from pliant polyurethane plastic which meets the requirements of the USP for Class IV plastics (See Note 1). The heavy wall catheter shall be fabricated from fluorinated ethylene propylene (FEP) which meets the requirements of the USP for Class IV plastics (See Note 1).

The needles and spring wire guide shall be fabricated from type 304 stainless steel in accordance with ASTM Designation F899.

Construction.

Multi lumen catheter. Multi-lumen catheter shall consist of a radiopaque catheter attached to a junction providing access to three extension lines. Extension lines shall each have a clamp and shall attach to a Luer lock fitting which shall be attached to a detachable Luer lock injection cap. Junction shall have perforated wings for securing to patient. The multi-lumen catheter shall be fabricated as shown in Figure 1.

Catheter 16 gauge needle and syringe. The 16 gauge catheter needle and syringe shall be constructed and provided assembled as shown in Figure 2.

Spring wire guide. The spring wire guide shall be as previously described and shall be enclosed in a protective plastic sheath. A 2-1/4 inch long rigid plastic sheath shall be provided at the "J" end to allow "J" end to be straightened .

The spring wire guide shall have a safe, sliding fit with the multilumen catheter.

Vessel dilator. The vessel dilator shall be 4-3/4 inches long, tapered at one end with a Luer lock fitting at the other end.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Catheter clamp. The catheter clamp shall consist of two parts to encase the catheter and shall have perforated wings to allow the clamp to be sutured to the patient.

Luer fittings. Luer fittings shall be in accordance with ANSI/HIMA MD70.1.

Radiopacity. The catheter shall be radiopaque in accordance with ASTM Designation F640.

Catheter flexibility. The multi-lumen catheter shall be wrapped around a 1/2 inch diameter rod without kinking or cracking. Water shall be passed through each extension. Luer fitting shall show no restriction to flow through the lumen and distal tip.

Catheter security of assembly. The catheter shall not tear or separate from the extension junction when subjected to tensile force of 2.0 pounds.

Catheter leakage. With the distal tip openings of the multi-lumen of the catheter sealed, 20 psig water shall be admitted through one of the injection caps. The other caps shall be securely attached. No leakage shall be observed when tested for 2 minutes.

Heavy metals extractability. Components coming in contact with intravenous solution or patients blood shall be tested for heavy metals extractability. The quantity of lead and cadmium shall not exceed 5 parts per million (PPM) and the amount of barium shall not exceed 10 ppm when tested in accordance with the USP (See Note 2).

Toxicity, pyrogencity, sterility. The catheters shall be nontoxic and nonpyrogenic in accordance with the USP for Transfusion and Infusion assemblies (the rabbit pyrogen test) or the Bacterial Endotoxins Test (LAL) with the rabbit pyrogen test used for LAL test failure. The set components and internal surface of the package shall be sterile with a Sterility Assurance Level of .000001 in accordance with AAMI guidelines. (See Note 3)

Sterility lot and traceability. A sterility lot is that quantity of product sterilized in the same sterilizing chamber at the same time. Each quantity of product shall be traceable to a given manufacturing operation or lot. Each unit package shall be traceable to a given sterility or acceptable manufacturing lot.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Workmanship. The catheterization set shall be free from defects which detract from its appearance on impair its serviceability. Components shall be free from flash, sharp edges, (other than needle points), distortion or foreign material.

Unit. Package (PG). One package containing 5 individually packaged catheter sets, as specified, constitutes one unit. The individual package shall be a sealed peel-open type container capable of maintaining sterility of contents unless package is damaged or opened.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be catheterization set. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be catheterization set. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE 1:

The following is acceptable as an alternate to USP Class IV plastics lot testing: The catheter shall be initially qualified for Class IV plastics in accordance with the USP, and simultaneously, tested for tissue culture cytotoxicity in accordance with HIMA "Guideline For Evaluating The Safety of Materials Used in Medical Devices". Subsequent production lots which show greater toxicity than the initial qualification lot shall be subjected to USP Class IV biological testing. In the event of a change in material formulation, USP Class IV initial qualification testing shall again be required.

NOTE 2:

Certificates of heavy metals testing. A certificate of compliance, stipulating that offered items meet the heavy metals extractable testing shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years and that there have been no changes to material, formulation and method of processing since prior test was performed.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:36Z
Check the source to verify that this is the currentversion before use.

NOTE 3:

In lieu of having each material batch represented in the finished goods toxicity and pyrogenicity test samples, the following shall be acceptable as an alternate: New raw materials shall be initially qualified through toxicity and pyrogenicity testing. Subsequent incoming materials will be tested physically for material consistency. Any changes to material or processing shall require material to be requalification tested.

NOTE 4:

The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-177-3716	CATHETERIZATION SET, CARDIOVASCULAR, Multi-Lumen, 7 Fr, Disposable, 5s

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5361
Location: CATHET/S11

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.


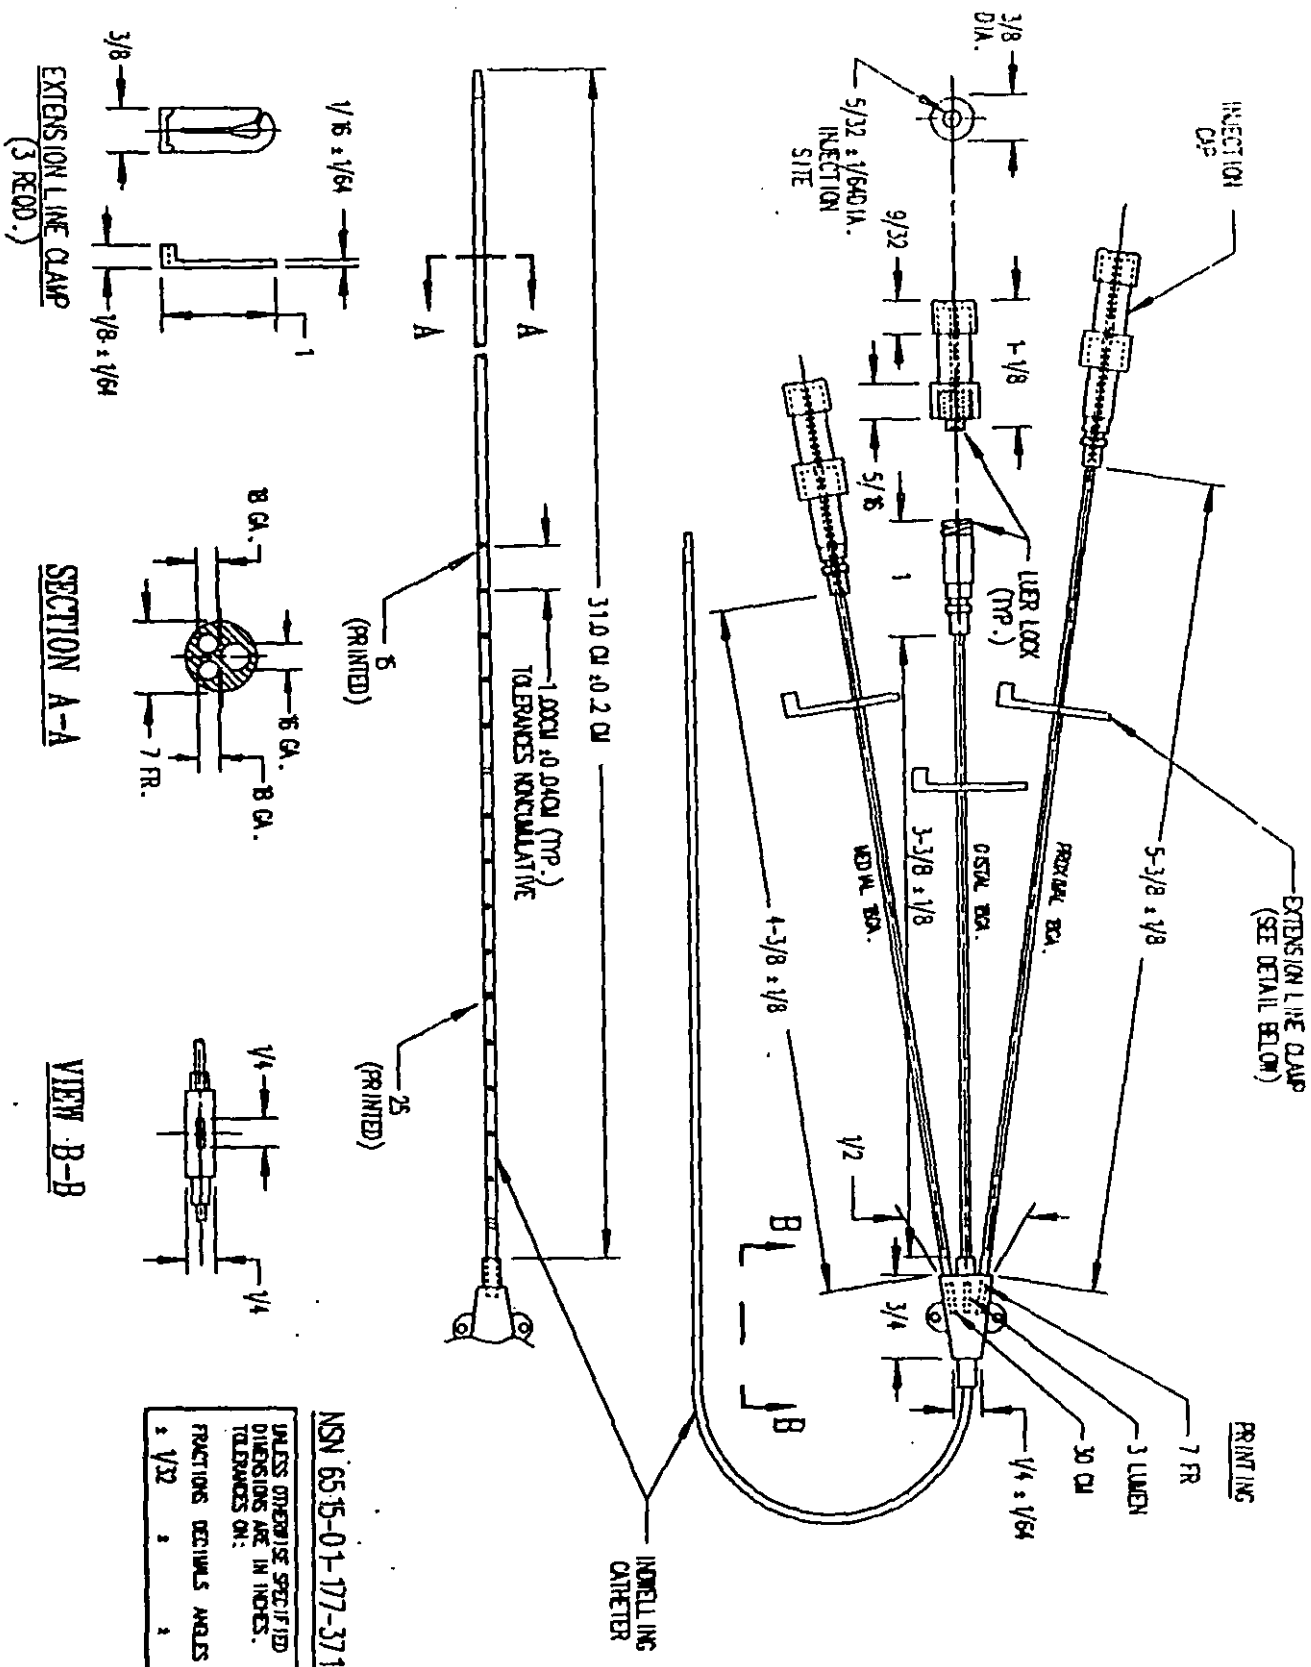


FIGURE 1 CATHERIZATION SET, VENOUS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

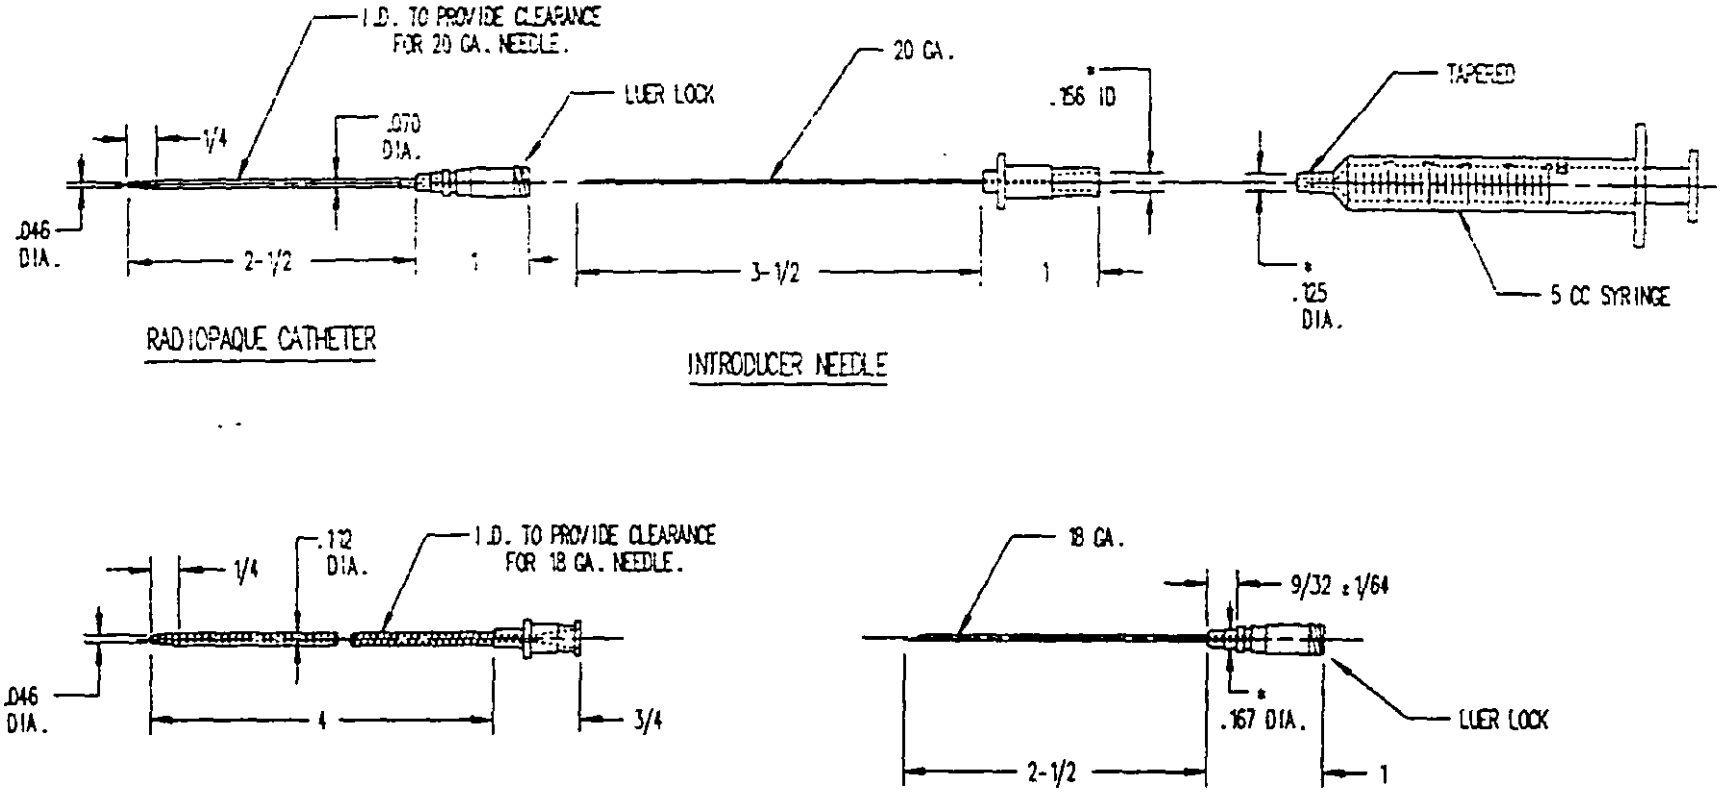

NOTES:

1. DIMENSIONS MARKED WITH "*" ARE FOR TOOLING PURPOSES ONLY. PRECISE SIZES SHALL BE DETERMINED BY FABRICATOR TO OBTAIN PROPER FUNCTIONING WITH MATING PARTS.

NSN 6515-01-177-3716

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES. TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
± 1/32	± .005	±

FIGURE 2 CATHERIZATION SET, VENOUS

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54633	30 May 1992

3. DOCUMENT TITLE

CATHETERIZATION SET, CARDIOVASCULAR

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	215-737-2870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 *Previous editions are obsolete.* 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.