INCH-POUND

A-A-54652
30 May 1992

COMMERCIAL ITEM DESCRIPTION

CATHETER, URETHRAL, X-ray, Whistle Tip

The General Services Administrations has authorized the use of this commercial item description.

This commercial item description covers one type of urethral catheter. This type shall consist of a pair of sterile, disposable, radiopaque, whistle tip urethral catheters for use in urological procedures.

Salient Characteristics.

General. The pair of urethral catheters shall be sterile, disposable, radiopaque, three-eyed and whistle tip with the left side catheter being color coded green and the right side catheter being red. (Right side, as an alternate, shall be blue coded.) The catheter pairs shall be provided in French size 5 or French size 6 as shown under notes.

Style, design and dimensions. The catheter shall be in accordance with Figure 1. Outside diameter of the body shall correspond to French size shown on the Figure. The catheter shall pass freely through the cystoscape opening of the size designated but not through the next smaller French size opening.

Material. The catheters shall be fabricated of nylon, polyethylene or polyurethane with a smooth exterior surface to facilitate the ease of insertion. The catheter shall have the rigidity required to withstand pressure of introduction through the cystoscope and into the ureter, together with the softness and pliability to prevent irritation of body tissues.

Identification marking and labeling. The catheter shall be permanently marked with the manufacturer's name or registered trademark. Foreign manufactured tubes shall bear the name of the country of origin.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Radiopacity. The catheter circumferential markings shall be radiopaque when tested in accordance with Method C of ASTM Designation F640.

Sterility. The catheters shall be sterile in accordance with the United States Pharmacopia (USP) for Sterile Devices. As an alternate, AAMI Guidelines for Biological Indicators, Sterilization Methods, Sterilization Validation, and Sterility Testing shall be as followed. Sterility assurance level shall be 0.000001.

Safety and toxicity. The catheter shall be safe and nontoxic when tested in accordance with USP requirements.

Pyrogenicity. The catheter shall be free from pyrogens when tested in accordance with the USP.

Biocompatibility. The catheter shall meet Type IV plastic biological requirements when tested in accordance with the USP.

Certificate of biocompatibility. A certificate of compliance, stipulating that offered items meet the requirements specified herein, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years, and that have been no changes to material, formulation and method of processing since actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and NSN, a statement certifying that material, processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person marking the certification.

Workmanship. The catheters shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing 12 pairs of catheters of one French size only, as specified, constitutes one unit. Each pair (one individually wrapped left catheter and one individually wrapped right catheter) shall be packaged, uncoiled, in a suitable peel open container capable of maintaining sterility of contents unless package is damaged or opened.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for test shall be conducting in accordance with MIL-STD-105. Inspection shall be conducted at Inspection level II and AQL (Acceptable Quality Level) of 1.0 percent. The unit of product for test purposes shall be one tube.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers and their Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATIONS
6515-01-174-2345	CATHETER, URETHRAL, X-Ray, Whistle Tip, Disposable, 5 Fr, 12 Pair
6515-01-174-2346	CATHETER, URETHRAL, X-Ray, Whistle Tip, Disposable, 6 Fr, 12 Pair

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5175
Location: \word\nish\catheter

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

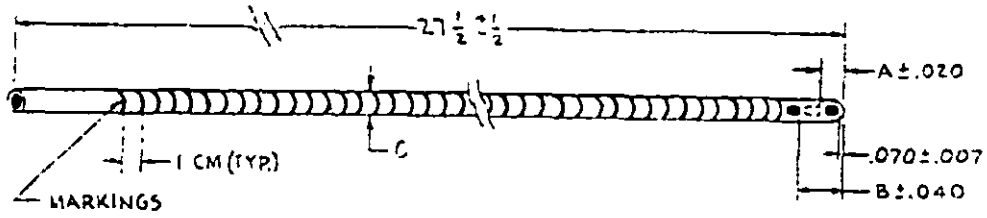

NSN	A	B	C
6515-01-174-2345	.195	.407	5FR
6515-01-174-2346	.200	.415	6FR
ALTERNATE 6515-01-174-2345	.294	.517	5FR
6515-01-174-2346	.294	.517	6FR

NOTE:
X-RAY OPAQUE

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES

FIGURE 1 CATHETER, URETHRAL, WHISTLE TIP, DISPOSABLE

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54652	30 May 1992

3. DOCUMENT TITLE
CATHETER, URETHRAL, X-ray, Whistle Tip

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial 215-737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-02-26T09:36Z
Check the source to verify that this is the current version before use.