INCH-POUND

A-A-54671
15 June 1992

COMMERCIAL ITEM DESCRIPTION

INHALER, MEDICAMENT, PLASTIC

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-I-37200A which is cancelled.

This commercial item description covers a Chromolyn Sodium Inhaler device suitable for use with Chromolyn Sodium capsules, 20 mg per capsule, in the treatment of respiratory problems.

Salient characteristics:

General. The inhaler shall consist of a body with a sliding sleeve, a capsule piercing device, a mouthpiece and permanently affixed spindle and a propeller. The sliding sleeve on the body shall cause the capsule to be pierced when operated in accordance with the instructions. The propeller shall securely accommodate the capsules and all components shall be securely assembled. A circular flange shall be provided at the base of the mouthpiece.

Material. The washers shall be fabricated of aluminum suitably anodized. Corrosion resistant steel of the inhaler shall be in accordance with ASTM Designation F899. Plastic components of the inhaler shall be fabricated of 11 amino-undecanoic acid (nylon 11).

Style, design and dimensions. The inhaler device shall be in accordance with Figure 1 design and dimensions.

Corrosion resistance. Corrosion resistant steel shall show no evidence of corrosion or plating of copper when tested in accordance with ASTM Designation F1089.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Inhalation test. The volume of air aspirated through the mouthpiece of the loaded inhaler (containing one capsule of Chromolyn Sodium) shall be at the rate of 60 liters/minute, 1-1/2 seconds duration, and repeated 4 times within 10 seconds. The capsule shall have an average weight loss of 90 percent, minimum and no more than 5 percent of the samples tested shall have less than 75 percent of their weight expelled.

Instructions for use. Each inhaler shall be provided with an instruction sheet containing illustrations and instructions for proper use of the inhaler. The instructions shall state that the capsule shall be pierced only once.

Identification marking and labeling. The inhaler shall be legibly marked with the contractor's name or trademark and the word "stainless".

Workmanship. The inhaler shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One inhaler, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one inhaler as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one inhaler. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-133-5426	INHALER, MEDICAMENT, PLASTIC

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MS

Agent:

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5417
Location: c:\word\nish\inhalecd

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

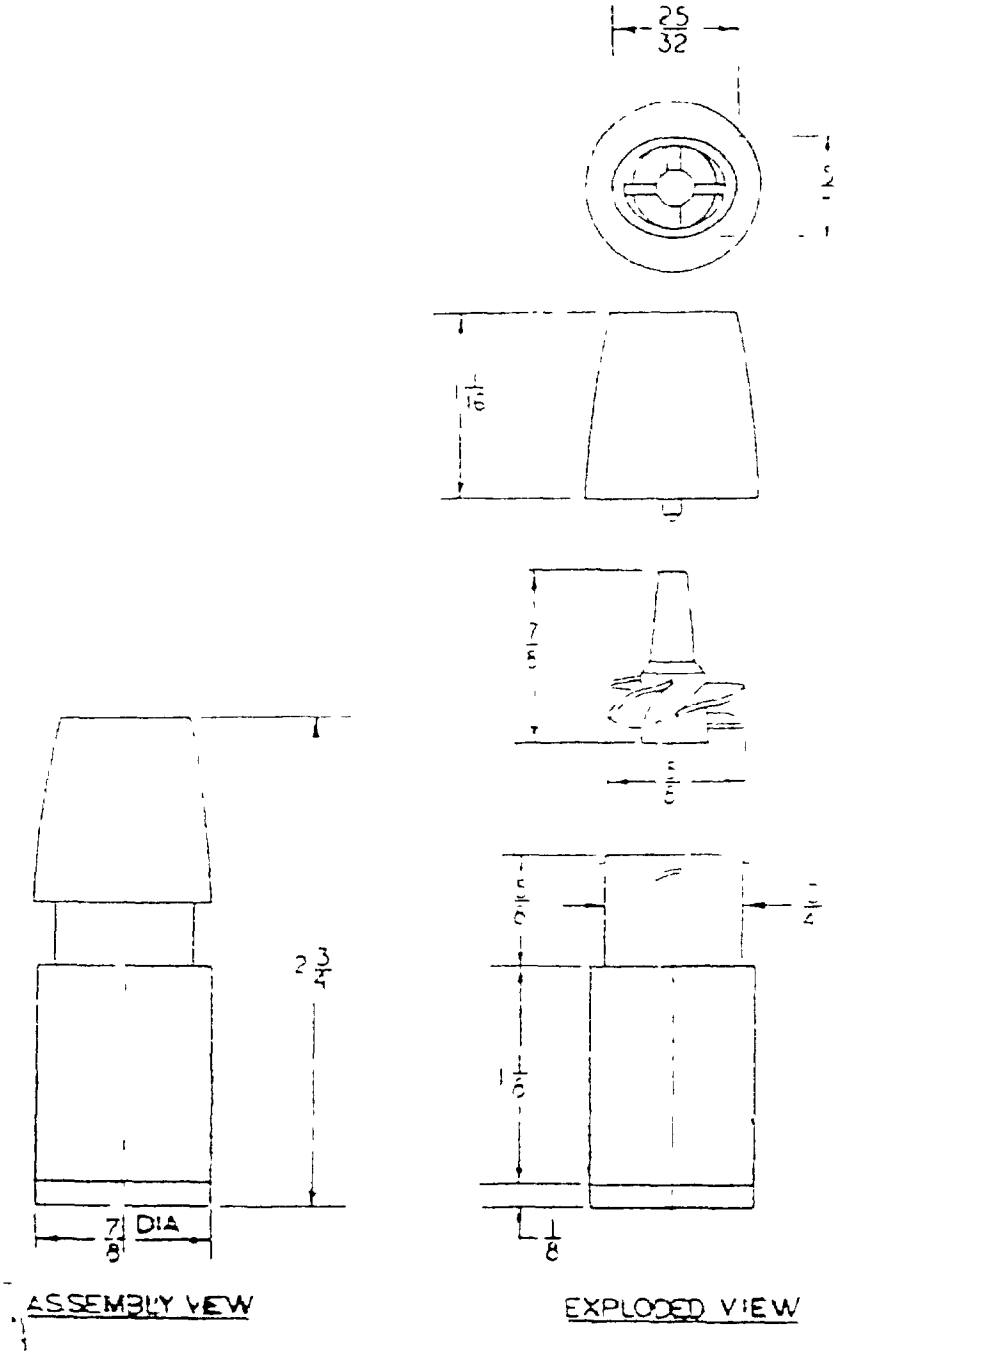

DIMENSIONS ARE IN INCHES AND ARE REFERENCE DIMENSIONS ONLY

INHALER, MEDICAMENT
FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:37Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3 and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54671	2 DOCUMENT DATE (YYMMDD) 15 June 1992

3 DOCUMENT TITLE
INHALER, MEDICAMENT, PLASTIC

4 NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)*

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	e DATE SUBMITTED (YYMMDD)

7 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	215-737-2870	444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 2026-04-26T09:37Z
Check the source to verify that this is the current version before use.