INCH-POUND
A-A-50060B
17 July 2001
SUPERSEDING
A-A-50060A
26 October 1992

COMMERCIAL ITEM DESCRIPTION

BALANCES, TRIP, LABORATORY

The General Services Administration has authorized the use of this commercial item description for all federal agencies.

1. SCOPE. This commercial item description (CID) establishes the government acquisition requirements for laboratory trip balances to be used as accurate weighing instruments in laboratories and pharmacies.

2. CLASSIFICATION. The balances shall be classified and identified by the types listed below. The selected type to be supplied shall be specified in the acquisition order (see 7.5(b)).

Type I Single beam, dual scale, metric and avoirdupois (avdp), capacity of 200 grams/5.1 pounds

Type II Double beam, metric, capacity of 2000 grams

3. SALIENT CHARACTERISTICS

3.1 Components. The balances shall be of the beam type with a base and the following components.

3.1.1 Weight beams. Each balance shall contain one or more weight beams.

3.1.2 Weighing surfaces. The weighing surfaces shall be approximately six-inch diameter stainless steel plates, polished or brushed flat, and free of obstructions. The platforms shall be readily interchangeable without the necessity of replacing any other part.

3.1.3 Knife edge. The knife edges shall be made of hardened steel and accurately ground.

3.1.4 Bearings. The bearings shall be made of agate. The bearing blocks shall be self-aligning to ensure continuous contact along the knife edges.

Beneficial comments, recommendations, additions, deletions, clarifications, etc. and any data that may improve this document should be sent to: Defense Supply Center Richmond (DSCR), ATTN: DSCR-VBD, 8000 Jefferson Davis Highway, Richmond, VA 23297-5610.

AMSC N/A FSC 6670

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:38Z
Check the source to verify that this is the current version before use.

3.1.5 Poises. The poises shall be of the center-reading sliding type.

3.1.6 Pointer. The pointer shall be easy to read.

3.1.7 Dust cover. Each balance shall be supplied with a dust cover of sufficient size to completely cover it.

3.1.8 Damping. The damping system shall be friction free and self adjusting.

3.1.9 Instructions. Each balance shall be furnished with two copies of instructions for installation, operation, and maintenance, as well as a list of component parts.

3.2 Sensitivity and beam graduations.

3.2.1 Type I. Type I balances shall have a zero load sensitivity of 0.1 gram/0.0035 ounce (avdp) per graduation, and a full load sensitivity of 0.2 gram/0.0070 ounce (avdp) per graduation, and a capacity of 2000 grams/5.1 pounds. The beam shall be graduated in 0.2 gram and 0.1 ounce divisions.

3.2.2 Type II. Type II balances shall have a full load sensitivity of 0.2 gram and a capacity of 2000 grams. The upper beam shall be graduated from 0 to 10 grams in 0.1-gram divisions while the lower beam shall be graduated from 0 to 200 grams in 10-gram divisions.

3.3 Nameplate. A permanent nameplate shall be attached to the product. Unless otherwise specified in the acquisition order (see 7.5 (c)), the nameplate shall display the following information:

a. Nomenclature
b. Manufacturer's name
c. Manufacturer's model designation
d. Balance type (see 2)
e. National stock number (if specified)
f. Contract or order number (if specified)
g. Date of manufacture (if specified)

4. REGULATORY REQUIREMENTS

4.1 Recovered materials. The offeror/contractor is encouraged to use recovered materials to the maximum extent practicable, in accordance with paragraph 23.403 of the Federal Acquisition Regulation (FAR).

5. PRODUCT CONFORMANCE PROVISIONS

5.1 Product conformance. The products provided shall meet the salient characteristics of this commercial item description, conform to the producer's own drawings, specifications, standards, and quality assurance practices, and be the same product offered for sale in the commercial marketplace. The government reserves the right to require proof of such conformance.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:38Z
Check the source to verify that this is the current version before use.

5.2 Market acceptability. The product offered must have been previously sold either to the government or on the commercial market.

6. PACKAGING

6.1 Preservation, packing, and marking. For acquisition purposes, the products shall be preserved, packed, and marked as specified in the acquisition order (see 7.5(d)).

6.2 Overseas packaging. Movable components of the balance shall be secured in a manner that will prevent movement or damage during shipment and storage. The balances shall be packed in a fiberboard box conforming to ASTM D 5118/D 5118M, "Standard Practice for Fabrication of Fiberboard Shipping Boxes" (DoD adopted). The box shall be closed, waterproofed, and reinforced in accordance with ASTM D 1974, "Methods of Closing, Sealing, and Reinforcing Fiberboard Boxes" (DoD adopted).

6.3 Overseas marking. Marking shall be in accordance with MIL-STD-129, "Standard Practice for Military Marking", or FED-STD-123, "Marking for Shipment (Civil Agencies)", as applicable.

6.4 Domestic packaging, packing, palletization, and marking. Packaging, packing, palletization, and marking shall be in accordance with ASTM D 3951,"Standard Practice for Commercial Packaging"(DoD adopted).

7. NOTES

7.1 Part or identification number (PIN). The following part or identification numbering procedure is for government purposes and does not constitute a requirement for the contractor.

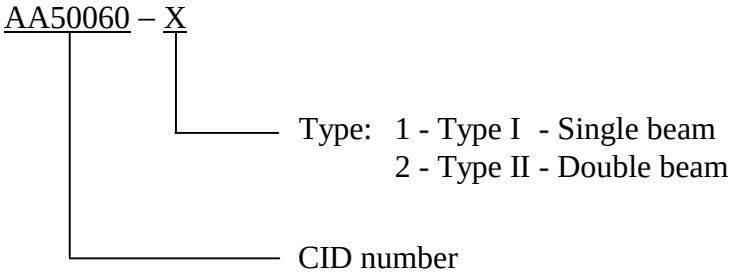

7.2 Sources of documents.

7.2.1 Government documents. Copies of FAR, military specifications and federal standards may be obtained from the U.S. Government Printing Office, Superintendent of Documents, Mail Stop: SSOP, Washington, DC 20402-9328. Electronic copies of CFR documents may be obtained from http://www.access.gpo.gov. Electronic copies of military specifications and federal standards may be obtained from http://astimage.daps.dla.mil/quicksearch/.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:38Z
Check the source to verify that this is the current version before use.

7.2.2 ASTM standards. Copies of ASTM standards may be obtained from the American Society for Testing and Materials, 100 Barr Harbor Drive, West Conshohocken, PA 19428-2959.

7.3 National stock number (NSN). The following is a list of NSNs that correspond to this CID. The list may not be indicative of all possible NSNs associated with this CID.

NSN	Type
6670-00-401-7195	II
6670-00-436-9857	II
6670-00-955-6486	II

7.4 Sources of supply. The manufacturers and/or suppliers listed below are known to supply products that meet the salient characteristics requirements of this document. Competition is not limited to the listed firms.

A. Daigger & Company
Vernon Hills, Il 60061

Alliance Scale Inc.
Canton, MA 02021-0509

Ohaus Corporation
Pine Brook, NJ 07058

Phillips Morris Scale Company
Seattle, WA 98119

Rice Lake Weighing Systems
Rice Lake, WI 54868

Totalcomp, Inc.
Fair Lawn, NJ 07410

7.5 Ordering data. Acquisition documents must specify the following information:

a. CID document number, revision, and CID PIN
b. Balance type (see 2)
c. Nameplate, if different (see 3.3)
d. Preservation, packing, and marking requirements (see 6)

7.6 Subject term (key word) listing.

beam
poise
scale
weight

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:38Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:
Army - GL
Navy - MS
Air Force - 03

Reviewers:
Army - MD
Navy - YD
Air Force - 71, 99

CIVIL AGENCY
COORDINATING ACTIVITY:

GSA - 7FXE

Preparing activity:
DLA - GS1

(Project 6670-0212)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:38Z
Check the source to verify that this is the current version before use.