A-A-54388
12 May 1991

COMMERCIAL ITEM DESCRIPTION

TUBE, TRACHEOSTOMY, DOUBLE CUFF

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers one type of a sterile disposable double cuffed tracheostomy tube suitable for long term ventilation of tracheostomy patients needing alternating cuff sites.

Salient Characteristics:

General. The tube shall be a single use, self-contained, sterile, disposable curved tracheostomy tube with winged neck flange, integral connector, two high volume/low pressure cuffs, 2 one-way inflation valves, inflation lines, inflation indicator, a spacing wedge and a 48 inch cotton tie.

Material. The tube shall be made of a polyvinyl chloride.

Style, design and dimensions. The tube shall be size 6 tracheostomy tube having a 7.0 mm I.D., 9.7 mm O.D. and 83 mm long. The tube shall have a radiopaque stripe over the entire length and shall have two thin walled high volume/low pressure cuffs. Each cuff shall have a pressure relief valve that limits cuff pressure to approximately 25 mm Hg. The tube shall have an integral 15 mm connector. The tube shall have a winged flange that conforms to neck anatomy to help minimize motion and trauma. The tube shall have the size clearly imprinted on the neck flange. The tube shall be in accordance with Figure 1.

Directions. Each package of tubes shall include a "Direction for Use" pamphlet.

Identification marking and labeling. The tube shall be permanently marked with the contractor's name or registered trademark. Foreign manufactured tubes shall bear the name of the country of origin.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Sterility. The tube shall be sterile in accordance with the United States Pharmacopeia (USP) for Sterile Devices. As an alternate, AAMI Guidelines for Biological Indicators, Sterilization Methods, Sterilization Validation, and Sterility Testing shall be as followed. Sterility assurance level shall be 0.000001.

Pyrogenicity. The tube shall be free from pyrogens when tested in accordance with the USP.

Biocompatibility. The tube shall be free from pyrogens when tested in accordance with the USP.

Certificate of biocompatibility. A certificate of compliance stipulating offered items meet the requirements specified herein, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years, and that there has been no changes to material, formulation and method of processing since the actual testing was performed. The certificate shall include the date the testing was performed, the test method and results, the name and title of the person evaluating the results, the current contract number and NSN, a statement certifying that material, processing and formulation have not changed since the time that biocompatibility was performed and the signature and title of the person making the certification.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. Shall be examined to verify that the design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements as specified.

Workmanship. The tube shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One individually packaged sterile tube, as specified, constitutes one unit. The individual package shall be a sealed peel-open container capable of maintaining sterility of contents unless package is damaged or opened

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more text characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. Inspection shall be conducted at Inspection level II and an AQL (Acceptable Quality Level) of 1.0 percent. The unit of product for test purposes shall be one tube.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers'own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the products is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM DESCRIPTION
6515-01-299-5658	TUBE, TRACHEOSTOMY, DISPOSABLE, DOUBLE CUFF, 7mm I.D., 83 mm long, 30 FR, Size 6, Each

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4949

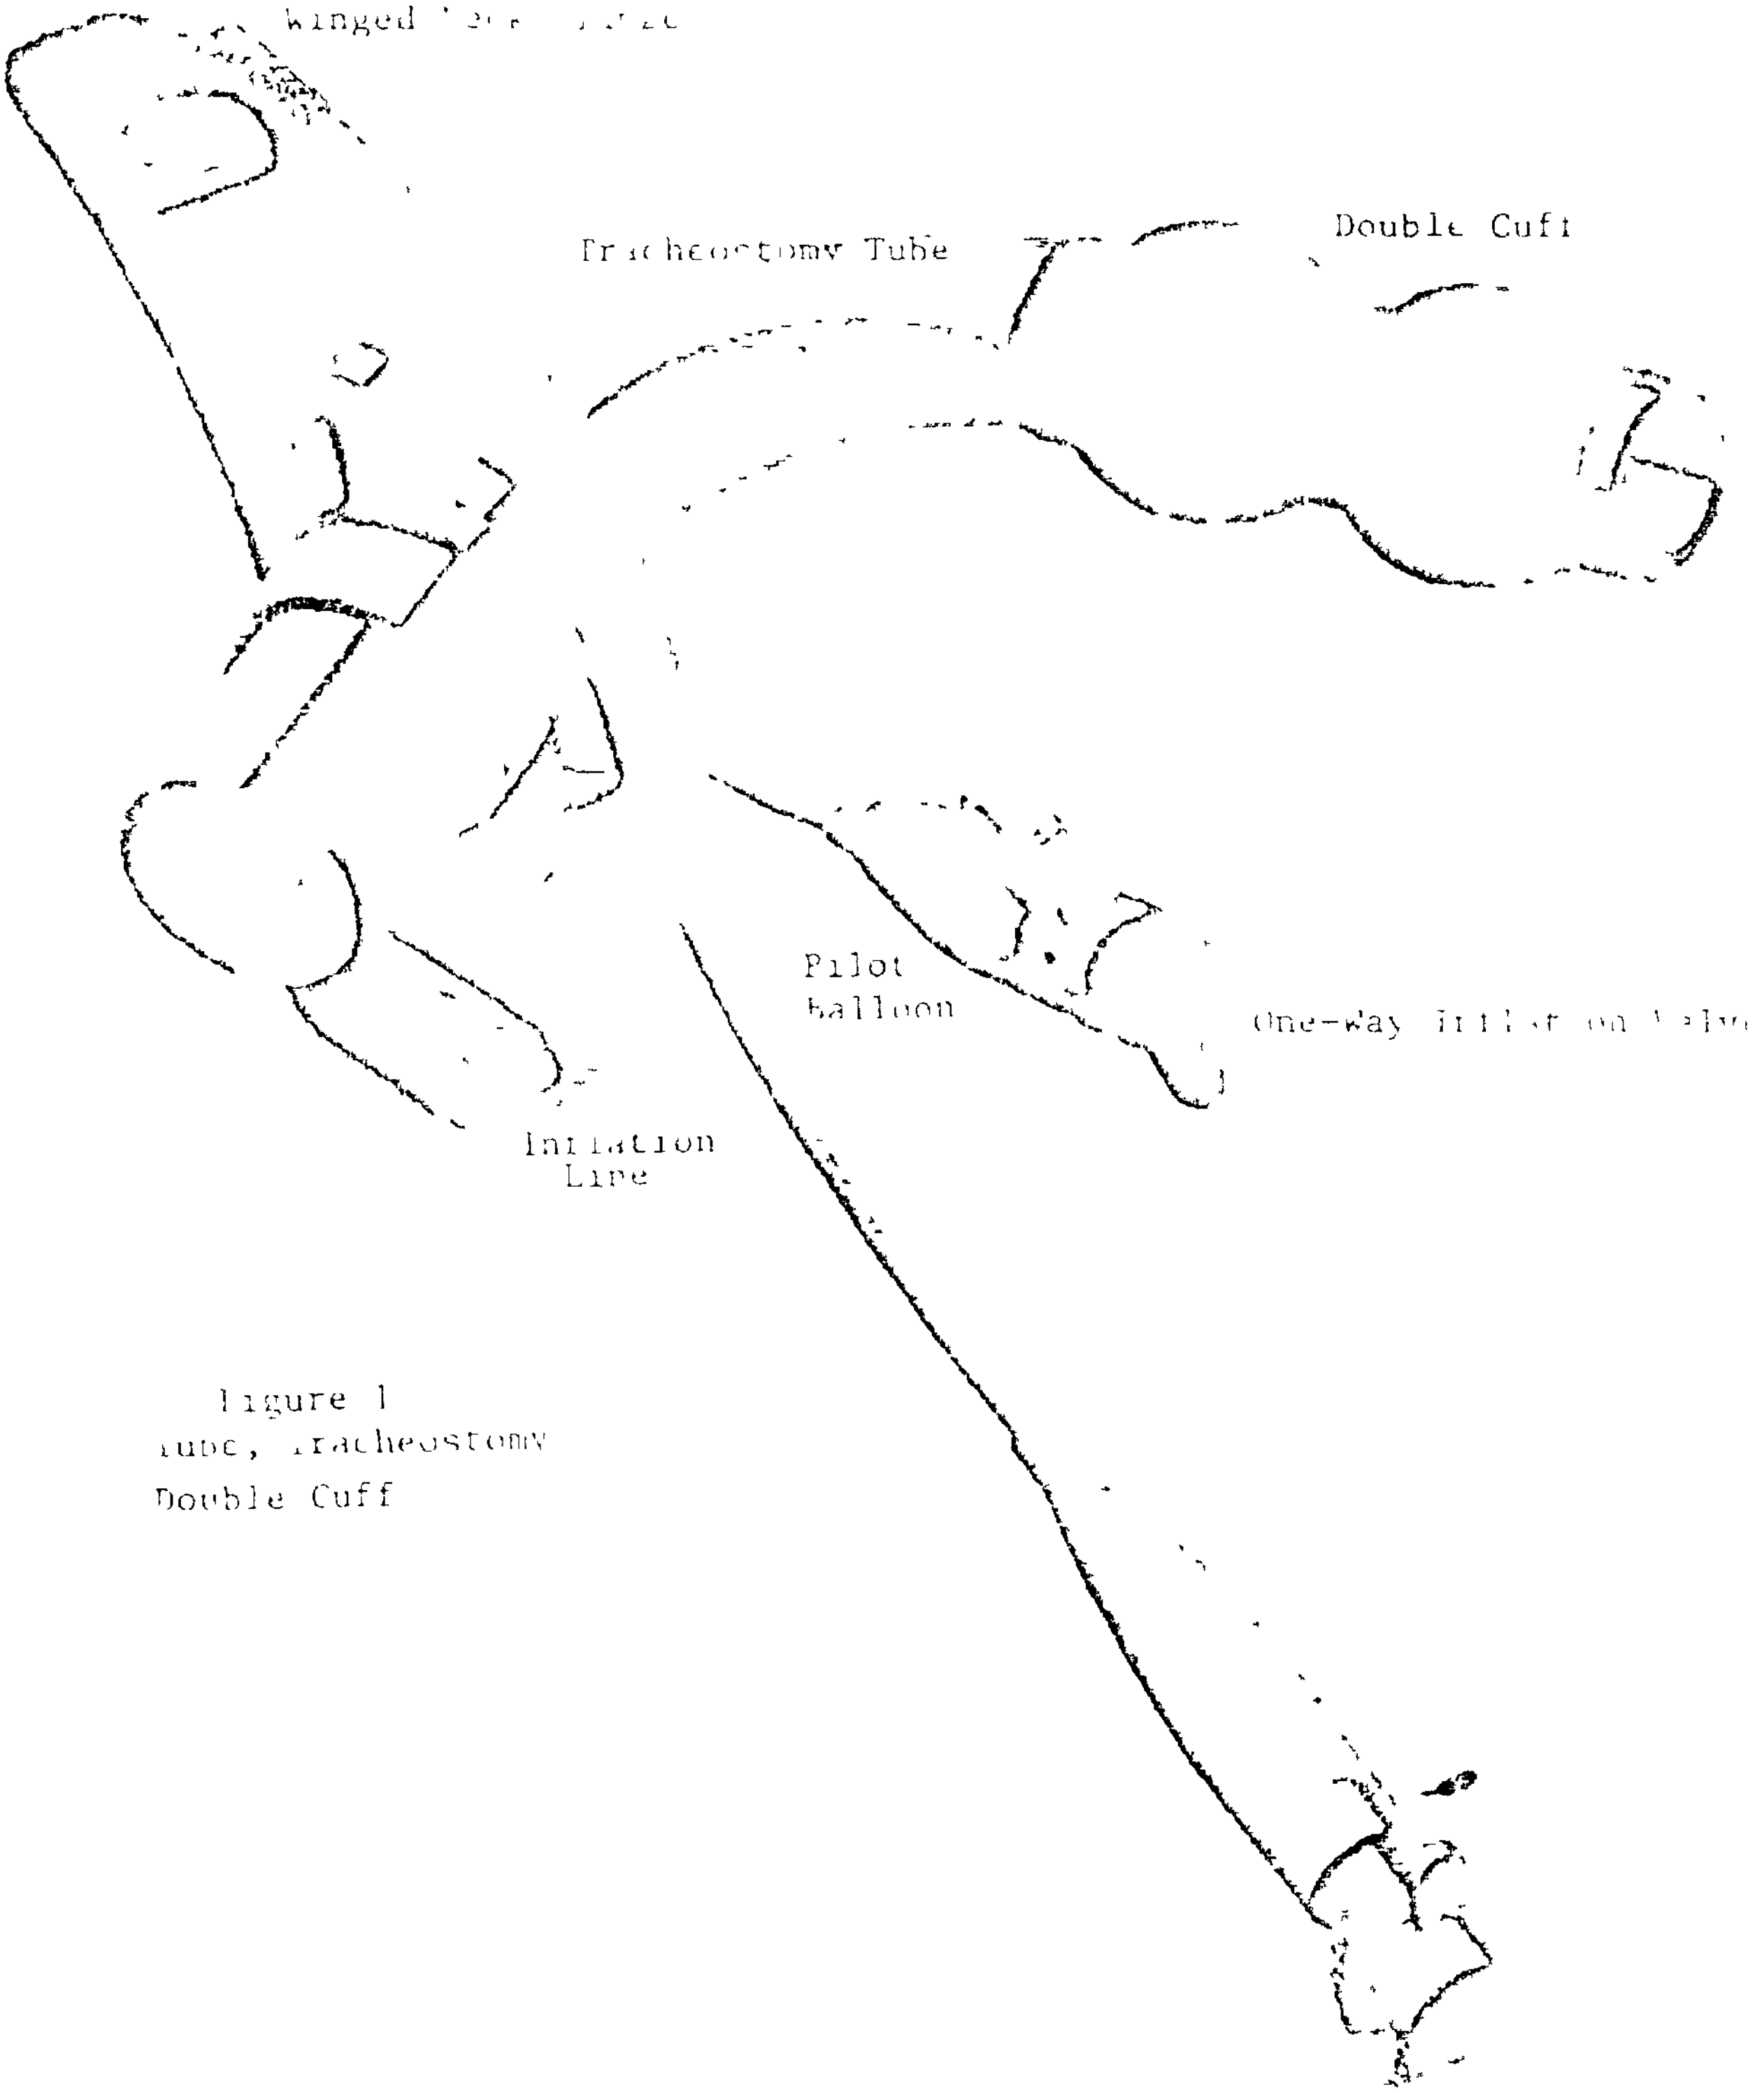
Winged Neck Plate
Tracheostomy Tube
Double Cuff
Pilot Balloon
One-Way Inflation Valve
Inflation Line

Figure 1
Tube, Tracheostomy
Double Cuff

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER A-A-54388	2. DOCUMENT DATE (YYMMDD) 5-12-91

3. DOCUMENT TITLE
TUBE, TRACHEOSTOMY, Double Cuff

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME Defense Personnel Support Center	b. TELEPHONE (Include Area Code) (1) Commercial (215)737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) ATTN: DPSC-HSTF 2800 S. 20th Street Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete.