A-A-54399
17 May 1991

COMMERCIAL ITEM DESCRIPTION

SPECULUM, NASAL (Vienna, 5-3/4 Inch)

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-S-37052A which is cancelled.

This commercial item description covers a nasal speculum of the Vienna style, suitable for the visual examination and treatment of the nose.

Salient Characteristics:

General. The speculum shall be a 5-3/4 inch, adult model, bivalve nasal speculum.

Material. Material of the speculum shall be Class 3 type 302, 303 or 304 steel in accordance with ASTM Designation F899.

Hardness. The speculum shall have a Rockwell Hardness B scale (HRB) of 75 to 80 when tested in accordance with ASTM Designation E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Style, design and dimensions. Handles shall possess indentations or serrations for gripping purposes. The lock shall be of the modified screw-type. The speculum shall be in accordance with Figure 1 for style, design and dimensions.

Finish. The speculum shall have a mirror, or mirror and satin finish. Finish of all surfaces including inside surface of the blades, shall be smooth and uniform.

Passivation. The speculum shall be properly passivated.

Corrosion resistance. The speculum shall show no evidence of corrosion when tested in accordance with ASTM Designation F1089.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

Performance. The speculum shall be capable of easy opening when nominal hand pressure is applied and shall close freely without binding or setting when hand pressure is released.

Identification marking and labeling. The speculum shall be legibly marked with the contractor's name or trademark and the word "stainless". Foreign manufactured specula shall bear the name of the country of origin.

Workmanship. The nasal speculum shall be free from defects which detract from its appearance or impair its serviceability. Specula shall be free from sharp edges, burrs, distortion, tool marks, corrosion, pits or foreign material.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. The speculum shall be examined to verify that the design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements as specified.

Unit. Each (EA). One nasal speculum, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one nasal speculum. Sampling shall be inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one speculum. Sampling shall be inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-369-9100	SPECULUM, NASAL, Vienna, 5-3/4 Inch

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PCC 45670 Project No. 6515-5030

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

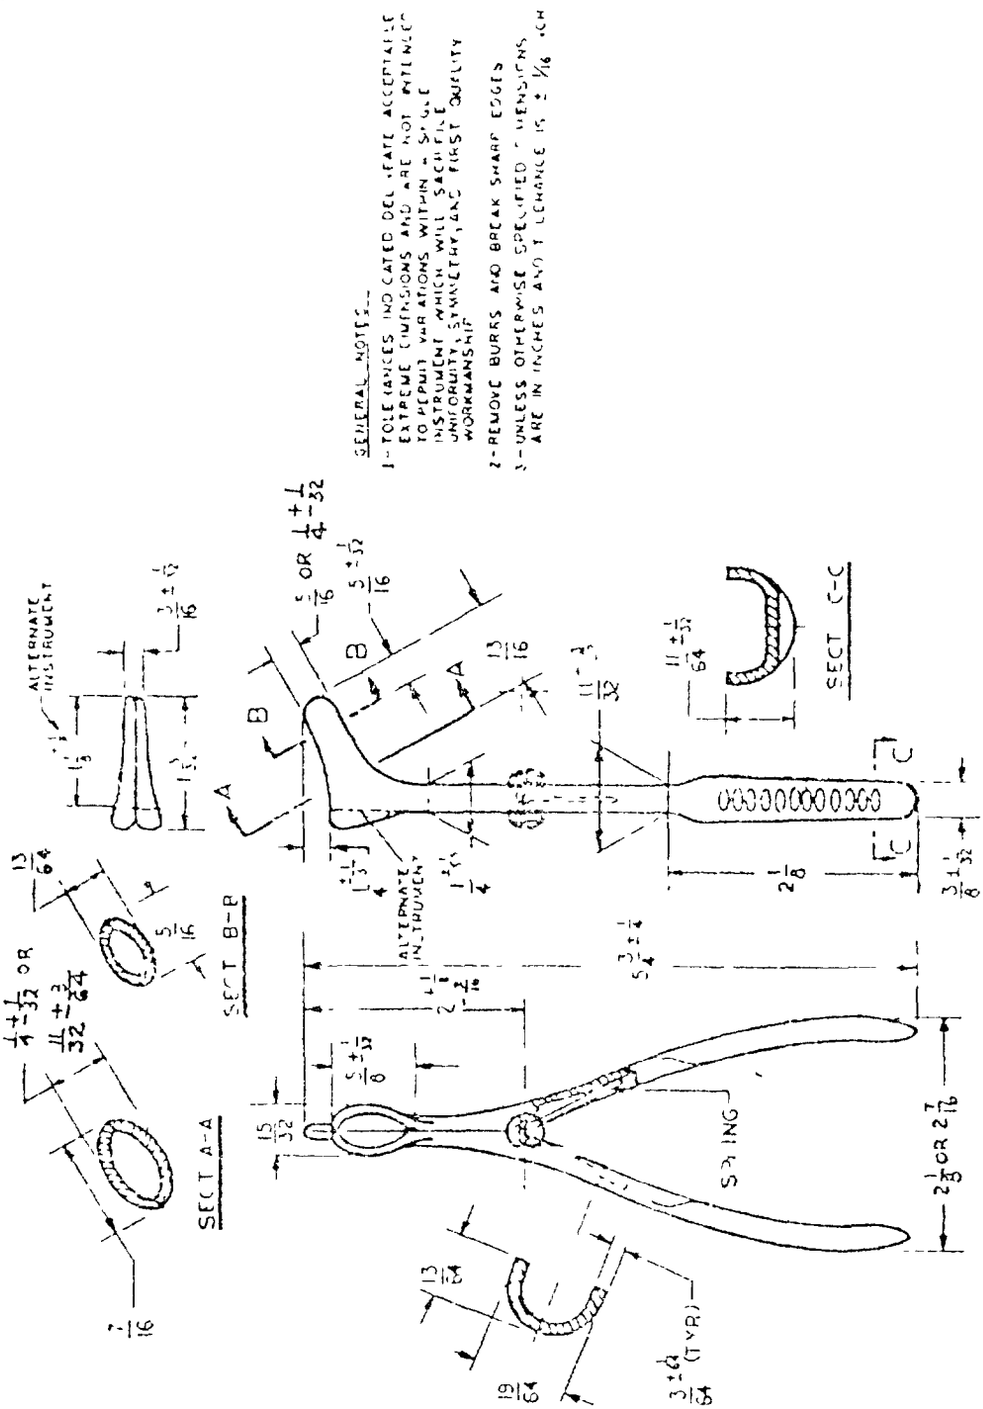

NSN 6515-00-329-9800

SPECULUM, NASAL, VIENNA, 5¾ INCH
FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of this form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

1. [illegible] NUMBER:	2. DOCUMENT NUMBER: A-A-54399	3. DOCUMENT DATE (YYMMDD): 17 May 1991

4. NOMENCLATURE: SPECULUM, NASAL (Vienna, 5-3/4 Inch)

4a. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE NUMBER (Include Area Code) (1) Commercial (2) AUTOVON
	e. DATE SUBMITTED

7. PREPARING ACTIVITY

a. NAME: Defense Personnel Support Center	b. TELEPHONE (Include Area Code) (1) Commercial: (215)737-2570 (2) AUTOVON: 444-2870
c. ADDRESS (Include Zip Code): ATTN: DPSC-WSTE, 2800 S. 20th Street, Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office, 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466, Telephone (703)756-2340, AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous edition is obsolete. — 96/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:33Z
Check the source to verify that this is the current version before use.