MILITARY SPECIFICATION

ANOSCOPE, BRINKERHOFF, 3-3/4 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of a conical rectal speculum, of the Brinkerhoff design.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The anoscope shall be in accordance with the applicable requirements of GG-I-526, and the following option exercises under that specification:

3.2 Material. The anoscope shall be fabricated from class 3 austenitic stainless steel, type 304 material in accordance with GG-I-526.

3.3 Hardness. After proper stress relieving, the Rockwell hardness shall be B75-B85.

3.4 Style, design, and dimensions. Shall be a conical rectal speculum, of the Brinkerhoff design, suitable for use in examination of the human rectum. Shall consist of a hollow cone with blunt tip, one side of which shall be open and which is covered by means of a sliding door arrangement; each cone shall have a handle, and a door arrangement which shall permit a variable sized opening in the speculum. Anoscope shall be in accordance with Figure I.

3.5 Finish. Shall be mirror, or mirror and satin.

3.6 Identification marking. In addition to GG-I-526 requirements, anoscopes of foreign manufacture shall also be marked "stainless".

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:41Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specifications where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Shall be in accordance with GG-I-526.

4.1.2 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the stainless steel may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination shall be one anoscope.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:41Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of product for test purposes shall be one anoscope.

Table II. Sampling for Tests

Component (unit of product)	Characteristic	Req.	Test Procedure	Insp. level	AQL (percent defective)
1-Anoscope	Composition analysis	3.2 & GG-I-526	GG-I-526	**	*
1-Anoscope	Hardness	3.3 & GG-I-526	GG-I-526	S-2	*
1-Anoscope	Dimensions	3.4	-------	S-1	*
1-Anoscope	Boil Test	GG-I-526	GG-I-526	S-2	*

* Acceptance number shall be zero for all sample sizes.

** Sufficient amount from each lot of each metal used in the construction of the anoscope shall be selected for composition analysis.

4.3 Examination. The anoscope shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any anoscope in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Instrument not constructed as specified.
102	Style and design not as specified.
103	Instrument not free of sharp edges, rough areas, burrs, cracks, grind marks or overlaps.
104	Sliding door not free and easy to open or close.
105	Sliding door not of flush fit with adjacent surfaces of the cone.
Minor	
201	Identification marking not present, correct, complete, or legible.
202	Finish not as specified.
203	Packaging and packing not as specified.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements in accordance with GG-I-526 and as specified herein.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One anoscope as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not Required	48 units

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:41Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be utilized.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-2.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Fiberboard boxes shall conform to the special requirements as specified in Table II of PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:41Z
Check the source to verify that this is the current version before use.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636. In addition, fiberboard boxes shall conform to the special requirements as specified in Table I of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The anoscope is intended for use in examination of the human rectum.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:41Z
Check the source to verify that this is the currentversion before use.

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-370-2300	ANOSCOPE, BRINKERHOFF, 3-3/4 INCH

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 6, dated 14 October 1971, for FSN 6515-370-2300, ANOSCOPE, Brinkerhoff, 3-3/4 inch.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1742


Review activities:

Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.

NOTES:

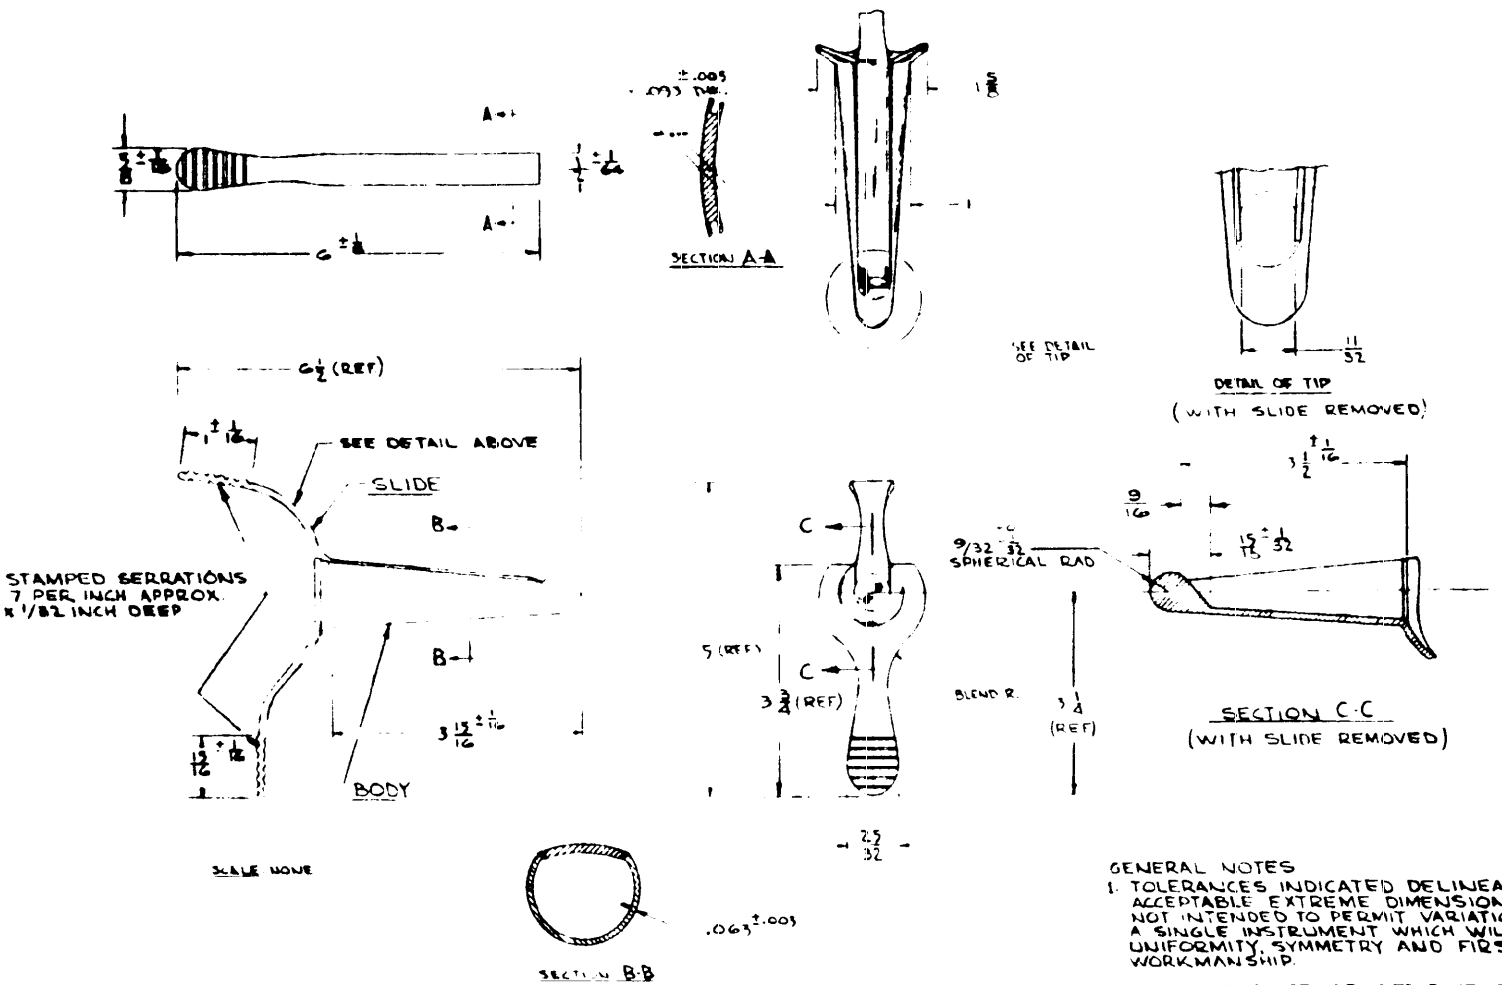

GENERAL NOTES

1. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.
2. UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCE IS ±1/32 INCH.

ANOSCOPE, BRINKERHOFF, 3 3/4 INCH

FIGURE 1

☆ U. S. GOVERNMENT PRINTING OFFICE: 1974-603-111 2790

HH-A-36977

Source: https://assist.dla.mil -- Downloaded: 2026/10-21T09:41Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4 REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

Commander
Defense Personnel Support Center
ATTN: DPSC-ATT
2800 South 20th Street
Philadelphia, Pa. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:41Z
Check the source to verify that this is the current version before use.