MILITARY SPECIFICATION

CURETTE, MASTOID, RICHARD

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers two sizes of Richard mastoid curettes suitable for use in removing diseased cells of the mastoid.

1.2 Classification. Curettes shall be furnished in the following sizes, as indicated below (see 6.1):

Size 1 (5/32 inch blade)

Size 5 (9/32 inch blade)

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
QQ-C-320	Chromium Plating (Electrodeposited).
QQ-N-290	Nickel Plating, (Electrodeposited).
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Miliatary

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.).

3. REQUIREMENTS

3.1 General requirements. The curettes shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The blades and shanks of the curettes shall be fabricated from class 4, type 420. The handles shall be class 4, type 420 or class 8, type 260 or 270.

3.3 Hardness. Rockwell hardness shall be C40-C45. Blades and shanks shall be first properly stress relieved.


3.4 Style, design and dimensions. Shall be mastoid curette, sharp, Richard design, with hollow handle, suitable for removal of diseased cells of the mastoid. Shall be in accordance with Figure I.

3.5 Finish. Shall be mirror, or mirror and satin.

3.6 Identification marking. In addition to GG-I-526 requirements, instruments of foreign manufacture shall be marked "stainless", when applicable.


Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T09:42Z
Check the source to verify that this is the current version before use.

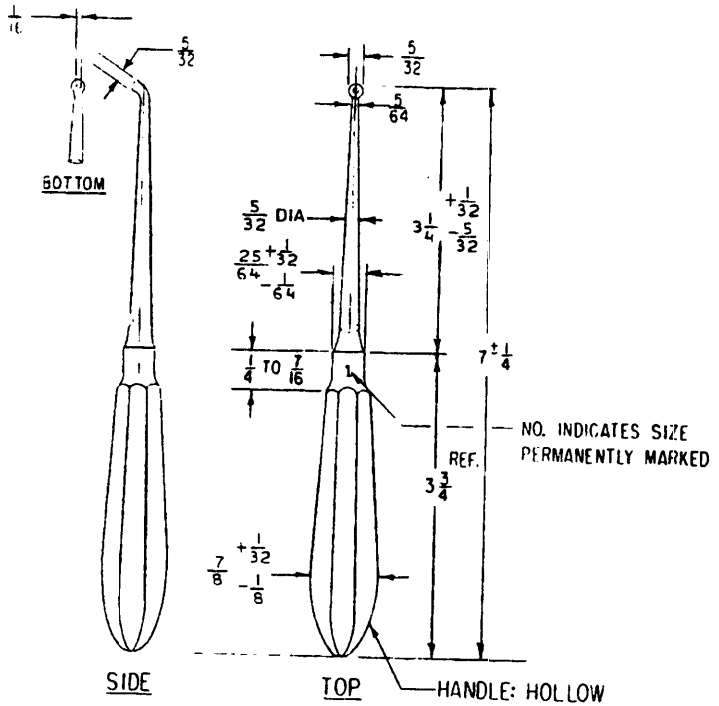

FSN-6515-322-6600

SIZE 1

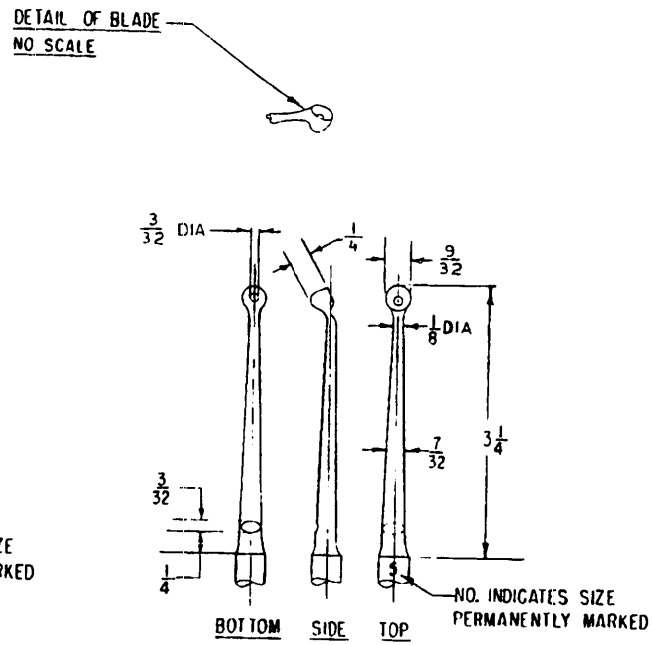

FSN-6515-322-6800

HANDLE SAME AS 6515-322-6600

SIZE 5

UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES AND TOLERANCES ARE AS FOLLOWS:

DIMS. 1/8 IN. AND UNDER ± .005 IN.
DIMS. OVER 1/8 IN. TO 1/4 IN. ± .010 IN.
DIMS. OVER 1/4 IN. TO 1/2 IN. ± .015 IN.
DIMS. OVER 1/2 IN. ± .032 IN.

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.

CURETTE, MASTOID, RICHARD

FIGURE 1

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein, Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel and brass, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in Table I. The unit of product for examination purposes shall be one curette.

Table I. Sampling for Examination

Type defect	Inspection level	AQL (percent defecitve)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:42Z
Check the source to verify that this is the currenversion before use.

* 4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. The unit of product for test purposes shall be one curette.

Table II. Sampling Criteria for Tests

Component	Characteristic	Req.	Test procedure	Insp. level	AQL
Curette	Composition analysis	3.2 and GG-I-526	GG-I-526	*	-
	Hardness (1)	3.2	4.4.1	S-2	1.5
	Dimensions	3.4	-----	S-2	2.5
	Plating (2)	3.6.1	QQ-N-290 & QQ-C-320	S-2	1.0
	Copper sulfate (1)	3.7.1	4.4.4.1	S-2	1.0
	Salt spray test (2)	3.7.2	4.4.4.2	S-2	1.0
	Boil test (For all material)	3.7.3	4.4.4.3	S-2	1.0

(1) For class 4 material.
(2) For class 8 material.
* Four ounces of each lot or each metal used in the construction of the curette shall be selected for chemical analysis.

4.2.3 Sample unit usage. Where feasible, the same sample unit shall be used for the determination of two, or more test characteristics.

4.3 Examination. The curettes shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects in Table III. Any curettes in the sample containing one or more defects shall be rejected and if the number of defective curettes in any sample exceeds the acceptance number for that sample, the lot represented by that sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Curette not of the proper size for the appropriate stock number.
102	Cutting edges not sharp.
103	Finish not uniform.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects (cont'd)

Categories	Defects
Major (cont'd)	
104	Curettes not free from burrs, sharp edges (except for cutting edges), pits, cracks, foreign matter, and corrosion.
105	Plated handles not free from flaking.
106	Blade and shank not permanently secured to handle.
107	Handle of solid stock construction.
Minor	
201	Curettes not marked with contractor's name or registered trademark.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Unit of issue. One curette, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be utilized.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-2.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall by adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commerical containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Fiberboard boxes shall conform to special requirements specified in Table II of PPP-B-636.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636. In addition, fiberboard boxes shall conform to the special requirements specified in Table I of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial container of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The mastoid curettes are intended for removal of diseased cells of the mastoid.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Size required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

6.3 This specification is intended to cover the following items appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-322-6600	CURETTE, MASTOID, Richard, size 1
6515-00-322-6800	CURETTE, MASTOID, Richard, size 5

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 5, dated 13 March 1972 for NSN 6515-00-322-6600 CURETTE, MASTOID, Richard, size 1, and NSN 6515-00-322-6800 CURETTE, MASTOID, Richard, size 5.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1749

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-C-36985

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:42Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:42Z
Check the source to verify that this is the current version before use.