MILITARY SPECIFICATION

CLAMP, BRONCHUS, DOUBLE CURVED, DAEMS, 9-1/2 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of bronchus clamp suitable for use in thoracic surgery.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard
PPP-B-676	Box, Set-up.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

Military

MIL-P-116 Preservation, Methods of.

MIL-L-10547 Liners, Case and Sheet, Overwrap; Water-vaporproof or Waterproof; Flexible.

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.

MIL-STD-129 Marking for shipment and storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The bronchus clamp shall be in accordance with the applicable requirements of GG-I-526, and the following option exercises under that specification:

3.2 Material. The clamp shall be fabricated from Class 4, type 410 or type 420 material.

3.3 Hardness. After proper stress relieving, the clamp shall have a Rockwell hardness of Rc40, minimum.

3.4 Style, design and dimensions. Shall be a double curved bronchus clamp of the Daems design, without teeth, with ratchet. Shall be in accordance with Figure 1.

3.4.1 Locks. Shall be box type lock.

3.5 Finish. Finish shall be mirror.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

3.6 Lock stiffness. Forceps of box lock construction shall have shanks tested for lock stiffness in accordance with GG-I-526.

3.7 Identification marking. In addition to GG-I-526 requirements, clamps of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS


4.1 Responsibility for inspection. Unless otherwise specified in contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

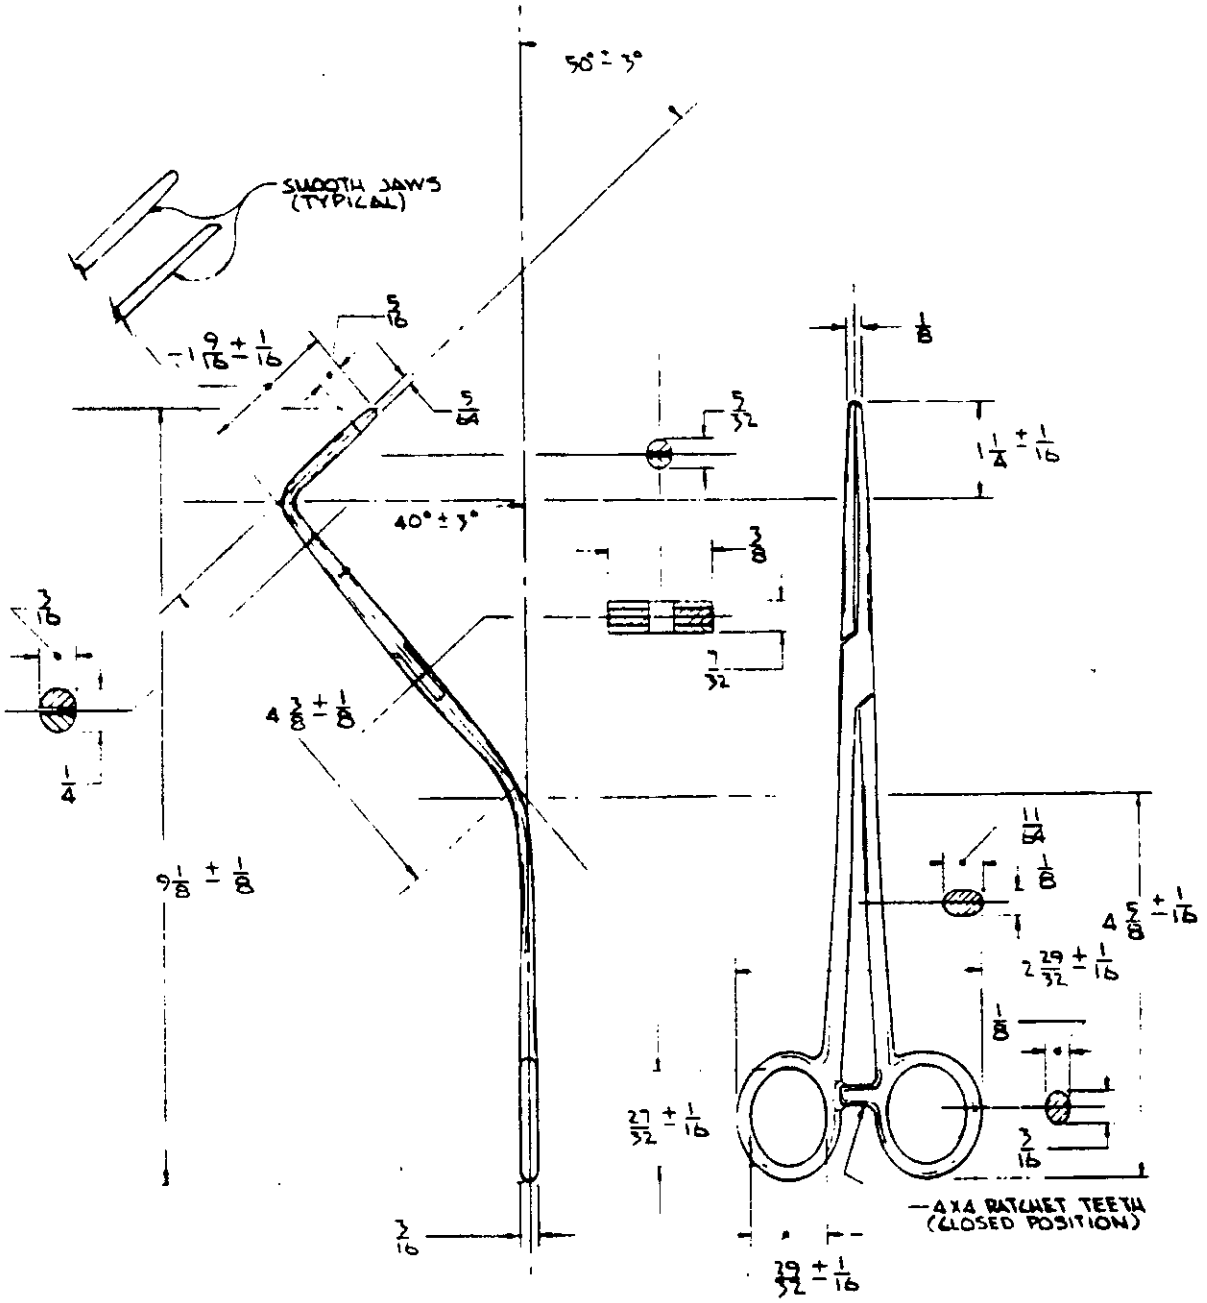

NOTES:

1. UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCES ARE AS FOLLOWS: FRACTIONS ± 1/32.
2. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination, Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one bronchus clamp.

Table I. Sampling Criteria for Examination

Type of defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Unit of Product for test purposes shall be one bronchus clamp.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test Procedure	Insp. level	AQL
1-Clamp	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*
	Hardness	3.3 and GG-I-526	GG-I-526	S-2	*
	Box lock stiffness	3.6	GG-I-526	S-2	*
	Copper sulfate	GG-I-526	GG-I-526	S-2	*
	Boil test	GG-I-526	GG-I-526	S-2	*

* Acceptance number shall be zero for all sample sizes.
** Four ounces of each lot of metal used in the construction of clamp shall be selected for chemical analysis.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

4.3 Examination. The clamp shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any clamp in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Clamp not free from cracks, pits, dents, nicks, sharp edges and burrs.
103	Ratchet teeth not uniform, or function poorly.
104	Clamp not of box lock design.
105	Holder not free from excessive play in box lock area.
Minor	
201	Finish not mirror, and not uniform.
202	Identification marking not present, correct, complete or legible.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.2).

5.1.1 Unit of issue. One clamp, as specified, constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with paragraph 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The bronchus clamps are intended for use in thoracic surgery.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-890-1678	CLAMP, BRONCHUS, Double Curved, Daems, 9-1/2 inch

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 2, dated 12 October 1964 for FSN 6515-890-1678 Clamp, Bronchus, Double Curved, Daems, 9-1/2 inch.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1763

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-C-37002

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:45Z
Check the source to verify that this is the current version before use.