MIL-I-36993A
22 June 1987
(Superseding)
MIL-I-36993
15 September 1974

MILITARY SPECIFICATION

IMPRESSION MATERIAL, DENTAL

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers a non-toxic impression and tissue treatment material suitable for allowing abused and distorted oral tissue to regain its normal anatomic configuration and physiologic tone.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DoDISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

Federal

RR-S-366	Sieve, Standard for Testing Purposes.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-601	Boxes, Wood, Cleated-plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

AMSC N/A FSC 6520

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RSTS, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.
MIL-STD-147	Palletized Unit Loads.
MIL-STD-794	Parts and Equipment, Procedures for Packaging of.

(Copies of specifications, standards and publications required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DoDISS specified in the solicitation. Unless otherwise specified, the issues of documents not listed in the DoDISS are the issues of the nongovernment documents which are current on the date of the solicitation.

U.S. DEPARTMENT OF HEALTH AND HUMAN SERVICES (HHS)
FOOD AND DRUG ADMINISTRATION (FDA)

Federal Food, Drug and Cosmetic Act and regulations promulgated thereunder.

(Application for copies should be addressed to the Food and Drug Administration, Washington, D.C. 20204.)

THE UNITED STATES PHARMACOPEIAL CONVENTION, INC.

The United States Pharmacopeia (USP).

(Application for copies should be addressed to the Mack Publishing Co., Easton, PA. 18042.)

The National Formulary (NF).

(Application for copies should be addressed to Mack Publishing Co., Easton, PA 18042.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

(Nongovernment standards and other publications are normally available from the organizations which prepare or which distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification takes precedence. Nothing in this specification, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Materials. Materials shall be of the highest quality throughout and suitable in all respects for the purpose intended. Any ingredients entering into the impression material which are not included in "The United States Pharmacopeia" (U.S.P) or "National Formulary" (N.F.) shall be of quality suitable for pharmaceutical use.

3.1.1 Impression material. The impression material shall conform to either one of the following two compositions: (see 3.1.2 and 3.1.3) providing differing ingredients from one formula are not interchanged with respect to the other formula.

3.1.2 Composition A. Powder shall be ethyl methacrylate resin. Liquid shall be denatured ethyl alcohol with methyl salicylate and glycolate plasticizers. Separating medium shall be essentially silicone with the main ingredient being dimethylpolysiloxane.

3.1.3 Composition B. Powder shall be ethyl methacrylate resin with zinc undecylenate. Liquid shall be formulated of an aromatic ester, fixed oil, ester plasticizer with a small amount of ethyl alcohol and deodorant. A suitable lubricant for separating the impression material from the gypsum casts shall be furnished.

3.2 Physical properties.

3.2.1 Odor and flavor. The material shall not have an unpleasant odor or flavor when tested as specified in 4.4.3.

3.2.2 Irritation and fungus growth. Unless otherwise specified, prior to delivery the manufacturer shall furnish a statement directly to the Directorate of Medical Materiel, Technical Services Branch, (DPSC-RSTS-2) Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, stating that the material does not normally irritate oral tissues and does not contain poisonous ingredients in sufficient concentration to be harmful to human beings when used as directed and that it does not support fungus growth.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the currentversion before use.

3.2.3 Fineness. When tested as specified in 4.4.4, 95 to 99 percent of the powder shall pass through an 80 mesh sieve.

3.2.4 Mixing time and uniformity. The time of mixing the impression material in accordance with manufacturer's directions to obtain the required consistency shall be no more than one minute when tested as specified in 4.4.5. The mix obtained shall be smooth, homogeneous, workable, and free from lumps and granules.

3.2.5 Pliability. When mixed according to manufacturer's instructions, impression material shall remain pliable, that is, shall be capable of deformation under an approximate pressure of 85 millimeters (mm) of mercury (the approximate equivalent of diastolic blood pressure), for a minimum of 2 days when applied inside provisional dentures and tested as specified in 4.4.6.

3.2.6 Working time. The working time (time during which material is plastic and moldable) when tested as specified in 4.4.7 shall be no less than 3 minutes.

3.2.7 Hardness. Impression material shall have a Shore durometer hardness of 5 to 12 when tested as specified in 4.4.8.

3.2.8 Reproduction of detail. The material shall reproduce a line 0.025 mm. wide when tested as specified in 4.4.9.

3.2.9 Strain in compression. The percentage of recovery shall be no less than 65 percent when the impression material is tested as specified in 4.4.10.

3.2.10 Weight loss. The weight loss for the impression material shall be no more than 3 percent when tested as specified in 4.4.11.

3.2.11 Dimensional accuracy. The maximum dimensional change at 15 minutes from the start of mix shall be 0.4 percent when tested as specified in 4.4.13.

3.3 Description. The impression material shall be a non-toxic impression and tissue treatment material. Unit of issue shall be a package containing a bottle of powder, a bottle of liquid, a bottle of separating medium (lubricant), a powder measure, a liquid measure, a minimum of 12 disposable mixing cups (or one reusable mixing vessel), and instructions for use (see 3.1.2 and 3.1.3). A spatula and patient education sheets may also be furnished at the manufacturer's option.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the currentversion before use.

3.3.1 Accessories. A powder proportioner suitable for scooping out the powder and a liquid proportioner suitable for measuring out the liquid shall be enclosed in each unit container. Volume of powder and liquid proportioners shall be appropriate to provide a mix with required consistency. A minimum of twelve disposable mixing cups shall be included in the unit package. Cups shall have a volume capacity sufficient for mixing individual portions. As an alternate to disposable cups, a reusable mixing vessel shall be included with a capacity of 2 ± 1/2 ounces. Supplementary accessories such as a spatula or patient education sheets may also be furnished at the manufacturer's option.

3.3.2 Immediate container. Contents of immediate container shall be as follows (see 3.1.1. and 3.1.2):

one 6-ounce (minimum) bottle of powder
one 6-ounce (minimum) bottle of liquid
one 1/2-ounce (minimum) bottle of separating medium (lubricant)

one powder measure
one liquid measure
sufficient mixing cups (12 minimum) disposable
or
one reusable mixing vessel
Instructions for use

Volume of liquid furnished shall be 5 percent in excess for the total powder-liquid ratio required by manufacturer's instructions. Bottles for powder and liquid may be either glass or plastic. If made of glass, caps shall be screw-on type. If made of plastic, caps shall be either screw on, or with pouring spout, except that for liquid, the cap shall be screwed on with an extra cap provided that has a pouring spout. The container for the lubricant (separating medium) shall be either plastic or glass. Cap shall either be screwed on with brush attached to cap or plastic with squeeze-type cap with protective cover. Powder and liquid measures shall be either glass or plastic and may be either colored clear or opaque. Disposable cups shall be either plastic (polypropylene) or foil lined paper cups. If a reusable mixing vessel is provided, it may be either glass or plastic. Spatula, if provided, shall be fabricated of a material that will not interact with the impression material. The immediate containers and all components shall be compatible, and shall not interact physically or chemically with the powder, liquid or mixed impression material.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

3.4 Amount of material in unit container. A single mix of the impression material, when prepared using the powder and liquid measures provided by the manufacturer, shall have a bulk displacement of between 10.8 and 15.2 milliliters (ml.). The total amount of material in the unit of issue shall be sufficient to prepare a minumum of 25 impressions when tested as specified in 4.4.12.

3.5 Instructions for use. Adequate and accurate instructions for manipulating the material shall accompany each unit container. These instructions shall include the following minimum requirements:

1. Preparation of the denture before treatment.
2. Preparation of the patient's mouth before treatment.
3. Proportions of powder and liquid to be used to give proper mix in terms of scoops of powder to scoops of liquid.
4. Method of mixing.
5. Mixing time.
6. Proper use and application of the lubricant (separating compound).

Instructions for use shall be furnished as a separate sheet in the unit container.

3.6 Delivery schedule. No more than three months shall have elapsed from the date of manufacture of the impression material to the date of delivery to the Government.

3.7 Marking. In addition to the requirements specified in 5.3.1, 5.3.2 and 5.3.3, each unit package of material shall be marked with a serial number or combination of letters and numbers which shall refer to the manufacturer's records for the particular lot or batch. Each bottle shall be marked as "Powder", "Liquid", "Separating Medium", or "Lubricant", according to the contents. Bottles shall also be marked with the name or trademark of the manufacturer and net weight.

3.8 Workmanship. The impression material shall be free from defects which may detract from its appearance or impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the currentversion before use.

The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of supplies to which records relate.

4.1.2 Inspection. Inspection, as used in this specification is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the components or materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the components or materials, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables I and III (see 4.2.1 and 4.3) and table II (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be as indicated in table I. Unit of product for examination purposes shall be the unit of issue (one package).

Table I. Inspection and Acceptable Quality Levels

Type defect	Inspection level	AQL (Percent Defective)
Major	II	1.5
Minor	II	4.0

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

4.2.2 Sampling for tests. The unit of product for testing shall be one container of powder and one container of liquid taken at random from each lot or batch number. Where feasible, the same test unit may be used for two or more different test characteristics. The number of determinations for each characteristic shall be as listed in table II.

Table II. Tests

Characteristic	Reqmt.	Test procedure	Unit of product to be tested per lot or batch number	Number of determinations per unit of product	Total number of determinations
Odor and flavor	3.2.1	4.4.3	1	1*	1
Fineness	3.2.3	4.4.4	1	1*	1
Mixing time and uniformity	3.2.4	4.4.5	1	1*	1
Pliability	3.2.5	4.4.6	1	3**	3
Working time	3.2.6	4.4.7	1	1*	1
Hardness	3.2.7	4.4.8	1	1*	1
Reproduction of detail	3.2.8	4.4.9	1	1*	1
Strain in compression	3.2.9	4.4.10	1	3**	3
Weight loss	3.2.10	4.4.11	1	3**	3
Dimensional accuracy	3.2.11	4.4.13	1	3**	3
Amount of material in unit container	3.4	4.4.12	1	2**	2

* A lot shall be rejected if any determination fails the test requirement.
** A lot shall be rejected if the average of the determinations per unit of product fails the test.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

medium and minimum time in each case shall be soybean casein digest for 7 days

4.3 Examination. Impression material shall be examined for defects, including, but not limited to, those listed in table III.

Table III. Classification of defects

Categories	Defects
Major	
101	Instructions not present in unit container, incorrect, incomplete.
102	All components not present in unit package.
103	Immediate containers leak.
104	Foreign material, such as dirt or lint present in powder or liquid.
Minor	
201	Packaging, packing, and marking not as specified.
202	Closure not as specified for immediate containers.
203	Unit container not marked with lot or batch number.

4.4 Tests.

4.4.1 Preparation of specimens. The specimens shall be prepared in accordance with the manufacturer's directions as furnished with the unit container (see 3.5).

4.4.2 Standard testing conditions. This paragraph shall apply for the tests specified in paragraphs 4.4.8, 4.4.9, 4.4.10 and 4.4.13. The impression material, mixed according to manufacturer's instructions shall be kept in an environment of 98 $\pm$ 2° F. and 95 $\pm$ 5 percent humidity (approximate "mouth temperature") except when tests are being performed. At the time of testing, the mix shall be removed from the "mouth temperature" environment and tested immediately so that the impression material will be as close to "mouth temperature" as possible.

4.4.3 Odor and flavor. The pleasantness or unpleasantness of the odor and flavor shall be determined by smelling and tasting the material.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

4.4.4. Fineness. Fifty grams of the powder as received from the manufacturer shall be placed on a No. 80 dry screening Tyler standard test sieve conforming to RR-S-366. One percent of a suitable anti-static agent shall be added and the sieve vibrated for 10 minutes. On completion of the test, the sieve shall be carefully examined for residue remaining on the upper surface of the wire or occluding the sieve openings.

4.4.5 Mixing time and uniformity. After mixing the impression material in accordance with instructions furnished (for not more than one minute), mix shall be observed for homogeneity, smoothness, and freedom from lumps and granules.


4.4.6 Pliability. After mixing the impression material in accordance with instructions furnished by the manufacturer, the mix shall be pliable and shall conform to the requirements specified in 3.2.5.


4.4.7 Working time. After mixing in accordance with manufacturer's instructions, the material shall remain workable and shall conform to the requirements specified in 3.2.6.

4.4.8 Hardness. After mixing in accordance with manufacturer's instructions, the impression material shall be formed into a specimen, approximately 10 x 2.5 x 5 mm, thick. Values for hardness shall be obtained by using a Shore A Durometer consisting of a blunt spring loaded indentor 1/32 inch in diameter which tapers to a 1/16 inch cylinder over a distance of 1/16 inch. The scale shall read from 0 to 100 hardness units. Readings shall be taken every 15 minutes for the first hour, with subsequent readings at 2,4,6,8, and 24 hours.

4.4.9 Reproduction of detail. A ring 16 mm high and approximately 3 centimeters (cm.) inside diameter shall be placed on a stainless steel test block similar to that shown in figure 1 so that the intersection of a cross-line and line A, 0.025 mm. (0.001 inch (in.)) wide, is in the center of the ring. As an alternate, a ring of the type specified above shall be positioned on a stainless steel test block similar to that shown in figure 2 so that the three lines of the test block are centered on the ring. The stainless steel test blocks may be lightly dusted with talcum powder and the excess talcum powder blown off, if the impression material adheres to the blocks. The ring shall be slightly overfilled with prepared material. A flat plate shall be placed on top and the excess material shall be squeezed out. Two minutes after the start of mix, the entire assembly shall be placed in a water bath maintained at 37 $\pm$ 1° Centigrade (C.) (98.6 $\pm$ 1.8° F.).

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

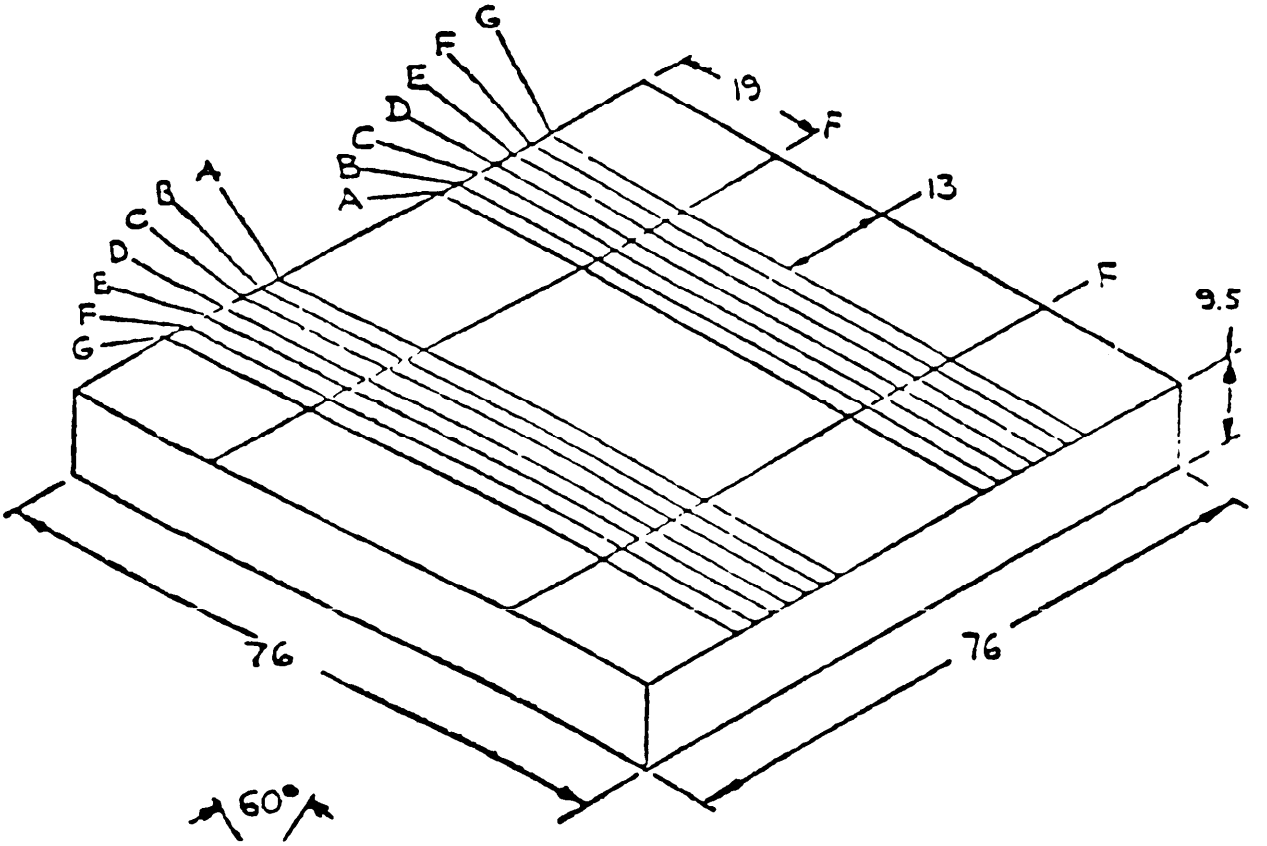




Cross Section of Ruled Lines

MILLIMETER

A = 0.025
B = 0.050
C = 0.075
D = 0.100
E = 0.150
F = 0.200
G = 0.300

Figure 1. Test Block for Detail Reproduction

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

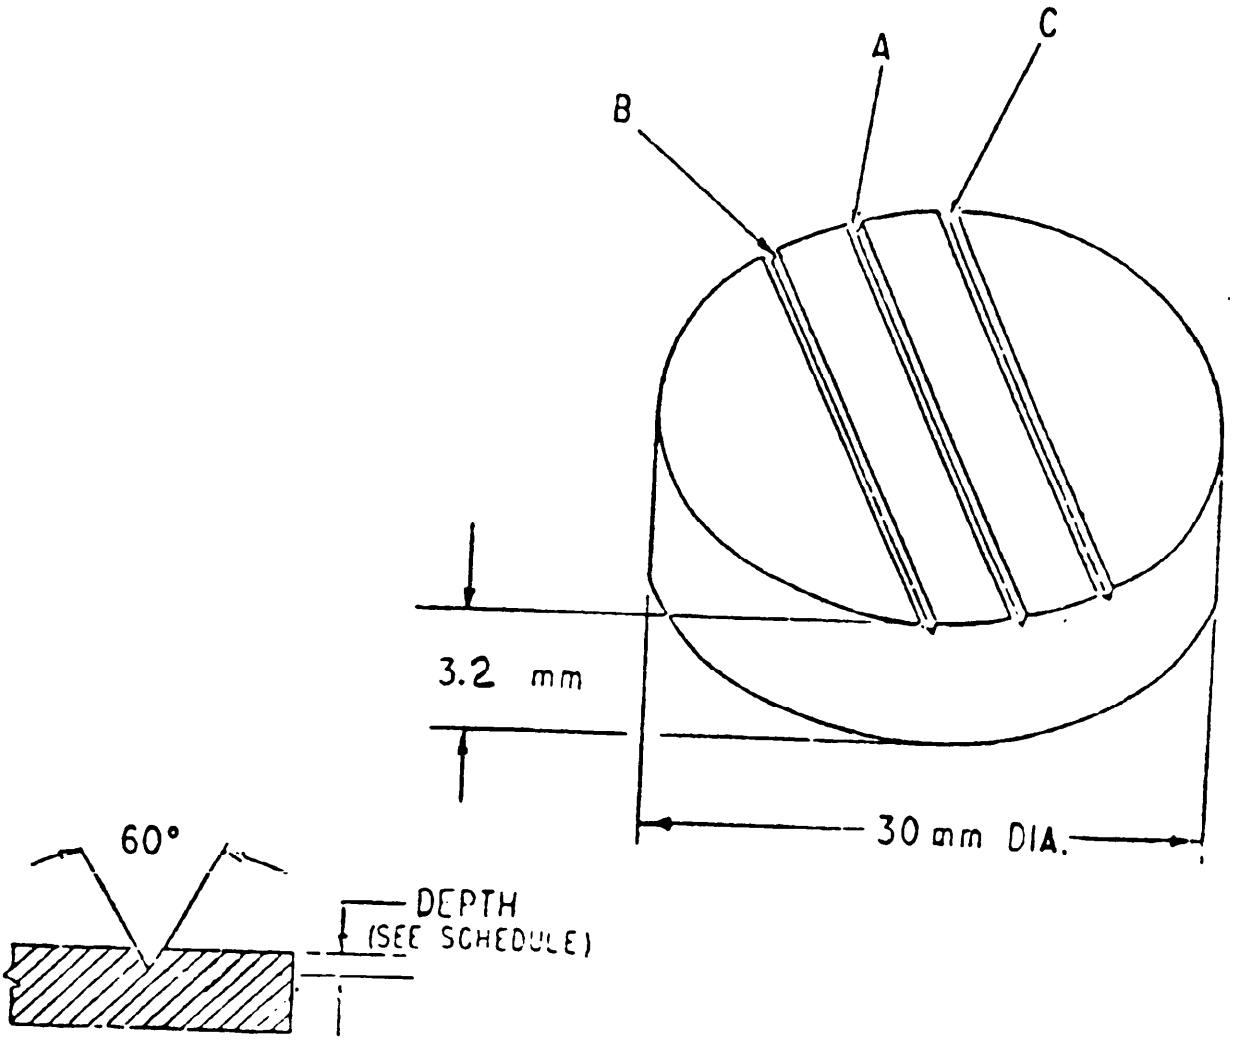

Cross Section of Ruled Lines

Depth of Ruled Lines:

Line "A" - 0.025 mm
Line "B" - 0.050 mm
Line "C" - 0.075 mm

Figure 2. Alternate Test Block for Detail Reproduction

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

The assembly shall remain in the water bath for 30 minutes. The ring with the impression material shall be separated from the test block immediately and the impression shall be examined under low angle illumination without magnification. The reproduction shall be considered to be satisfactory if the 0.025 mm. wide line is continuous for the full inside diameter of the ring.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

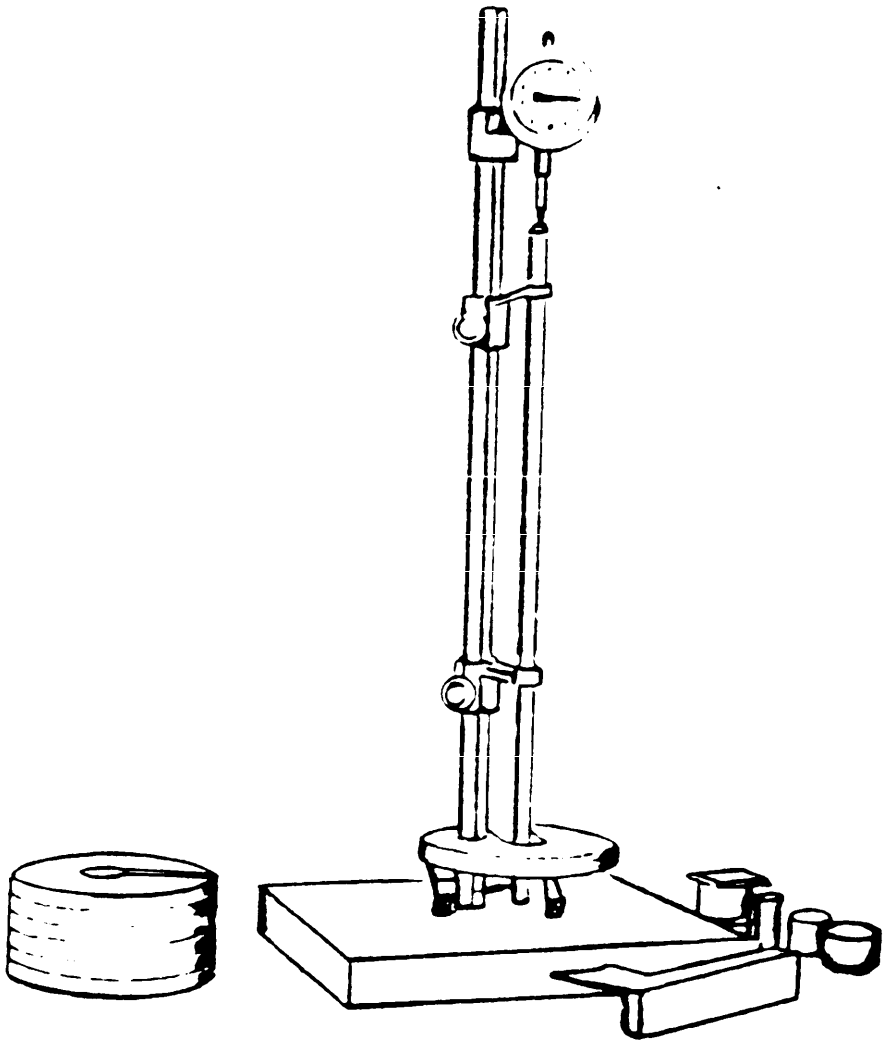


Figure 3. Fixture for Determining Properties in Compression

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

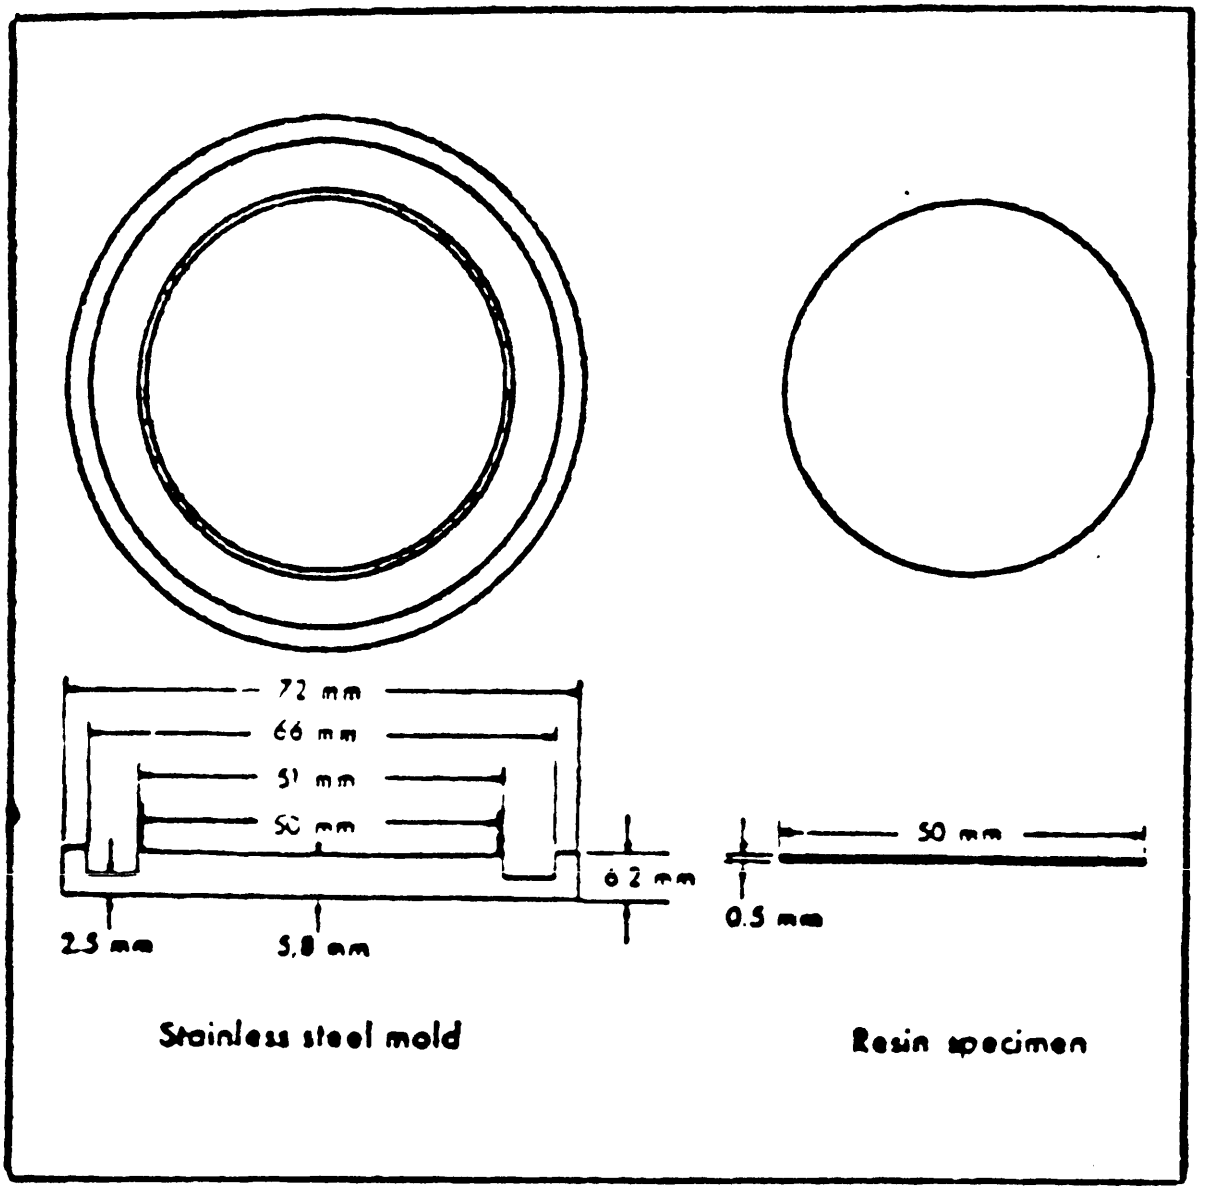


Figure 5. Details of Mold and Resin Specimen

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

4.4.10 Strain in compression. Test specimens shall be made by placing a ring 30 mm. inside diameter and 16 mm. high on a flat glass or metal plate and filling the ring slightly more than half full with the impression material. A mold of 12.7 mm. inside diameter, 25.4 mm. outside diameter, and 19 mm. high shall be placed immediately inside the ring and forced into the material until the mold touches the plate and the material has exuded onto the top of the mold. A flat glass or metal plate shall be pressed on the top of the mold to remove excess material. After the initial 15-minute set, the specimens shall be subjected to a 200 grams per square centimeter (g/cm^2) load for 30 seconds using a suitable instrument (see figure 3). The specimen shall then be measured and this measurement shall be considered the maximum strain in compression. Thirty minutes after the start of mix (15 minutes after the load has been applied), the specimen shall be measured and compared with the original height (19 mm. shall be considered the original height). The ratio of this measurement with the original height shall be considered the percentage of recovery.

4.4.11 Weight loss. The weight loss test shall be made in duplicate on disks 50 $\pm$ 1 mm. in diameter and 0.5 $\pm$ 0.1 mm. thick (see figure 4). These specimens shall be made in a stainless steel die (see figure 4). The gypsum in the shallow half of the flask shall be poured against a glass plate to obtain a smooth plane surface. Trial packing shall be conducted with a sheet of polyethylene used as a separator. Before final closure of the flask, a sheet of tin foil shall be substituted for the polyethylene. All surfaces of the disk shall be smooth and the top and bottom shall be flat. Test shall be conducted under uniform atmospheric conditions of 23 $\pm$ 2°C. and 50 $\pm$ 10% relative humidity. The specimens shall be removed from the dies 15 minutes from the start of mix and weighed on a Mettler type balance which has an accuracy of 10 milligrams (mg.). This reading is recorded as the original weight. The specimens shall be weighed again in 45 minutes, and percentage loss in weight calculated.

4.4.12 Amount of material in unit container. A single mix of material shall be prepared using the powder and liquid measures provided by the manufacturer, and the resulting volume (bulk displacement) measured to the nearest 0.1 ml. The number of impressions shall be calculated for a unit of issue using the bulk displacement value obtained.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the currentversion before use.

4.4.13 Dimensional accuracy. The material shall be tested for dimensional accuracy using the test block shown in figure 1. An impression tray 2 millimeters larger in all dimensions than the steel test block shall be constructed of self-curing acrylic tray resin. A standard mix of the impression material shall be prepared and placed in the impression tray. Two minutes from the start of mix, the impression tray shall be placed over the test block. The test block and tray shall be placed in a water bath at 37° ± 1°C. Fifteen minutes from the start of mix, the test block and tray shall be removed from the water bath and the tray shall be separated from the test block. A stone cast shall be poured immediately on the impression. To determine the dimensional accuracy of the material, the distance of the two "F" lines on the test block shall be measured and compared with the distance of the "F" lines reproduced on the stone cast. A suitable microscope shall be used to take the measurements. The difference between the measurements made of the "F" lines on the test block and the lines reproduced on the stone cast represents the dimensional accuracy of the material.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.2 Unit package. One bottle of liquid, one bottle of powder, one bottle of lubricating medium, two measuring vials or cups, and a mixing vessel or disposable cups, as specified, shall be packaged in a box conforming to PPP-B-636, type CF, class domestic; PPP-B-566, or PPP-B-676. Box design shall include suitable interior fittings or shall contain sufficient cushioning material to insure against shifting or damage to the contents. Closure shall be as specified in the applicable box specification. As specified in 3.5, instructions for use shall be inserted in each unit package.

5.1.2 Level C. The level C preservation for this item shall conform to the MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.1).

5.2.1 Level A. Six unit packages shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type; PPP-B-621, class 2; PPP-B-636; type CF, class weather-resistant. Closure and strapping shall be as specified in the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall be as specified in the liner specification. Case liner shall not be required for fiberboard boxes. Fiberboard boxes shall be waterproofed as specified in PPP-B-636.

5.2.2 Level B. Six unit packages shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type, PPP-B-621, class 1 or PPP-B-636, class domestic. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. Six unit packages shall be packed in accordance with the requirements of MIL-STD-794 for level C.

5.2.4 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which insure safe delivery to destination.

5.2.5 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantity for shipment to one destination exceeds250 lbs (excluding the pallet) or 20 cubic feet. Loads shall be unitized as specified in MIL-STD-147, on Type IV or Type V 4-way entry pallets. Pallet shall have a length of 40 inches and a width of 48 inches. pallet loads, including the pallet, shall not exceed 54 inches in height, 40 inches in length and 48 inchs width. Quantity for shipment to one destination of less than 250 lbs or 20 cubic feet need not be palletized.

5.2.4.1 Levels A and B. Components, packed as specified in 5.2.1 and 5.2.2, shall be unitized on pallets as specified in 5.2.5.

5.2.4.2 Level C. Components, packed as specified in 5.2.3, shall be unitized as specified in MIL-STD-794.

5.3 Marking.

5.3.1 Unit package. Each unit pack shall be marked in accordance with the requirements of the Federal Food, Drug and Cosmetic Act and regulations promulgated thereunder, and as specified in MIL-STD-129. Marking shall include the contract or purchase order no., lot (control) no., name of contractor, date of manufacture in lieu of date packed, and the legend: "STORE AT CONTROLLED ROOM TEMPERATURE 15° - 30°C (59° - 86°F)" or similar commercial legend.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

5.3.2 Levels A, B, and C. Each exterior container and unitized load shall be marked as specified in MIL-STD-129. Marking shall include the lot (control) no., date of manufacture in lieu of date packed and the legend: "STORE AT CONTROLLED ROOM TEMPERATURE 15° - 30°C (59° - 86°F)" or similar commercial legend.

5.4 General.

5.4.1 Exterior containers. Exterior containers (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.3.

6. NOTES

6.1 Ordering data.

6.1.1 Acquistion requirements. Acquistion documents should specify the following:

(a) Title, number, and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 National Stock Number (NSN) coverage. This specification covers the following item appearing in the Federal Supply Catalog:

Stock Number	Item Identification
6520-00-104-7617	IMPRESSION MATERIAL, DENTAL, Tissue Conditioner Type.

6.3 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Military requirements.

6.4 Subject term (key word) listing:

Impression Material
Tissue Conditioner
Methacrylate Resin

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

Military Interests:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD - MB

Agent:

DLA-DM

Review activities:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activities:
VA-OSS
PHS
FDA-MPQAS

47383

Project No. 6520-1850

Location: NCR Disk #1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:43Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:43Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
MIL-I-36993A	IMPRESSION, MATERIAL, DENTAL

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil – Downloaded: 2025-10-21T09:43Z
Check the source to verify that this is the current version before use.