A-A-50860A
24 March 1989
SUPERSEDING
A-A-50860
24 January 1983

COMMERCIAL ITEM DESCRIPTION

CUSHION, RING, INFLATABLE

Plastic

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Interim Federal Specification L-C-001804 which is cancelled.

This Commercial Item Description covers an oval, or circular, inflatable ring cushion suitable for patients who experience painful pressure when they are in the sitting or reclining position.

Salient characteristics:

The inflatable ring cushion shall be a vinyl plastic cushion ring with embossed surface suitable for use by medical patients who experience painful pressure when in the sitting or reclining position. The cushion shall be designed to provide circumferential support in rectal and adjacent areas.

The cushion, if oval, shall be 16 inches plus or minus 1 inch in length by 14 inches plus or minus 1 inch in width. The inside hole cut-out shall be 7 inches plus or minus 1 inch in length by 5 inches plus or minus 1 inch in width. The design of the oval cushion shall be similar to the cushion shown in figure 1. The cushion, if round, shall have a 16 inch plus or minus 1 inch outside diameter with a 6 inch plus or minus 1 inch diameter inside hole cut-out.

The vinyl plastic sheeting thickness shall be 0.017 inch plus or minus .002 inch (single thickness). The vinyl shall not be compounded with any known skin sensitizers or irritants. The vinyl sheets shall be sealed or bonded, by dielectric welding, forming an airtight product. The seals shall be free of wrinkles or bunching.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

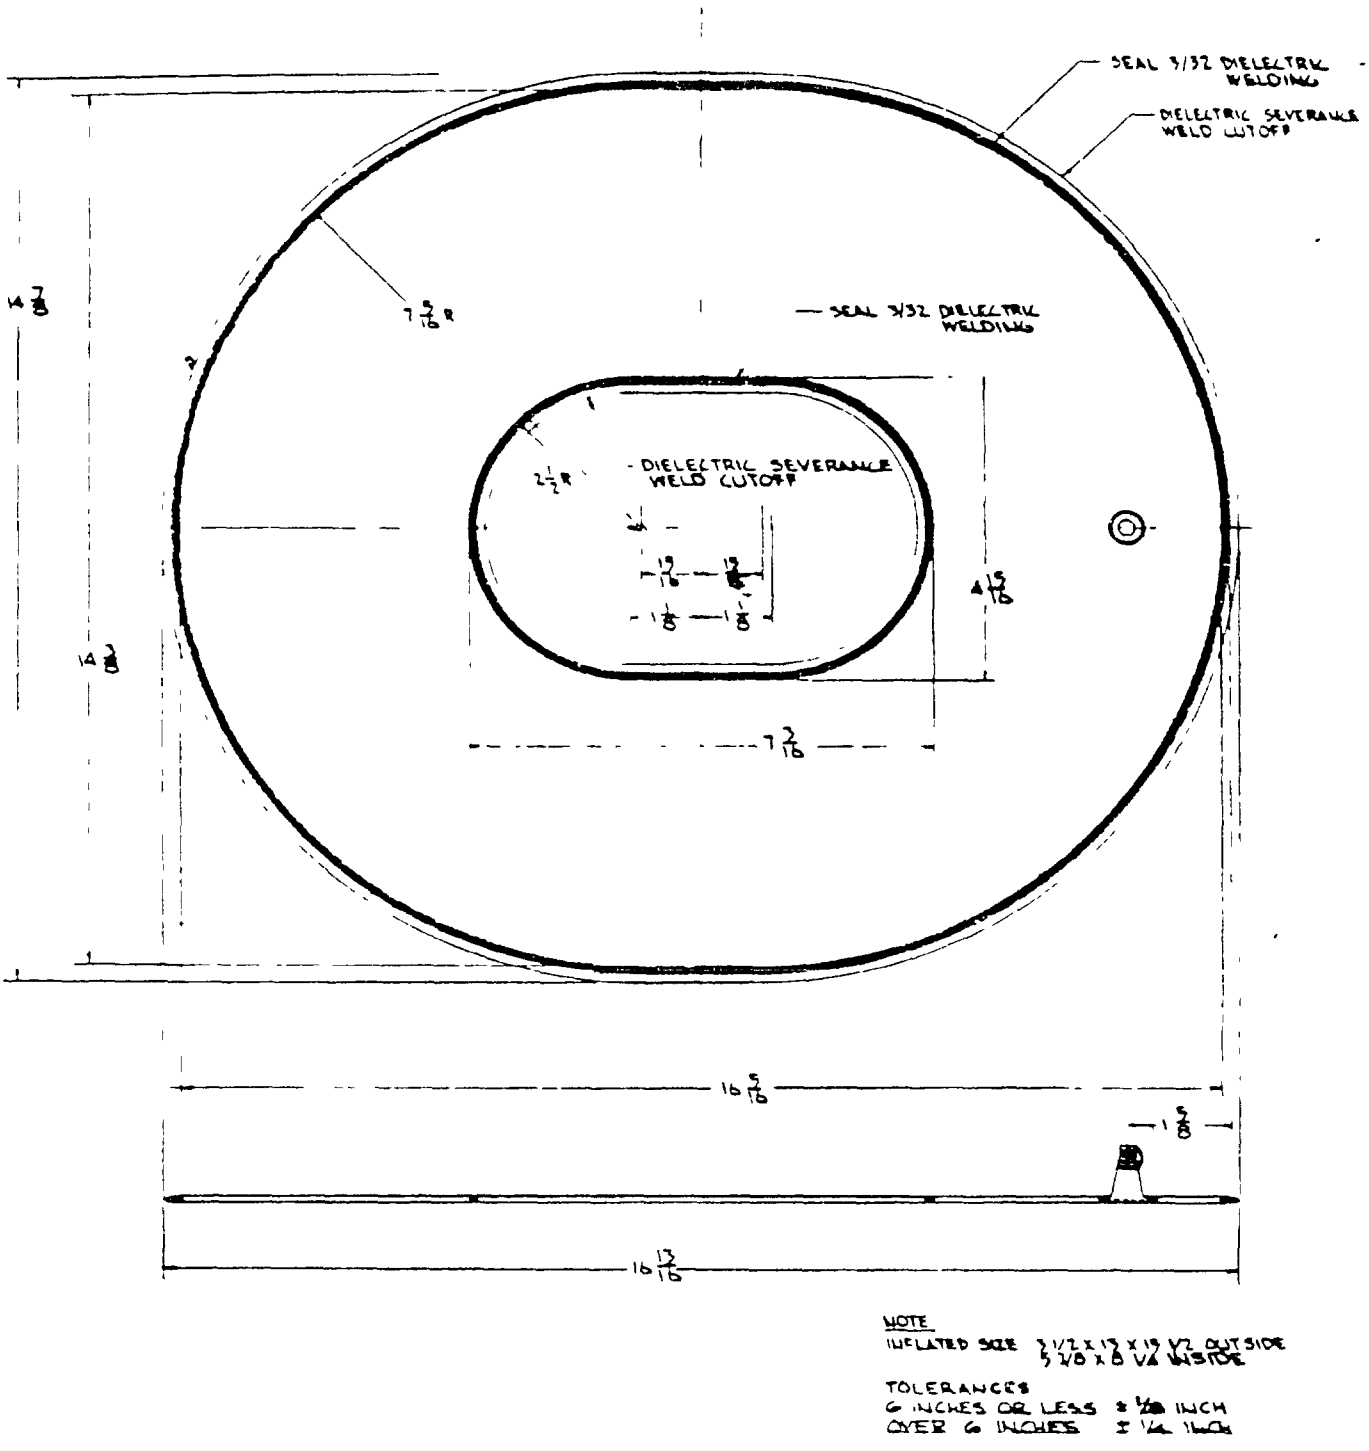


FIGURE 1. Inflatable ring cushion

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

The cushion shall be equipped with a retractable check-type valve having an integral plug closure. The retractable valve shall be heat sealed to the cushion body in a location suitable for inflation purposes and shall easily close and roll flush into the inflated cushion to safegard against accidental deflation or patient injury.

The cushion shall be capable of being cleaned by washing with soap and water.

The cushion shall be free of cuts, cracks, tears, pin holes, patches, or imbedded foreign matter. It shall be free of dirt, grease, oil, or loose foreign matter.

The cushion, when fully inflated, shall support the equivalent of a 200 pound seated adult for a minimum of eight hours without significant loss of air.

Each ring shall be individually packaged in a polyethylene bag closed with a piece of pressure sensitive adhesive tape.

Workmanship. The inflatable ring cushion shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing twelve cushions, individually packaged, as specified, constitutes one unit. Each cushion shall be packaged in a plastic bag and closed to prevent accidental opening.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one inflatable ring cushion as specified in this description.

Defects.

Cushion is not complete with all components.

Cushion is not fabricated from embossed vinyl plastic.

Vinyl plastic is not 0.017 inch plus or minus .002 inch thick.

Cushion is not individually packaged in a polyethylene bag closed with a piece of pressure sensitive adhesive tape.

Vinyl sheeting is not free of cuts, cracks, or tears.

Cushion seams are not completely heat sealed.

Vinyl sheeting is not free of pin holes, patches, or imbedded foreign matter.

Heat seals are not free of wrinkles or bunching.

Vinyl sheeting is not free of dirt, grease, oil, or loose foreign matter.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one inflatable ring cushion.

a. First article. Where a first article sample is required, all tests shall be performed on that unit.

b. Acceptance testing. When a first article sample has not been required, one unit shall be subjected to the performance test specified herein. If a test article sample has successfully passed all tests, performance test shall not be required at acceptance.

Tests

Air Tightness, A completely inflated ring cushion with the valve closed shall be completely submerged in water for a minimum of one minute. Any evidence of air bubble formation from air leaks through the cushion body shall constitute a defect.

Bursting Strength. An evenly distributed load of 300 pounds shall be suddenly applied to the fully inflated cushion. From initial contact to full load shall not exceed half a second. Bursting of a cushion seam shall constitute a defect.

Leakage. An evenly distributed load of 300 pounds shall be applied for a minimum of 8 continuous hours. Any evidence of leakage shall constitute a defect.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6530-00-444-3375

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6530-2018

Location: CID/CUSHION/H13-32

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
-A-50860A	CUSION, RING, INFLATABLE, Plastic

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street City State ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *Last First MI* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.