A-A-50881A
28 October 1985

COMMERCIAL ITEM DESCRIPTION

PAD, DENTAL RUBBER DAM

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers pads used for protective purposes during dental procedures.

Size 1 - Holder Size.
Size 2 - Frame Size.

Salient characteristics:

Description. The size 1 rubber dam pad shall be for use with a strap holder and the size 2 pad shall be for use with all dam frames. The pad shall be suitable for protecting the facial skin from irritation by the rubber dam and from saliva, water, and perspiration during dental procedures.

Material. The pads shall be fabricated of soft, calendered, nonwoven fabric. The material shall be absorbant and shall have good wet strength to resist tearing when wet.

Design and dimensions. The pads shall be trapezoidal in shape with rounded corners and cut outs for the nose and mouth. The pads shall be symmetric about a plane through the vertical centerline. The pads shall be embossed on both sides. The dimensions of the pads shall be as shown in figure 1.

Tensile strength. The material shall have tensile strengths (dry) of 10 pounds-in the machine direction and 1.4 pounds in the cross direction, with a tolerance of ± 20 percent.

Weight. Fifty pads shall weigh a minimum of 125 grams for size 1 and 56.5 grams for size 2 pads.

Workmanship. Pads shall be free from holes, tears and defects which detract from their appearance or impair their serviceability. Pads shall be furnished clean and ready for use.


Unit. Package (PG). One package containing fifty pads, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.
Source: https://assist.dla.mil - Downloaded: 2026-10-20T08:48Z
Check the source to verify that this is the current version before use.

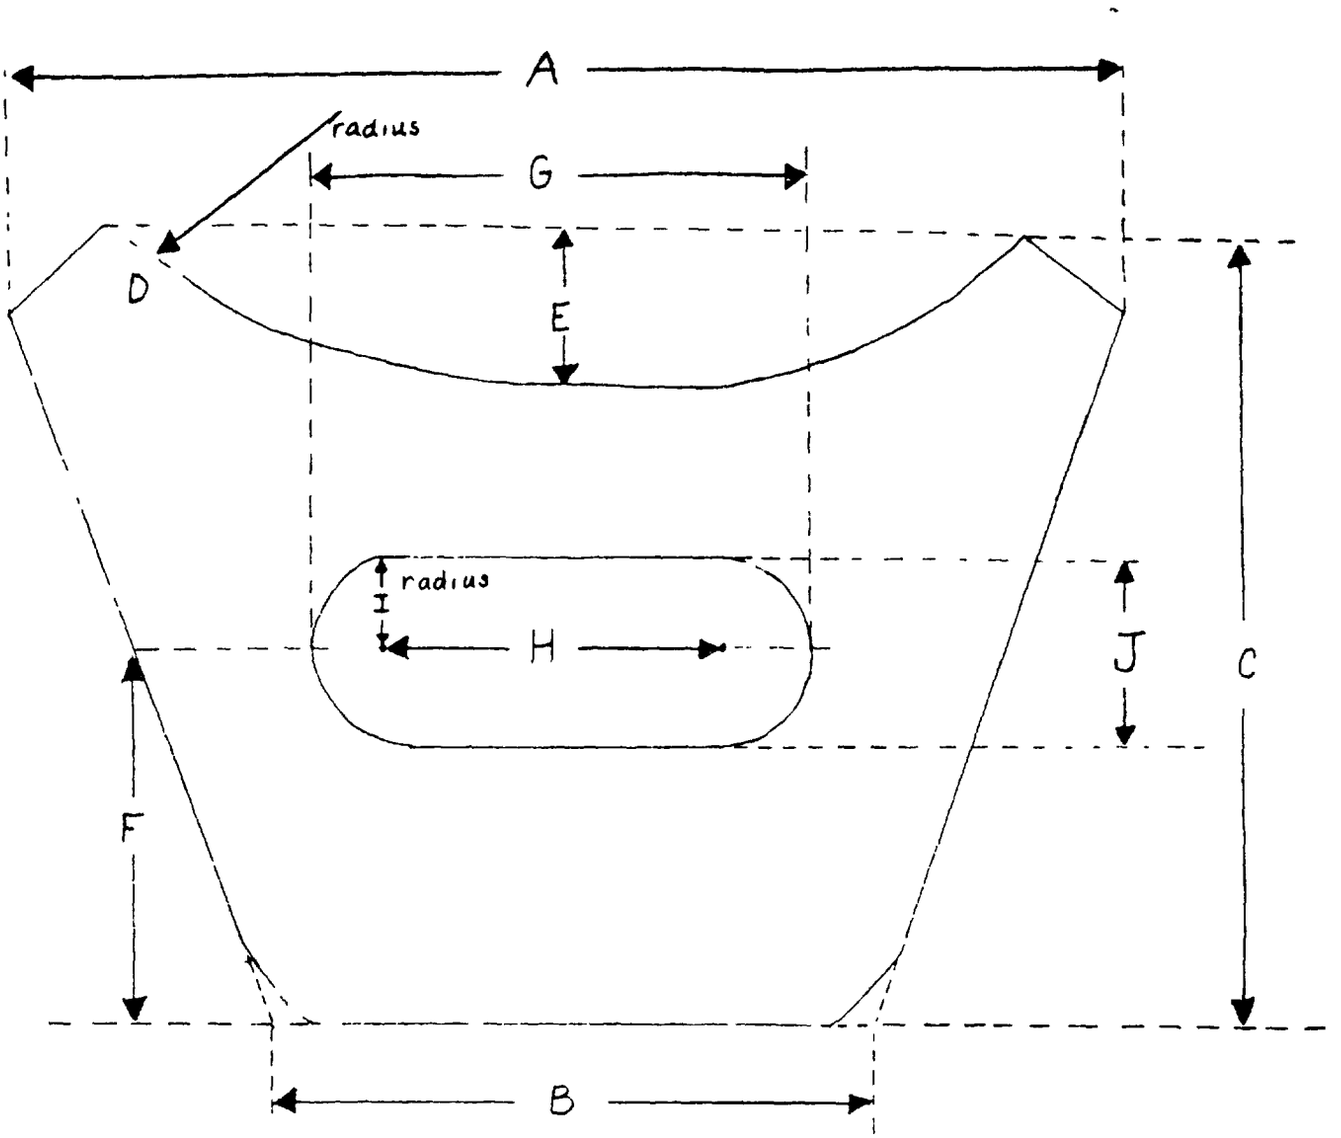

SIZE	DIMENSIONS									
	A	B	C	D	E	F ± 3/32	G ± 3/16	H ± 1/16	I ± 1/16	J ± 1/8
1-HOLDER	11 3/8	8	6	4 1/4	1 15/16	2 5/8	3	1 9/16	23/32	1 7/16
2-FRAME	7	3 15/16	5	4 11/32	1	2 17/32	2 27/32	1 13/32	23/32	1 7/16

NOTES:
1. All dimensions are in inches.
2. Unless otherwise specified, tolerance is ± 1/4 inch.

Figure 1. - PAD, DENTAL RUBBER DAM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one rubber dam pad. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5 except for dimensions which shall be conducted at inspection level S-4, AQL 4.0. Sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 4.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers are covered by this document:

Stock Number	Item Identification	Designation
6520-00-542-2750	PAD, DENTAL RUBBER DAM, 50s	Size 1
6520-01-158-4351	PAD, DENTAL RUBBER DAM, 50s	Size 2

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

51795

Project No. 6520-1851

Location S2-10-8

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.