FEDERAL SPECIFICATION

APPLICATOR, METAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers ear, nose, and throat applicators suitable for application of medication.

1.2 Classification.

1.2.1 *Types and styles.*—Applicators shall be of the following types and styles, as specified (see 6.1):

Type I.—Ear applicator.
  Style 1.—Triangular tip (Allen).
  Style 2.—Twisted tip.
Type II.—Nasal applicator (Uebe, triangular tip).
Type III.—Pharyngeal applicator (spiral tip).
  Style 1.—Curved.
  Style 2.—Straight.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

GG-I-526—Instruments, Dental and Surgical: General Specifications.
QQ-W-339 — Wire; Copper, Medium-Hard Drawn.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specification:

MIL-P-12902 — Packaging of Surgical, Dental and Veterinary Instruments, Diagnostic Equipment, and Related Items.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 — Marking for Shipment and Storage.

(Copies of Military Specifications and Standards, required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

3. REQUIREMENTS

3.1 Material.—Applicators shall be fabricated of classes and compositions, specified in table I, in accordance with Federal Specification GG–I–526 and as otherwise specified.

3.2 Style, design, and dimensions.—Applicators shall be suitable for application of medication and as hereinafter specified.

3.2.1 *Type I (ear applicator).*—Type I, styles 1 and 2, shall be an ear applicator in accordance with figure 1. Style 1 shall have a triangular tip (Allen type or equal), and style 2 shall have a twisted tip.

3.2.2 *Type II (nasal applicator).*—Type II shall be a nasal applicator with triangular tip (Uebe design or equal), and shall be in accordance with figure 2.

3.2.3 *Type III (pharyngeal applicator).*—Type III shall be a pharyngeal applicator, flexible, with spiral end. Style 1 applicator shall be in accordance with figure 3, and style

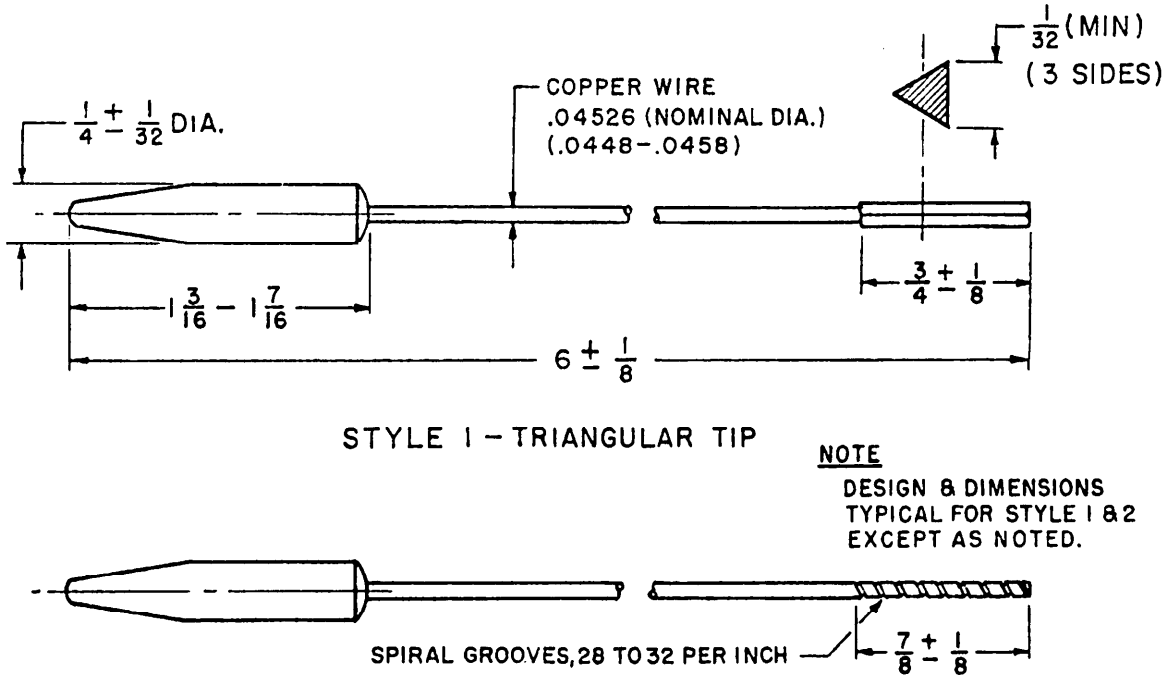


FIGURE 1.—Type I (ear applicators).

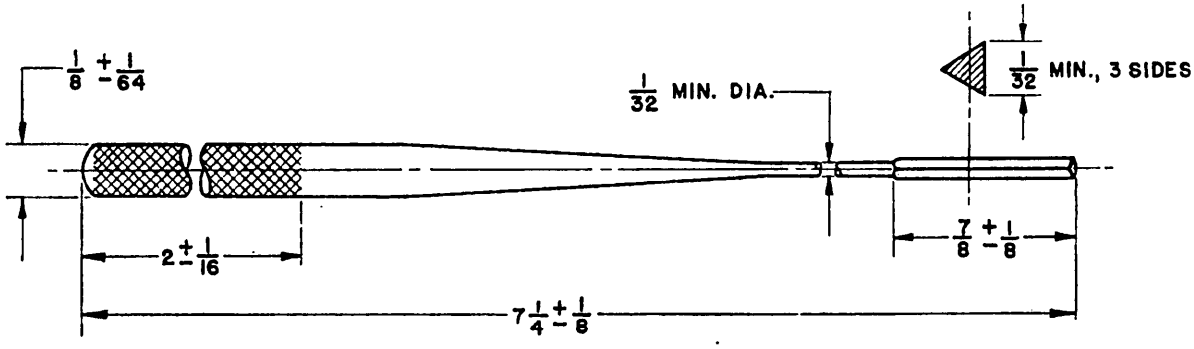


FIGURE 2.—Type II (nasal applicator).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

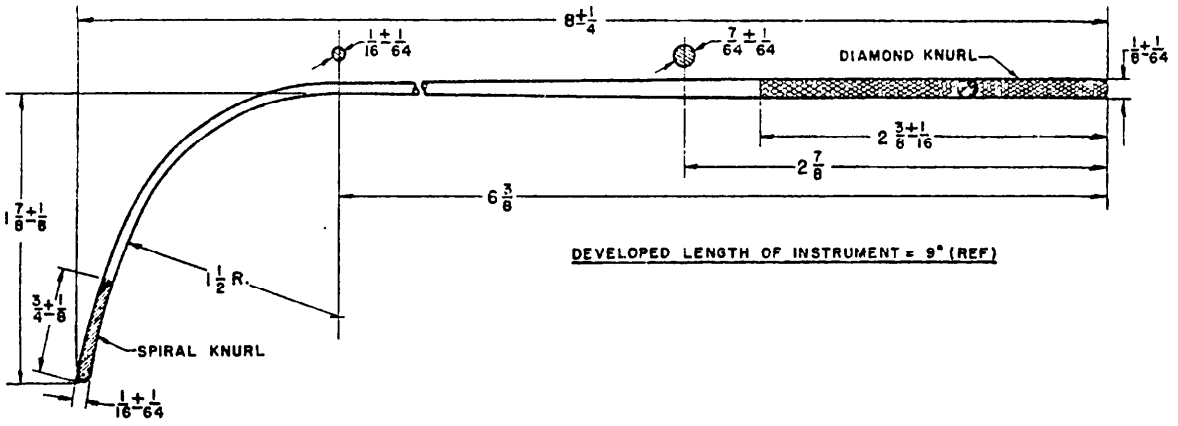


FIGURE 3.—Type III (pharyngeal applicator, style 1).

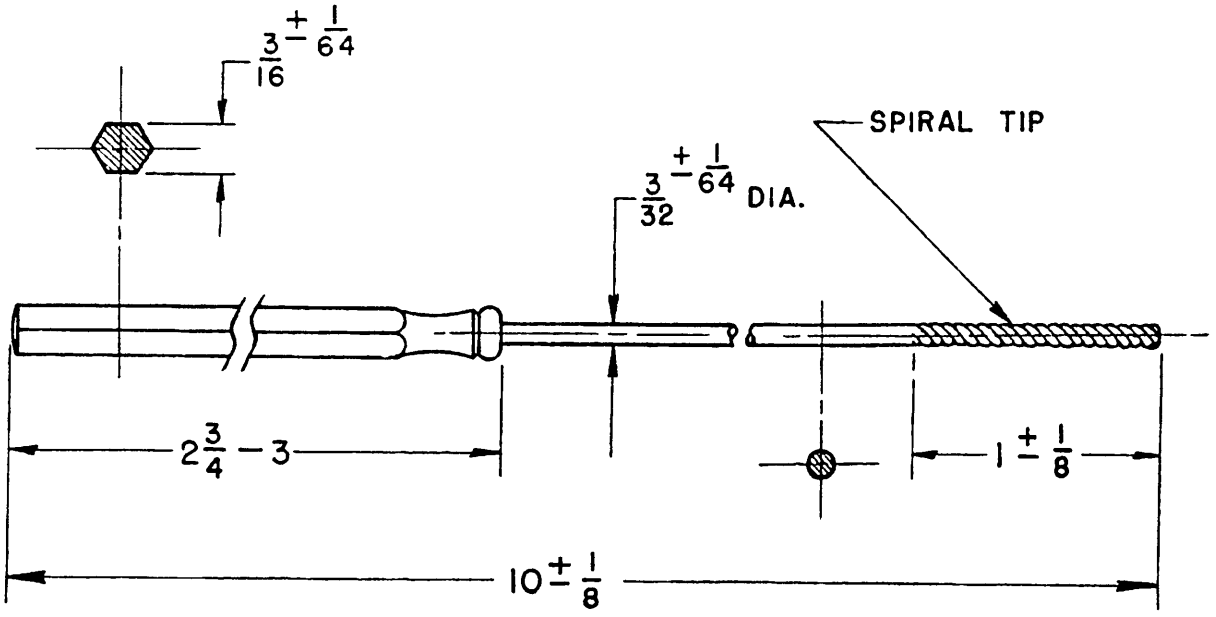


FIGURE 4.—Type III (pharyngeal applicator, style 2).

2 applicator shall be in accordance with figure 4.

3.3 Finish.—Type II, nasal applicator, shall have a mirror finish and all other applicators shall have finishes suitable for the purpose intended, in accordance with the requirements of Federal Specification GG–I–526.

3.4 Additional requirements. — Except as specified herein, the applicators shall comply with applicable requirements and tests of Federal Specification GG–I–526. The requirements of that specification for micrometallographic examination shall not apply.

3.5 Workmanship.—Workmanship shall be first class throughout. Applicators shall be free from defects which detract from their appearance or which may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Supplier responsibilities for inspection.—Unless otherwise specified herein, the supplier is responsible for the performance of all inspection requirements prior to submission for Government inspection and acceptance. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. Inspection records of the examinations and tests shall be kept complete and available to the Government as specified in the contract or order.

4.1.1 Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.*—When available, certificates of quality supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 *For examination.*—Sampling for examination shall be conducted in accordance with Military Standard MIL–STD–105.

4.2.2 *For tests.*—Sampling for tests shall be conducted in accordance with Military Standard MIL–STD–105 (see table II of this specification).

4.2.3 *Raw materials.*—A sufficient quantity of each lot of each metal used in the construction of the applicators shall be selected for chemical analysis.

4.2.4 Where possible, the same sample units shall be used for the determination of two or more test characteristics.

4.3 Examination.—The applicators shall be examined to determine compliance with all requirements contained in this specification.

4.4 Tests. — Tests shall be conducted, as necessary, to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

For civil agency procurement the levels of preservation, packaging, and packing protec-

TABLE I.

Type	Style	Component	Material	Specification designation (GG–I–526)
I (ear)	1 and 2	Stem	Copper	Class 4, composition P (except shall not be plated) and shall meet physical requirements of Federal Specification QQ–W–339 (except for mass resistivity)
		Handle	Aluminum alloy	
II (nasal)	--	Entire instrument	Corrosion-resisting steel	Class 2, composition K or G(c)
III (pharyngeal)	1	Entire instrument	Copper, nickel plated	Class 4, composition P, shall be nickel plated only, salt spray test requirement shall not apply
	2	Stem	Corrosion-resisting steel	Class 2, composition H
		Handle	Corrosion-resisting steel or brass	Class 2, composition H or class 4, composition N

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

TABLE II.—*Requirement applicable to individual unit only*

Component	Characteristic	Req.	Test procedure	Unit of product	Insp. level	AQL
Applicator	Hardness	GG–I–526	GG–I–526	1–Applicator	L3*	**
	Copper sulfate test	GG–I–526	GG–I–526	1–Applicator	L3*	**
	Boil test	GG–I–526	GG–I–526	1–Applicator	L3*	**
	Thickness of coating	GG–I–526	GG–I–526	1–Applicator	L3*	**

*A minimum of three units shall be tested regardless of lot size.
**Acceptance number shall be zero for all sample sizes.

tion used are defined in Federal Standard No. 102.

5.1 Packaging and packing.

5.1.1 *Unit of issue.*—One applicator, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units indicated in table III shall be packaged in each unit, intermediate and exterior container, as applicable for the required level of protection specified in procurement document.

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Type I applicators.*—Packaging and packing shall conform to Military Specification MIL–P–12902, Procedure Code No. 36.

TABLE III.—*Packaging quantities*

Unit package	Intermediate package	Exterior container
1 unit	12 units	576 units

5.1.3.2 *Type II or type III applicators.* — Packaging and packing shall conform to Military Specification MIL–P–12902, Procedure Code No. 30.

5.1.4 *Level B.*

5.1.4.1 *Type I applicators.*—Packaging and packing shall conform to Military Specification MIL–P–12902, Procedure Code No. 24.

5.1.4.2 *Type II or type III applicators.*—Packaging and packing shall conform to Military Specification MIL–P–12902, Procedure Code No. 20.

5.1.5 *Level C.* — The subject commodity shall be packaged and packed according to the supplier's commercial domestic practice to assure acceptance by the carrier and safe delivery to destination at the lowest transportation rate or rating. Containers shall comply with carrier rules and regulations applicable to the mode of transportation without assessment of penalty charges for improper packing.

5.1.6 *Level D.* — The subject commodity shall be packaged and packed according to the supplier's commercial export practice to assure acceptance by the carrier and safe delivery to destination at the lowest transportation rate or rating. Containers shall comply with carrier rules and regulations applicable to the mode of transportation without assessment of penalty charges for improper packing.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the current version before use.

5.2 **Marking.**

5.2.1 *Civil agencies.*—In addition to any special marking required by the contract or order, marking shall be in accordance with Federal Standard No. 123.

5.2.2 *Military agencies.*

5.2.2.1 *Interior packages.*—Each unit package and each intermediate container shall be marked in accordance with Military Specification MIL–P–12902 except that the ASMPA stock number will not be required.

5.2.2.2 *Exterior container.*—Exterior container shall be marked in accordance with Military Standard MIL–STD–129, except that 6.2(c), 6.2(d), 6.5, and 7.5.1 shall not be applicable. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 **Ordering data.** — Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Types and styles required (see 1.2).

(*c*) Selection of applicable level of preparation (see part 5).

(1) Level B packaging is intended to provide economical but limited protection, and should be specified only when it is determined the applicators will be held in covered storage not more than 12 months from date of initial packaging.

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 **Transportation description.**—Transportation description applicable to this item is:

Surgical Instruments NOIBN
Carload minimum weight 10,000 pounds subject to Rule 34 of the Uniform Freight Classification.
Truckload minimum weight 10,000 pounds subject to Rule 34 of National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

CUSTODIANS:
Army—Army Medical Service
Navy—Bureau of Medicine and Surgery
Air Force.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.