FEDERAL SPECIFICATION

CABINETS, INSTRUMENT, MEDICAL

This specification was approved on the above date by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. CLASSIFICATION

1.1 Types, classes, and sizes.—The instrument cabinets covered by this specification shall be of the following types, classes, and sizes, as specified:

Type I.—Instrument cabinets

Class 1.—Two-door type
Size 30.—30 inches in width
Size 36.—36 inches in width
Class 2.—Single-door type
Size 25.—25 inches in width

Type II.—Instrument and dressing cabinets

Type III. — Instrument, dressing, and medicine cabinets

1.2 Grades.—The instrument cabinets shall be of the following grades, as specified:

Grade A.—Metal parts of corrosion-resisting steel
Grade B.—Metal parts of carbon steel

2. APPLICABLE SPECIFICATIONS

2.1 The following Federal Specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

DD-G-451—Glass, Flat and Corrugated, for Glazing, Mirrors, and Other Uses.
FF-C-81—Casters; Metal-Chair.
QQ-M-151—Metals; General Specification for Inspection of.
QQ-S-636—Steel; Carbon (Low-Carbon), Sheets and Strips.
QQ-S-766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.
TT-E-491—Enamel; Gloss, Synthetic (for Metal and Wood Hospital Furniture).
TT-P-659 — Primer-Surfacer; Synthetic, Tints and White (for Metal and Wood Hospital Furniture).

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application accompanied by money order, coupon or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C. Prices may be obtained from the Superintendent of Documents.)

2.2 Specifications applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Material.

3.1.1 *Glass.* — The glass shall conform to the applicable requirements of Specification DD-G-451 for type II, clear sheet glass of A quality and $\frac{1}{8}$ inch thickness.

3.1.2 *Carbon steel.*—The carbon steel shall conform to the requirements of Specification QQ-S-636; the thickness shall be as hereinafter specified with a permissible tolerance of plus or minus 0.005 inch.

3.1.3 *Corrosion-resisting steel.*—The corrosion-resisting steel shall conform to the applicable requirements of Specification QQ-S-766 for class 1 or 2. The thickness shall be as hereinafter specified with a permissible tolerance of plus or minus 0.004 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

3.2 Construction.—The cabinets shall be substantially and rigidly constructed. They shall be suitably reinforced and assembled with all parts in proper alignment and all doors, latches, and locks shall function properly. All seams and joints shall be welded, ground smooth, and filled without ridge or crevice. The corners and edges shall be rounded. The seams shall be interlocking. The compartments shall be essentially dustproof.

3.3 Top.—The top of each cabinet shall be of sheet steel 0.050 inch in thickness; shall have an integrally rolled edge approximately ½ inch in diameter on front and sides; and shall fit snugly over outside of the body. The corners shall be welded and ground smooth. The top shall be welded to the body on all four sides.

3.4 Glass-panelled doors. — The glass-panelled door frames shall be of double-shell design constructed of sheet steel 0.050 inch in thickness. The outer shell shall be die-formed to an approximate $\frac{3}{8}$-inch-radius cove on one end, then formed integrally backward in Z-formation to accommodate the rubber-cushioned glass panels. The inner shell shall be properly formed and reinforced to secure the glass panels firmly in place, and suitably arranged to permit easy replacement of panels. The doors shall fit in the rabbeted frame of the cabinet, closing flush with the front surface against suitable rubber bumpers. Cabinet frames and door frames shall be notched to receive the hinges so that only the butts are visible from the outside or fully concealed.

3.5 Front frame. — The top front filler member, front vertical edges of the cabinet ends, and the front edge of the cabinet bottom shall be properly formed to make a rabbeted framing for flush fitting doors.

3.6 Glass panels. — The side and door panels of glass shall be of $\frac{1}{8}$-inch-thick clear sheet glass. They shall be fully cushioned in rubber channels, held in place by properly formed and reinforced retaining members constructed of sheet steel 0.050 inch thick, and suitably arranged to permit easy replacement of panels.

3.7 Glass shelves.—The glass shelves shall be of clear sheet glass $\frac{1}{4}$ inch in thickness. They shall be mounted on heavy-gage clip-type brackets, fitting adjustable stripping which shall permit adjustment every ½ inch in height. All edges of shelves shall be ground smooth and polished.

3.8 Bottom.—The bottom of the cabinets shall be of 0.050-inch-thick sheet steel, having front top edge suitably formed to make a rabbeted recess for receiving the door in flush position. The front edge of the recess shall be flanged downward approximately 1½ inches and hemmed. The back and sides of the cabinet bottom shall be flanged upward approximately 1 inch and suitably welded to the body.

3.9 Back.—The back of the cabinets shall be of sheet steel 0.050 inch in thickness, having the top edge flanged inward at an angle of 90°.

3.10 Door hinges.—The door hinges shall be semi-concealed, approximately 5½ inches in height, fast-pin, five-knuckle, butt type, constructed of heavy wrought bronze or brass of suitable width and shape for application of the cabinet doors. Hinges shall be fastened to the cabinet by machine screws, nuts, and lock washers, and screwed to reinforcing angles welded to door filler, or to the glass-panelled door frame as applicable.

3.11 Latches.—The latches shall be heavily constructed using either $\frac{5}{8}$-inch by $\frac{1}{4}$-inch bar stock, or $\frac{1}{4}$-inch diameter bar rod for the latching rods. Latches and rods shall be firmly secured in place and shall be constructed of the same material as the cabinet.

3.12 Locks.—Each cabinet shall be equipped with at least one locked compartment. The lock shall be of the pin-tumbler, grooved-key,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

cabinet type that is integral with the door pull. Two keys of noncorrosive metal shall be furnished with each cabinet (or lock if appropriate), no two cabinets being keyed alike.

3.13 Base.—Unless otherwise specified, the cabinet shall have four offset-type legs permanently attached to the bottom of the cabinet. The legs shall be pressed or die-formed, approximately 6 inches in height, and constructed of sheet steel 0.109 inch in thickness. They shall be formed with ample offsets for proper support of the cabinet, and shall be fitted with a suitable welded socket or integral device welded to inside of leg and extending full height of leg for additional support for proper attachment of an adjustable glide or caster. Surfaces of the cabinet shall be properly reinforced where legs are attached. The leg assembly shall be sturdy and capable of withstanding strain caused by moving the cabinet in any direction.

3.13.1 When specified in the invitation for bids, the cabinet shall be furnished with a four-leg or enclosed (as specified) detachable base. The base shall be sturdy and capable of withstanding strain caused by moving the cabinet in any direction.

3.13.2 *Glides.*—Unless otherwise specified, the legs shall be fitted with screw- or socket-type adjustable glides approximately 2 inches in diameter and constructed of heavy gage corrosion-resisting steel or brass heavily chromium-plated over nickel. Glides shall not extend beyond the back line of the cabinet.

3.13.3 *Casters.*—When specified in the invitation for bids, casters shall be furnished in lieu of glides. The casters shall be of the swivel type and shall conform to the applicable requirements of Specification FF-C-81 for type I, size A.

3.13.4 *Make-weight.* — A make-weight of lead or similar material shall be fastened underneath the bottom at the rear of the cabinet and shall be heavy enough to prevent inadvertent tipping of cabinet while empty and with doors open.

3.14 Identification marking. — Each cabinet shall be permanently and legibly marked with the name or registered trade-mark of the manufacturer.

3.15 Type I.—Type I instrument cabinets shall consist of a single storage compartment with glass-panelled sides and doors, and six removable glass shelves. (See fig. 1.)

3.15.1 *Class 1.*—Class 1 cabinets shall be constructed with two glass-panelled doors. The designation of right and left in reference to the doors is determined by facing the front of the cabinet. The two doors shall each open in the center of the cabinet. The right-hand active leaf of the doors shall be fitted with a 3-way latch engaging at top, side, and bottom simultaneously, operated from the outside by a suitable knob or handle. The left-hand or inactive leaf shall be fitted inside with a 2-way latch operated from the inside of the cabinet, engaging at top and bottom. The knob or handle on the active leaf shall be fitted with an integral lock. The knob or handle on the left inactive leaf shall match that of the right-hand door, but without a lock.

3.15.1.1 *Size 30.*—Size 30 cabinets shall be of the design shown in figure 1, type I. The dimensions over-all shall be approximately 30 inches wide, 16 inches deep, and 72 inches high.

3.15.1.2 *Size 36.*—Size 36 cabinets shall be of the design shown in figure 1, type I, except that the dimensions over-all shall be approximately 36 inches wide, 16 inches deep, and 72 inches high.

3.15.2 *Class 2.*—Class 2 cabinets shall be constructed with one glass-panelled door. The door shall be hung on three hinges and shall be fitted with a three-point lock (oper-

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

ated by one key at the center point), to lock at top, center, and bottom.

3.15.2.1 *Size 25.*—Size 25 cabinets shall be of the general design shown in figure 1, type I, except that they shall have a single right-hand door. The dimensions over-all shall be approximately 25 inches wide, 15 inches deep, and 70 inches high.

3.16 Type II.

3.16.1 *Design.*—Type II cabinets shall be of the general design shown in figure 1, type II, consisting of an upper and a lower storage compartment. The dimensions over-all shall be approximately 30 inches wide, 16 inches deep, and 60 inches high.

3.16.2 *Upper compartment.* — The upper compartment shall be not less than 30 inches high inside, with glass-panelled sides, one glass-panelled door, and three adjustable glass shelves.

3.16.3 *Lower compartment.* — The lower compartment shall be not less than 20 inches high inside, with all-metal sides, one all-metal door, and two removable metal shelves.

3.16.3.1 *Metal shelves.* — The all-metal shelves shall be of sheet steel 0.037-inch minimum thickness, with all edges turned down 1 inch and under ½ inch, forming a channel-shaped section. The corners shall be welded and ground smooth.

3.16.3.2 *Lower door.*—The lower door shall be of double-walled construction with the outer panel of sheet steel 0.037-inch minimum thickness, and the inner panel of sheet steel 0.031-inch minimum thickness. The door shall be filled with a sound-deadening material such as cellufoam or equivalent.

3.16.4 *Latch.*—Both the upper and lower compartment doors shall be fitted with a 3-way latch engaging at the top, side, and bottom simultaneously, and operated from the outside by a suitable knob or handle. The knob or handle on the upper door shall have an integral lock. The knob or handle on the lower door shall match that of the upper door but shall be without a lock.

3.17 Type III.

3.17.1 *Design.*— Type III cabinets shall be of the general design shown in figure 2, type III, consisting of an upper and lower section, with a distance of 12 inches between sections. The dimensions over-all shall be approximately 36 inches wide and 78 inches high. The designation of right and left in reference to the cabinet is determined by facing the front of the cabinet.

3.17.2 *Upper section.* — The upper section shall have glass-panelled sides, two glass-panelled doors, and three adjustable glass shelves. The dimensions over-all shall be approximately 36 inches wide, 8 inches deep, and 30 inches high.

3.17.2.1 *Doors.* — Each of the two upper doors shall open in the center of the cabinet. The right-hand door shall be fitted with a 3-way latch engaging at the top, side, and bottom simultaneously, and operated from the outside by a suitable knob or handle, and shall close against a strike welded to the back of the left door. The knob or handle on the right-hand door shall have an integral lock. The left door shall have a suitable catch to prevent it from swinging open and shall have a dummy handle of similar design to that on the right door.

3.17.2.2 *Narcotic locker.* — Unless otherwise specified, the upper unit shall be provided with a narcotic locker constructed of steel 0.050 inch in thickness, which shall be securely welded to the side, back, and base of the inside of the lower left-hand section. The door of the narcotic locker shall be of double-walled construction and shall fit into the rabbeted frame of the locker, closing flush with the seamlessly welded front surface. The locker frame shall be notched to receive the hinges so that only the butts are

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the currentversion before use.

visible from the outside. The narcotic locker shall be approximately 18 inches long, 9 inches high, and of such depth as to make a snug fit inside the cabinet.

3.17.2.2.1 *Latch.*—The door of the narcotic locker shall be equipped with a heavily constructed 3-way latch engaging at the top, side, and bottom simultaneously, and controlled by a door knob or handle. The handle shall have a pin-tumbler, grooved-key, cabinet-type lock that is integral with the door-pull. Two keys of noncorrodible metal shall be furnished with each lock. The narcotic locker and the cabinet shall not be keyed alike.

3.17.3 *Lower section.* — The lower section shall consist of a partitioned unit with a drawer compartment on the left side and a storage compartment on the right. The dimensions over-all shall be approximately 36 inches wide, 16 inches deep, and 30 inches high, with a counter-top height of 36 inches. The body shall be constructed of steel 0.050 inch thick, having top edges flanged inward at 90° and shall be suitably welded together. The entire lower section shall be covered by a finished top of 0.062-inch-thick steel. The front and side edges of the finished top shall be flanged downward not less than 1 inch and hemmed. The back of the top shall rise vertically to meet the upper section and return to the working surface where it shall be fully welded. The front facia shall be seamlessly welded. The bottom shall be constructed of 0.050-inch-thick sheet steel with the front edge suitably formed to provide a rabbeted recess for receiving the drawer and door in flush position. The front edge of the recess shall be flanged downward approximately 1½ inches and hemmed. The back and sides of the bottom shall be flanged upward 1 inch and welded to the body.

3.17.3.1 *Drawer compartment.*—The drawer compartment shall have three sheet-steel drawers of 0.037-inch minimum thickness, welded to box-type double-walled fronts of the same thickness which shall be fitted with chromium-plated brass or cast-aluminum handles. The double-walled drawer fronts shall be filled with sound-deadening material such as cellufoam or equivalent.

3.17.3.1.1 *Drawer slides.* — The drawers shall travel on sheet-steel slides 0.078 inch in thickness and approximately 2¼ inches high. The slides shall be welded to the drawer housing. The front of the slide shall have a roller bearing with a face not less than ¼ inch wide. Behind the roller bearing the slide shall be formed to provide a track approximately ⅝ inch wide by approximately ⅝ inch high, under which another roller bearing shall ride. This bearing shall be fastened to the back of the companion glide or Z-shaped member welded to each side of the drawer body.

3.17.3.1.2 *Fit.* — The drawer heads shall close against suitable rubber bumpers and shall fit flush with the front of the casing, resting in an integral rabbeted frame.

3.17.3.2 *Storage compartment.*

3.17.3.2.1 *Shelf.* — The storage compartment shall be furnished with one removable shelf of sheet steel 0.037-inch minimum thickness, with all edges turned down 1 inch and under ½ inch, forming a channel-shaped section. The corners shall be welded and ground smooth.

3.17.3.2.2 *Door.*—The storage compartment shall have a door of double-walled construction with the outer panel of sheet steel 0.037-inch minimum thickness, and the inner panel of sheet steel 0.031-inch minimum thickness. The door shall be filled with a sound-deadening material such as cellufoam or equivalent and shall fit flush in rabbeted frame again suitable rubber bumper. The door shall be fitted with a 3-way latch engaging at the top, side, and bottom simultaneously, and operated from the outside by a suitable knob or handle.

3.17.4 *Understructure.* — The upper compartment shall be firmly mounted on an angle

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the currentversion before use.

frame of the understructure and neatly fastened with screws, nuts, and lock washers. The understructure shall consist of a welded frame made of a length of drawn or formed steel angle approximately 1 inch by 1½ inches by 0.109 inch in thickness. A strut approximately 1 inch by ¼ inch shall be welded to the rear corners and square tubing approximately 1¼ inches on a side made of steel 0.062 inch in thickness shall be welded to the front corners. The understructure shall be of the same material composition as the cabinet. Struts shall be fastened to the finished top, splashback, and lower unit by means of screws, nuts, and lock washers, and the end posts shall be similarly fastened to lower cabinet top by means of threaded shoes welded into base of posts with bolts extending through the top.

3.18 Grades.

3.18.1 *Grade A.* — Grade A cabinets shall have metal work of corrosion-resisting steel. The exterior and interior shall be polished to a No. 4 finish without streaks, waves, or similar blemishes. Exterior back of cabinets may be finished in a No. 2 mill finish. Screws, nuts, and washers shall be of corrosion-resisting steel. All other hardware shall be brass, bronze, or steel, heavily chromium-plated over nickel with a satin finish.

3.18.2 *Grade B.*

3.18.2.1 *Metal.* — Grade B cabinets shall have metal work of carbon steel. For exposed surfaces such as doors, tops, sides, etc., it shall be either full-pickled, full cold-rolled, reannealed, stretcher-levelled and oiled steel, or hot-rolled steel with one pass of cold rolling and then annealed and pickled. For the unexposed parts such as bottoms and drawer bodies, the requirements shall be the same except that the steel may be single-pickled and the stretcher levelling may be omitted. The sheet steel shall be bright, smooth, of uniform gage, and free from blemishes. Commercial variations in flatness and thickness will be permitted along or across any one sheet. The steel shall be capable of being formed into the required shapes without fracture or near fracture. All hardware shall be brass, bronze, or steel, chromium-plated over nickel and shall have a bright, hard finish.

3.18.2.2 *Finish.*—All metal surfaces except those required to be unpainted for the proper operation of the particular part, shall be finished in white enamel, unless otherwise specified. Before finishing, all exposed welds and joints shall be buffed or otherwise smoothed. The parts shall be putty-glazed, baked, and then sprayed with a primer coat conforming to the requirements of Specification TT-P-659, followed by spraying with two coats of enamel conforming to the applicable requirements of Specification TT-E-491, class B. The parts shall be baked after each coat. The unpainted metal surfaces shall be finished with a suitable corrosion-resisting coating.

3.19 **Workmanship.** — The workmanship shall be first class throughout. The instrument cabinets shall be free from defects which detract from their appearance or which may impair their serviceability.

3.19.1 *Welding.*—Welding shall be durable and sound in every detail. Welding rods shall be of a composition similar to that of the welded members. Component members shall be carefully and properly aligned prior to welding into permanent position as a straight, rigid, and level assembly. All exposed welds shall be ground smooth to eliminate traces of pit marks and seams and shall be polished to blend with adjacent surfaces. Spot welds on exposed surfaces shall show no objectionable pits or extrusions. When surface of metal is defaced in fabrication, it shall be filed or ground smooth and, when necessary, filled to prevent unsightly blemishes on the finished surfaces. Spot welds shall be spaced not more than 2 inches on centers, tightly fused, and of sufficient strength to pull the spot out of the parent metal when pulled apart.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the currentversion before use.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *Cabinets.* — Unless otherwise specified, at least one cabinet of each type, class, size, and grade shall be taken at random from each lot delivered.

4.1.2 *Enamel and primer.*—Unless otherwise specified, the manufacturer shall furnish 1 quart of enamel and primer from the lot used in the manufacture of the commodity for tests.

4.2 Inspection.—Each sample shall be inspected for type, class, size, grade, finish, construction, dimensions, design, workmanship, packaging, packing, and marking.

4.3 Tests.—Tests shall be conducted as described in the applicable specifications listed in section 2.

5. PREPARATION FOR DELIVERY

5.1 Packaging. — Unless otherwise specified, each cabinet shall be packaged in accordance with accepted commercial practice.

5.2 Packing.—Instrument cabinets shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.* — Unless otherwise specified, packages shall be marked with the name, type, class, size, and grade of the commodity, the quantity contained therein, and the names of the contractor and the manufacturer.

5.3.2 *Shipping containers.* — Unless otherwise specified, each shipping container shall be marked with the name, type, class, size, and grade of the commodity as defined by the contract or order under which the shipment is made, quantity contained therein, name of the contractor, number of the contract or order, name and address of the consignee, and the gross weight.

6. NOTES

6.1 Ordering data. — Purchasers should specify the type, class, size, and grade required, whether four-leg or enclosed detachable base is required, whether casters in lieu of glides are required, and should exercise any desired options offered herein. (See 1.1, 1.2, 3.13, 3.13.1, 3.13.2, 3.13.3, 3.17.2.2, 3.18.2.2, 4.1, 5.1, 5.3, 6.3, and 7.2.6.)

6.2 This specification covers the following items listed in the Armed Services Catalog of Medical Matériel:

7–026–850—Cabinet, Instrument, CRM, 16 by 30 by 72 inches.

7–027–000—Cabinet, Instrument, CRM, 16 by 36 by 72 inches.

7–029–000 — Cabinet, Instrument and Dressing, CRM, 16 by 30 by 60 inches.

7–029–240—Cabinet, Medicine, Combination Type, with Narcotic Locker, CRM.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the currentversion before use.

are normally procured to meet Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications.*

Federal Specification:

NN-B-621—Boxes, Wood, Nailed and Lock-Corner.

Military Specifications:

JAN-P-106—Packaging and Packing for Overseas Shipment—Boxes; Wood, Nailed.

JAN-P-125—Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.

JAN-P-140—Packaging and Packing for Overseas Shipment—Adhesives, Water-Resistant, Case-Liner.

MIL-M-3157—Marking of Domestic Shipments by Contractors for Supplies and Equipment Consigned to the Medical Departments of the Armed Services.

Navy Department Specification:

General Specifications for Inspection of Material.[1]

(Copies of specifications required for Army and Air Force purchases may be obtained upon application to the procuring agency. Both the title and identifying symbol or number should be stipulated when requesting copies.

(Copies of Federal and Military specifications required for Navy purchases and Navy Department specifications may be obtained without cost upon application to the Bureau of Supplies and Accounts, Department of the Navy, Washington 25, D. C., except that Naval activities should make application to Commanding Officer, Naval Supply Depot, Scotia 2, New York. Both the title and identifying symbol or number should be stipulated when requesting copies of specifications.)

7.2.2 *Inspection procedures (Navy).*—For Naval purchases, the general inspection procedure shall be in accordance with Navy Department General Specifications for Inspection of Material.

7.2.3 *Packaging.*—One cabinet shall constitute one unit. Glass shelves shall be removed and interleaved with corrugated fiberboard sheets of adequate size. The shelves so treated shall then be backed on both sides with corrugated fiberboard sheets and packed in a nailed wood box conforming to the requirements of Specification NN-B-621. The box shall contain sufficient excelsior to provide at least 2 inches of clearance between the shelves and the interior faces of the box. All exterior finished faces of the unit shall be protected with kraft paper and by cushioning with excelsior pads, flexible corrugated fiberboard, or other suitable materials. Wrapping and cushioning material shall be secured by tying with cotton cord or tape, or sealing with kraft gummed paper tape. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit. Keys shall be fastened together and tied to the handle, which shall be adequately protected against damage.

7.2.4 *Packing.*

7.2.4.1 *Domestic.*—Each unit shall be packed for type 3 load in a nailed wood box conforming to the requirements of Speci-

[1] Applicable to Navy purchases only.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the current version before use.

fication JAN-P-106. Each shipping container shall include skids of appropriate size to facilitate handling and to maintain the unit in an upright position. The unit and wood box containing the glass shelves shall be adequately secured within the shipping container by means of bolts, wooden braces or blocks, or other suitable devices to insure against shifting and breakage, or marring of surfaces. The work shall be accomplished in such a manner that the weight of the unit will not be carried directly by its legs.

7.2.4.2 *Overseas.* — Each unit shall be packed as described in 7.2.4.1. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Specification JAN-P-125, for case liners; seams and closures shall be sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Specification JAN-P-140.

7.2.5 *Marking.*

7.2.5.1 *Packages.*—Each package shall be marked with the stock number, nomenclature, type, class, size, grade, quantity, and the name of the contractor. When the contractor is not the manufacturer, the name of the manufacturer shall also appear as the manufacturer.

7.2.5.2 *Shipping containers.*

7.2.5.2.1 *For domestic shipment.* — Each shipping container shall be marked in accordance with Military Specification MIL-M-3157.

7.2.5.2.2 *For overseas shipment.* — Each shipping container shall be marked as specified by the procuring agency.

7.2.6 *Ordering data.* — Procurement documents should specify whether the subject commodity is to be packed and shipping containers marked for domestic or overseas shipment. (See 7.2.4 and 7.2.5.)

NAVY INTEREST: Md

(See following figures 1 and 2.)

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.


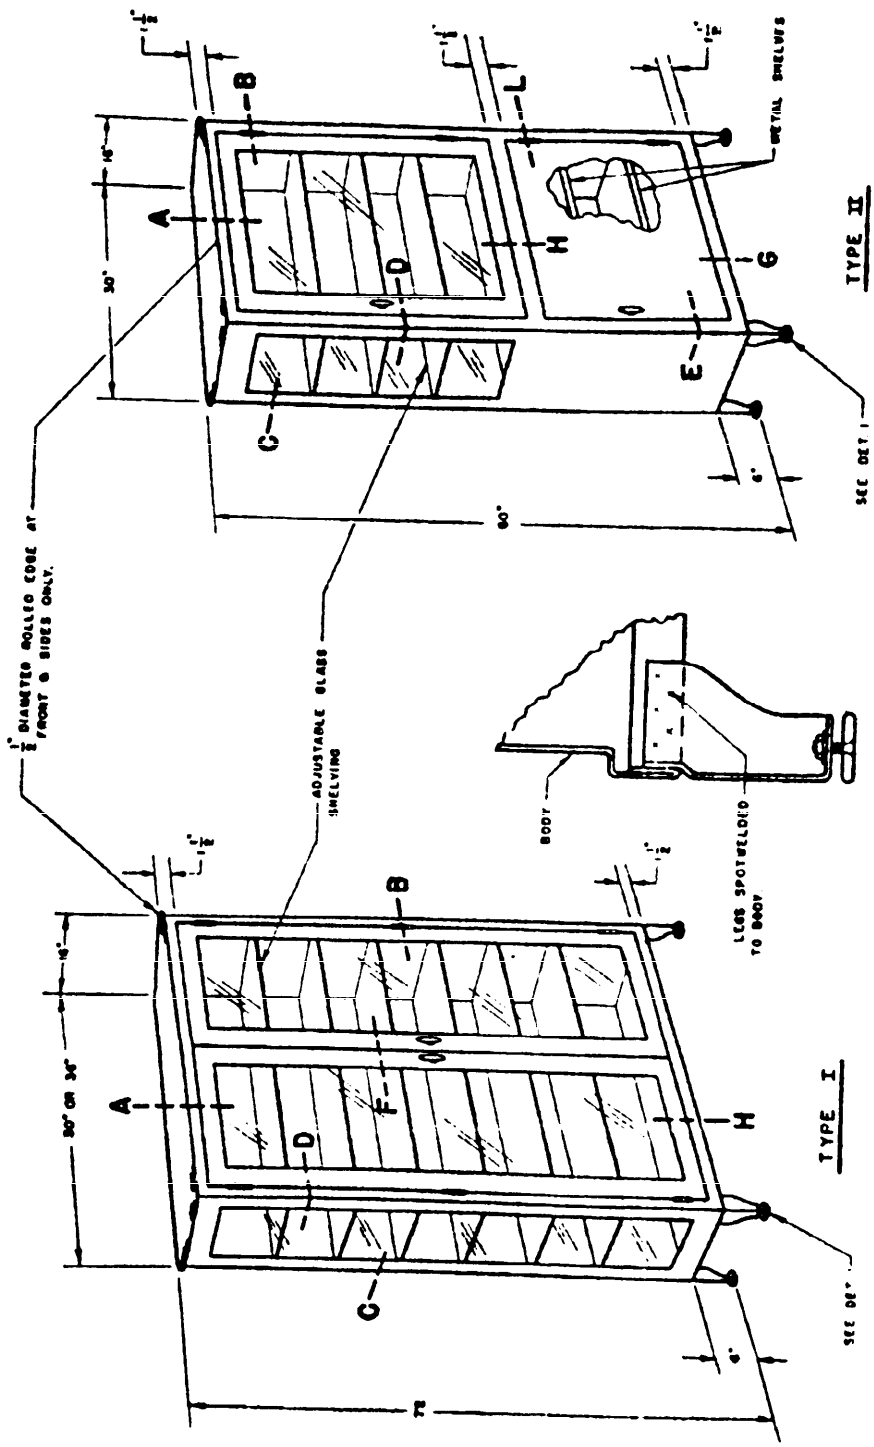


FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

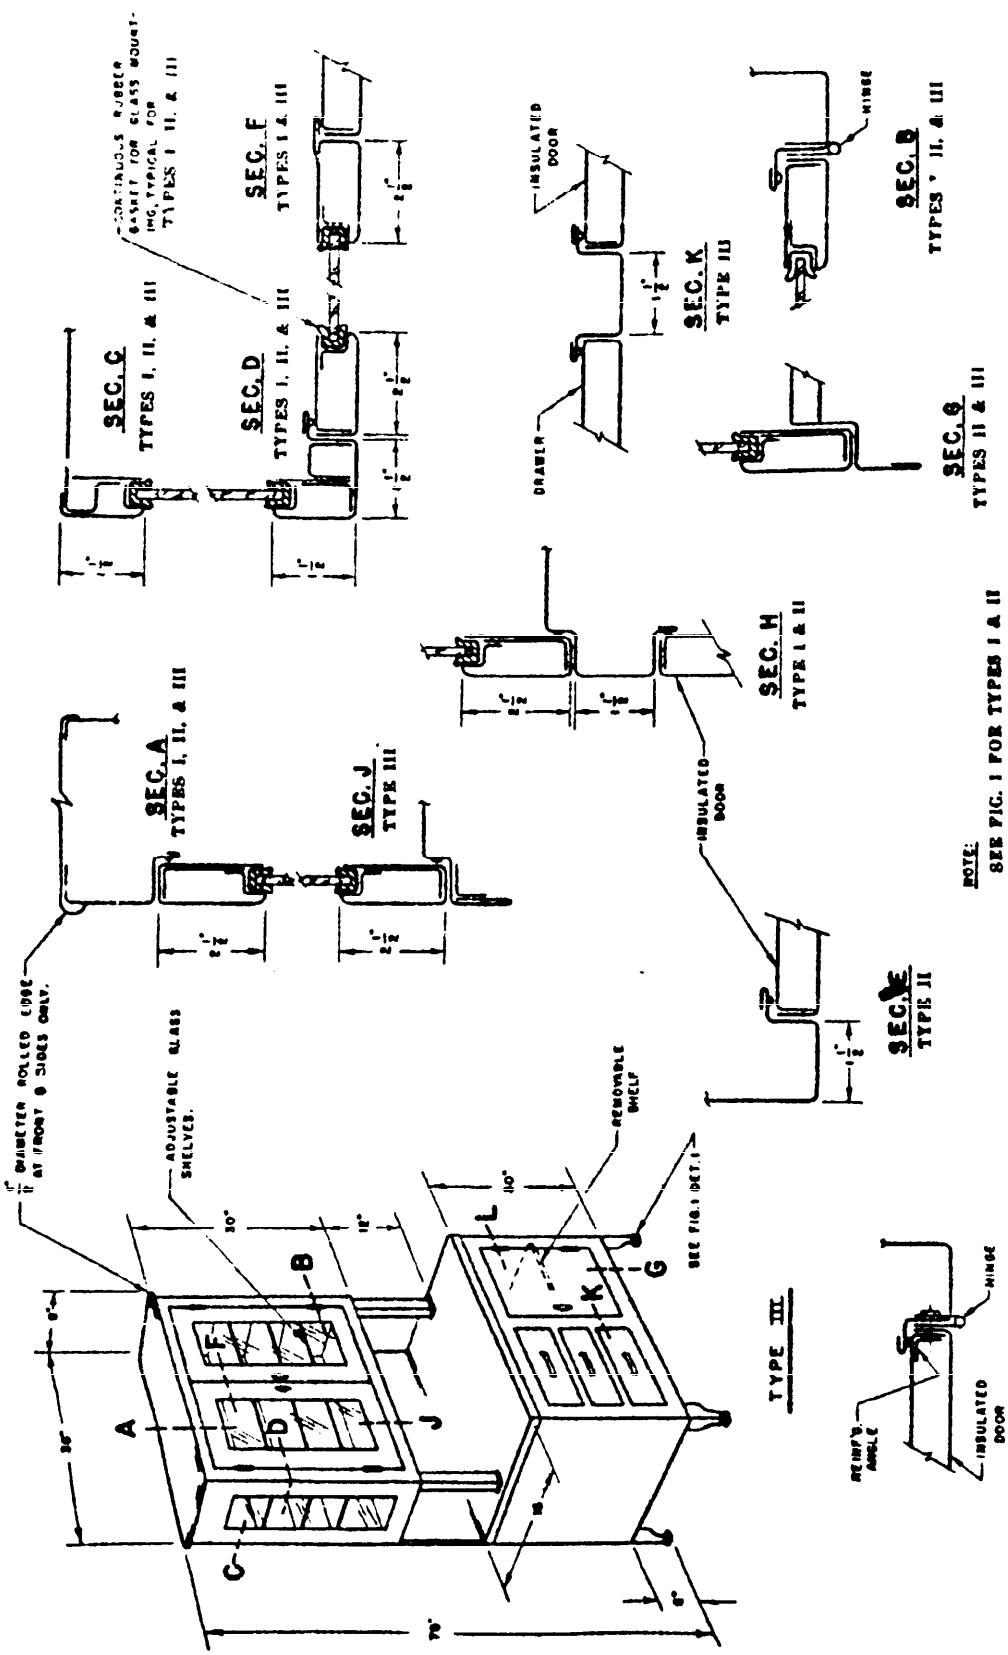

NOTE:
SEE FIG. 1 FOR TYPES I & II

FIGURE 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.