GG-H-590
JANUARY 14, 1959

FEDERAL SPECIFICATION

HOLDER, RADIOGRAPHIC FILM CASSETTE

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 This specification covers a vertical type cassette holder designed for wall mounting and suitable for holding standard radiographic film cassettes from 5 by 7 inches to 14 by 17 inches, and a standard radiographic 14- by 17-inch stationary grid.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

L–L–31 — Laminated Thermosetting Sheets, Rods, and Tubes.
QQ–A–591—Aluminum Alloy Die-Castings.
QQ–A–601—Aluminum Alloy Sand Castings.
QQ–S–636 — Steel; Carbon (Low-Carbon), Sheets and Strips.
PPP–B–601—Boxes, Wood, Cleated-Plywood.
PPP–B–621—Boxes, Wood, Nailed and Lock-Corner.
PPP–B–636—Boxes, Fiber.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Std. No. 123—Marking for Domestic Shipment. (Civilian Agencies).
Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL–F–1148—Fibre, Insulation.
MIL–L–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material.—Satisfactory high grade materials shall be used throughout. Materials shall be suitable for the purpose and of sufficient strength to maintain operational alignment for life of the equipment.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the currentversion before use.

3.1.1 *Sheet, plate, and strip stock.*—Sheet, plate, and strip stock shall conform to the requirements of Federal Specification QQ–S–636.

3.1.2 *Cast aluminum.* — Cast aluminum shall conform to the requirements of Federal Specification QQ–A–591 or QQ–A–601.

3.1.3 *Bushings.*—Bushings may be metallic or nonmetallic. Metallic bushings shall be brass; nonmetallic bushings shall be fiber conforming to grade BH, form S, of Military Specification MIL–F–1148, nylon or laminated thermosetting plastic conforming to type II, grade C, of Federal Specification L–L–31.

3.2 **Construction.**—The wall mounted cassette holder shall be constructed as shown in figure 1. The holder shall be 37¾ ± ¼ inches high, 16¼ ± ¼ inches wide, and 3¾ ± ¼ inches deep and shall consist of at least the following components:

Mounting base	3.2.1
Carriage track	3.2.2
Cassette carriage	3.2.3
Chinrest	3.2.4
Height indicator	3.2.5

3.2.1 *Mounting base.*—The mounting base shall consist of one or more rigid sheet metal plates. Suitably placed holes for mounting the unit to the wall, and the accessories for mounting the unit, shall be provided.

3.2.2 *Carriage track.*—There shall be suitable tracks or channels to hold the cassette carriage. The carriage tracks shall be chrome-plated steel, corrosion-resisting steel solid bars, tubular steel (corrosion-resistant or chrome-plated), or aluminum tubing (alloy 2024-T3, or equal), and shall be smooth, parallel and of a suffcient length to permit a range of motion of at least 15 inches with a 14- by 17-inch cassette mounted on the cassette carriage with its long axis vertical. The minimum wall thickness of all tubing shall be 0.049 inch.

3.2.3 *Cassette carriage assembly.*—The cassette carriage shall be reinforced with steel and shall move freely and smoothly in a vertical direction. There shall be a locking device to permit locking the cassette carriage at any point in its vertical travel. The cassette carriage shall be adjustable to hold and lock in place any standard type cassette, with the cassette in either the horizontal or vertical position. The cassette carriage shall be marked to facilitate centering of cassettes. The front of the cassette carriage shall be open so that the cassette is always in view as an aid to centering. In addition, there shall be grooves, tracks, or a guide rail to support the 14- by 17-inch grid close to the cassette, when any size cassette from 5 by 7 inches to 14 by 17 inches is being used in either horizontal or vertical position. An adjustable cassette adapter, as specified in 3.2.3.1, shall be supplied so that any standard size cassette may be used with a standard 14- by 17-inch grid. The bushings, riding the carriage tracks, when fabricated of a nonmetallic material shall be encased between two sheets of steel and the assembly securely and permanently fastened to the carriage. The nonmetallic bushings shall be approximately 3/32 inch thick and shall make contact with the carriage tracks in at least eight points (four on each side). The brass bushings may be full length for each section for a total of four bushings.

3.2.3.1 *Adjustable cassette adapter.*—The adjustable cassette adapter shall be fabricated of aluminum or sheet steel. The adapter shall have a clamping device 1⅞ inches long for holding the cassette, and a locking device, such as knurled thumbscrew (setscrew) to lock the cassette in place.

3.2.4 *Chinrest.*—Chinrest shall be of cast aluminum or other suitable material. The chinrest shall be highly polished and shall have no sharp corners or edges. The chinrest shall be permanently fastened to the top edge of the cassette carriage. The chinrest shall be shaped to the contour of the chin so as to

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

facilitate positioning of the patient in chest radiography.

3.2.5 *Height indicator.*—A height indicator fabricated of sheet steel shall be furnished. The height indicator shall be graduated in inches and shall be constructed so as to become an integral part of the cassette holder. The height indicator shall be numbered to help in aligning the cassette carriage with the X-ray tube. The height scale shall be adjustable to correspond to the tabletop or cassette to focal spot scale on any X-ray tube-stand. Height indicator shall be interchangeable for right- or left-side mounting.

3.3 **Finish.** — The wall mounted cassette holder shall be degreased, primed, and finished with smooth enamel in the manufacturer's standard color. Trimming shall be chrome or other suitable corrosion-resistant material. The finish shall not fade, crack, or peel under normal conditions of use.

3.4 **Interchangeability.** — All individual parts or assemblies of parts of any complete unit supplied on a contract shall be interchangeable with corresponding parts or assembly of parts of all other units supplied on that contract.

3.5 **Identification marking.** — Each wall mounted cassette holder shall be permanently and legibly marked in a conspicuous location with the Federal stock number, manufacturer's name or registered trade-mark, model number, serial number, contract number, and the letters "U.S.". Marking shall be accomplished by stamping, or by means of a metal nameplate permanently affixed, and shall be of a size such as required for ready readability and identification.

3.6 **Service data.**—The contractor shall enclose with each unit two copies each of one or more booklets which contain complete instructions for installation, operation, maintenance, and a list of component parts. Each part of the unit other than common fasteners, etc., shall be identified in the service data and parts list by the manufacturer's part number.

3.6.1 *For Military Medical Supply Agency procurement.*—The contractor shall mail six (6) additional copies of the service data, required in 3.6, to the contracting officer for distribution.

3.7 **Workmanship.**—Workmanship shall be first class throughout. The wall mounted cassette holders shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 **General.**—The provisions contained in this section are applicable to inspection performed by and for the Government. Sampling, inspection, and test procedures for components or materials described shall be in accordance with this specification and with specifications and standards referenced herein to the extent applicable, except that this specification shall govern in the event of conflict.

4.1.1 *Supplier responsibilities for inspection for military procurement.*—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government, upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

4.1.2 Inspection, as used in this specification, is defined as both examination (visual

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and the test results obtained, and indicating that material is as specified, may be furnished.

4.2 Sampling. — Sampling shall be conducted in accordance with Military Standard MIL–STD–105 and appendix thereto.

	Inspection level	AQL (percent defective)
For visual examination:		
Major	II	1.0
Total	II	4.0
For dimensional examination	L5	2.5
For component testing	L5	*

* Acceptance number shall be zero (0) for all sample sizes.

4.2.1 *Raw materials.*—Four ounces of each lot of each metal used in the construction of the holder shall be selected for chemical analysis (see 4.4.1).

4.2.2 *Components.*—Sufficient samples of the components shall be selected from each lot of material used in the manufacture of the holder to perform tests as required by the applicable subsidiary specifications or by tests specified herein. When sample size for components covered by the subsidiary specifications is not specified, the sample size for each test shall be as indicated in 4.2. No test result shall fall below the minimum or exceed the maximum values specified. The sample unit for testing shall be the quantity necessary to perform all required tests one time each.

4.2.3 Where possible, the same sample shall be used for the determination of two or more tests.

4.3 Inspection. — The holder shall be inspected to determine compliance with all requirements contained in sections 3 and 5 of this specification. Nonconformance with these requirements will be permitted to the extent indicated in 4.2.

4.3.1 *Classification of defects.*—Inspection shall be conducted in accordance with the following classifications of defects:

	*Categories and defects**
Major	
101.	Holder not complete with all specified component parts.
102.	Cassette carriage fails to slide smoothly and freely over the entire length of its travel.
103.	Locks on either cassette carriage or adjustable cassette adapter fail to fix or release at any set position.
104.	Adjustable cassette adapter fails to slide smoothly and freely over the length of its travel.
105.	Channels in upper and lower horizontal members of carriage assembly, including cassette adapter, not properly located and aligned to accommodate cassette and grid.
106.	Component parts not free of cracks and burs or sharpness at edges.
107.	Plating not free of blistered, excessively scratched or unplated areas.
108.	Cassette carriage adjustment not within range required to hold any standard type cassette in vertical or horizontal position.
109.	Height indicator scale not present or not graduated as specified.
110.	Height indicator scale not adapted for right- or left-side mounting.
Minor	
201.	Cassette carriage not marked to facilitate centering cassettes.
202.	Finish not smooth, adherent and free of chipped, cracked, blistered, or bare areas.
203.	Identification marking not present and complete or not permanent and legible.
204.	Service data, in duplicate, not included with each unit.

* Inspection is not restricted to the classified defects listed above.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.8.2 *Dimensional examination.* — The holder shall be inspected for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests.—Tests shall be conducted in accordance with the applicable specifications to determine compliance with this specification.

4.4.1 *Chemical composition.* — Test for chemical analysis shall be conducted in accordance with method 111 or 112 of Fed. Test Method Std. No. 151 (see 4.1.3).

5. PREPARATION FOR DELIVERY

For civil agency procurement the levels of preservation, packaging, and packing protection used are defined in Federal Standard No. 102.

5.1 Packaging.

5.1.1 *Unit of issue.*—One holder, as specified, constitutes one unit.

5.1.2 *Level A.*

5.1.2.1 *For nonmilitary agencies.* — Each unit shall be packaged in a carton of appropriate size fabricated from not less than 200 pound test fiberboard and constructed in accordance with Federal Specification PPP–B–636, type I or II, class 1 or 2, style RSC. Each carton shall be adequately secured to prevent accidental opening.

5.1.2.2 *For military agencies.*—Each unit shall be packaged in a carton of appropriate size fabricated from not less than 200 pound test fiberboard and constructed in accordance with Federal Specification PPP–B–636, type I, class 1. Each carton shall be adequately secured to prevent accidental opening.

5.1.3 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Each unit carton shall be overpacked in an exterior container designed for type 3 load, and constructed in accordance with Federal Specification PPP–B–601, table II, using type III, class 1 plywood or PPP–B–621, table IV, style 2, 2½, 3, or 4. Closure shall comply with appendix of applicable specification.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing of the liner shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Each unit carton shall be overpacked in an exterior container constructed in accordance with Federal Specification PPP–B–601, table I, using type III, class 1 plywood, or PPP–B–621, table II, style 2, 2½, 3, or 4.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *For nonmilitary agencies.*—Unit and shipping containers shall be marked in accordance with Federal Standard No. 123.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

5.3.2 *For military agencies.*—Marking of unit carton will not be required. Exterior container shall be marked in accordance with Military Standard MIL–STD–129, except that 6.2(c), 6.2(d), and 6.5 shall not be applicable. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 **Ordering data.** — Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following item appearing in the Armed Services Medical Stock List:

6525–299–8300 — HOLDER, RADIOGRAPHIC FILM CASSETTE

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 **Transportation description.**—Transportation description applicable to this item is:

Holder, Photographer's Material, NOIBN
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.
Motor volume minimum weight 20,000 pounds.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

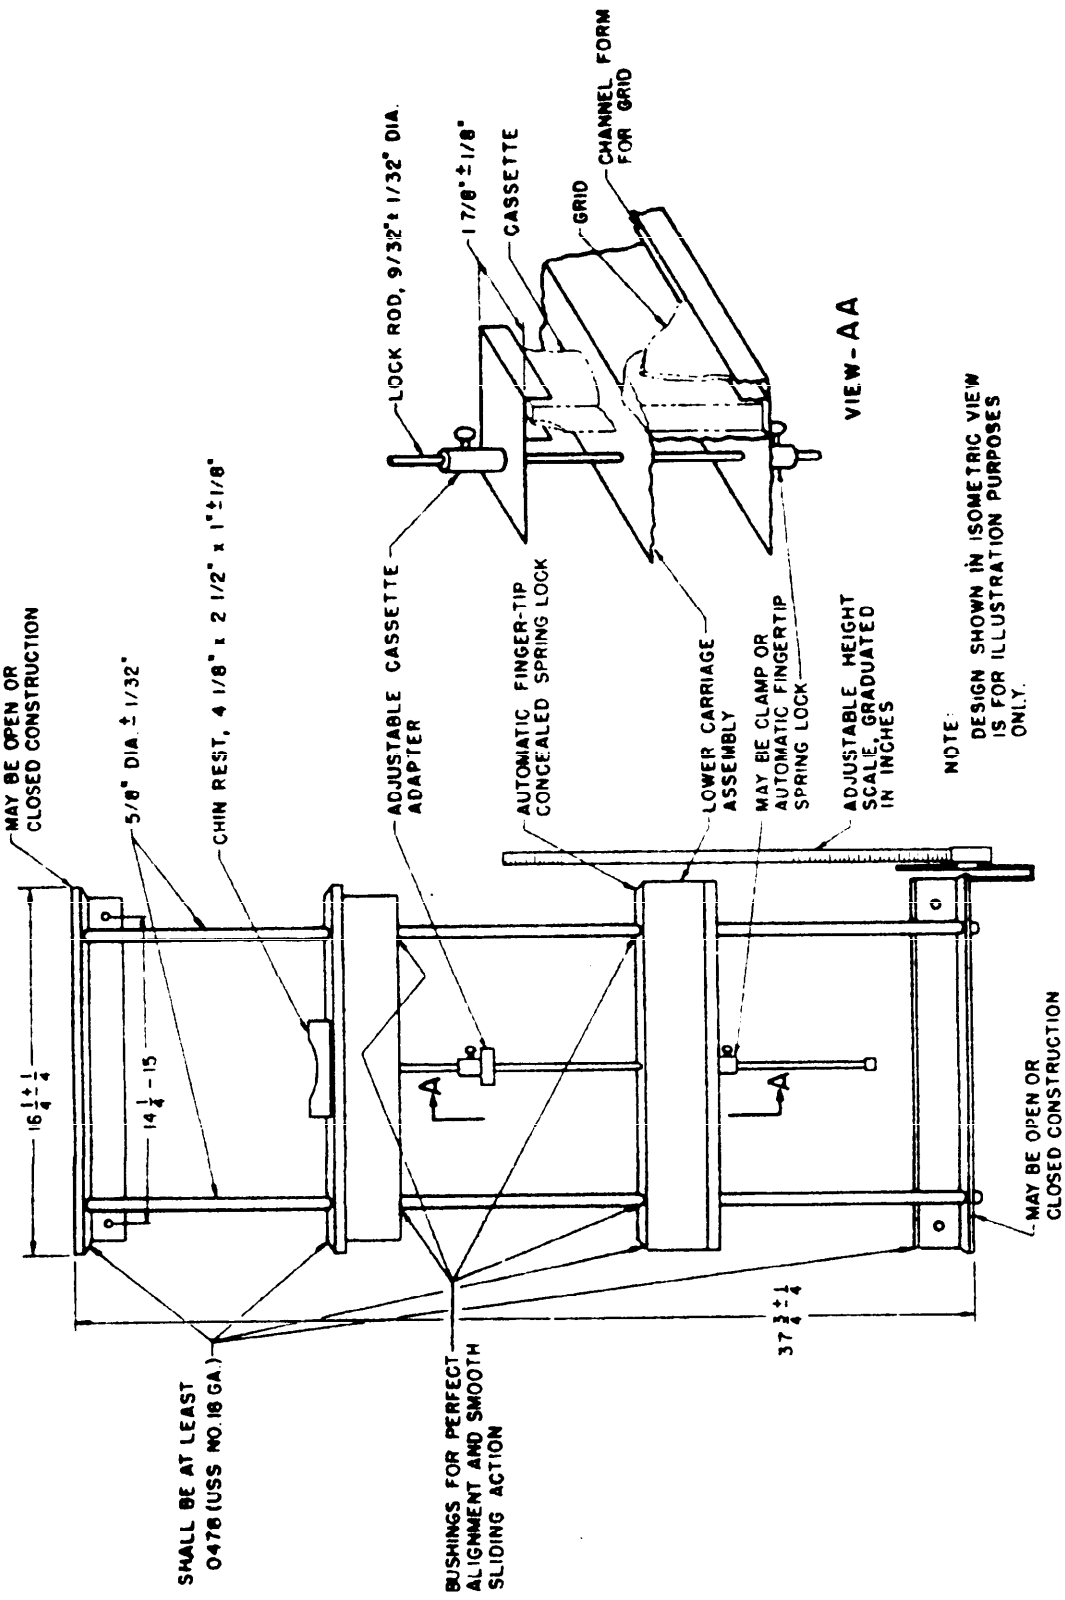


FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.