GG–P–636
9 OCTOBER 1952

FEDERAL SPECIFICATION

PRESS, FLASK, DENTAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers a flask press for holding acrylic cases under pressure during the curing process. Flask press shall serve as a press to close the flask and as a spring clamp when the springs in the base are engaged. Press shall have a capacity of two flasks, each $2\frac{5}{16}$ inches in height.

2. APPLICABLE SPECIFICATIONS

2.1 There are no other specifications and standards applicable to this specification except those referenced in section 7 by individual departments.

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application, accompanied by money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C., or to the GSA Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, and Seattle. Prices may be obtained from the Superintendent of Documents or from the GSA Regional Offices.)

3. REQUIREMENTS

3.1 **Material**—Flask press shall be made of cast bronze, except as hereinafter specified. When materials are used which are not specifically designated they shall be entirely suitable for the purpose.

3.2 **Component parts.**—Flask press shall consist of a holding handle, wrench, frame, pressure screw, upper pressure plate, lower pressure plate, and two springs. Each part shall conform to the dimensions, style and design as shown in figure 1. Commercial tolerances will be permitted.

3.2.1 *Holding handle.*—The holding handle shall consist of a steel rod inserted into a wooden handle equipped with a steel ferrule.

3.2.2 *Wrench.*—The wrench shall be an Allen-type, hexagonal-shaped, steel wrench, suitable for use with the pressure screw. Unless otherwise specified, the wrench shall be $4\frac{3}{4}$ inches long, as shown in figure 1.

3.2.3 *Frame.*—The base, top, and sides of the frame shall be cast in one piece. The top shall be equipped with a lifting loop, constructed of bronze wire, positioned as shown in figure 1. Top of frame shall be drilled to receive steel rod of holding handle.


3.2.4 *Pressure screw.*—The pressure screw shall be broached at the top for the insertion of the Allen wrench (see 3.2.2).

3.2.5 *Upper pressure plate.*—The upper pressure plate shall be notched on the ends to fit the sides of the frame and shall be permanently attached to the pressure screw.

3.2.6 *Lower pressure plate.*—The lower pressure plate shall be notched on the ends to fit the sides of the frame, shall have two screws inserted as guides and shall be designed with a stop on each side which shall be an integral part of the plate.

203431-52-(68)

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the current version before use.

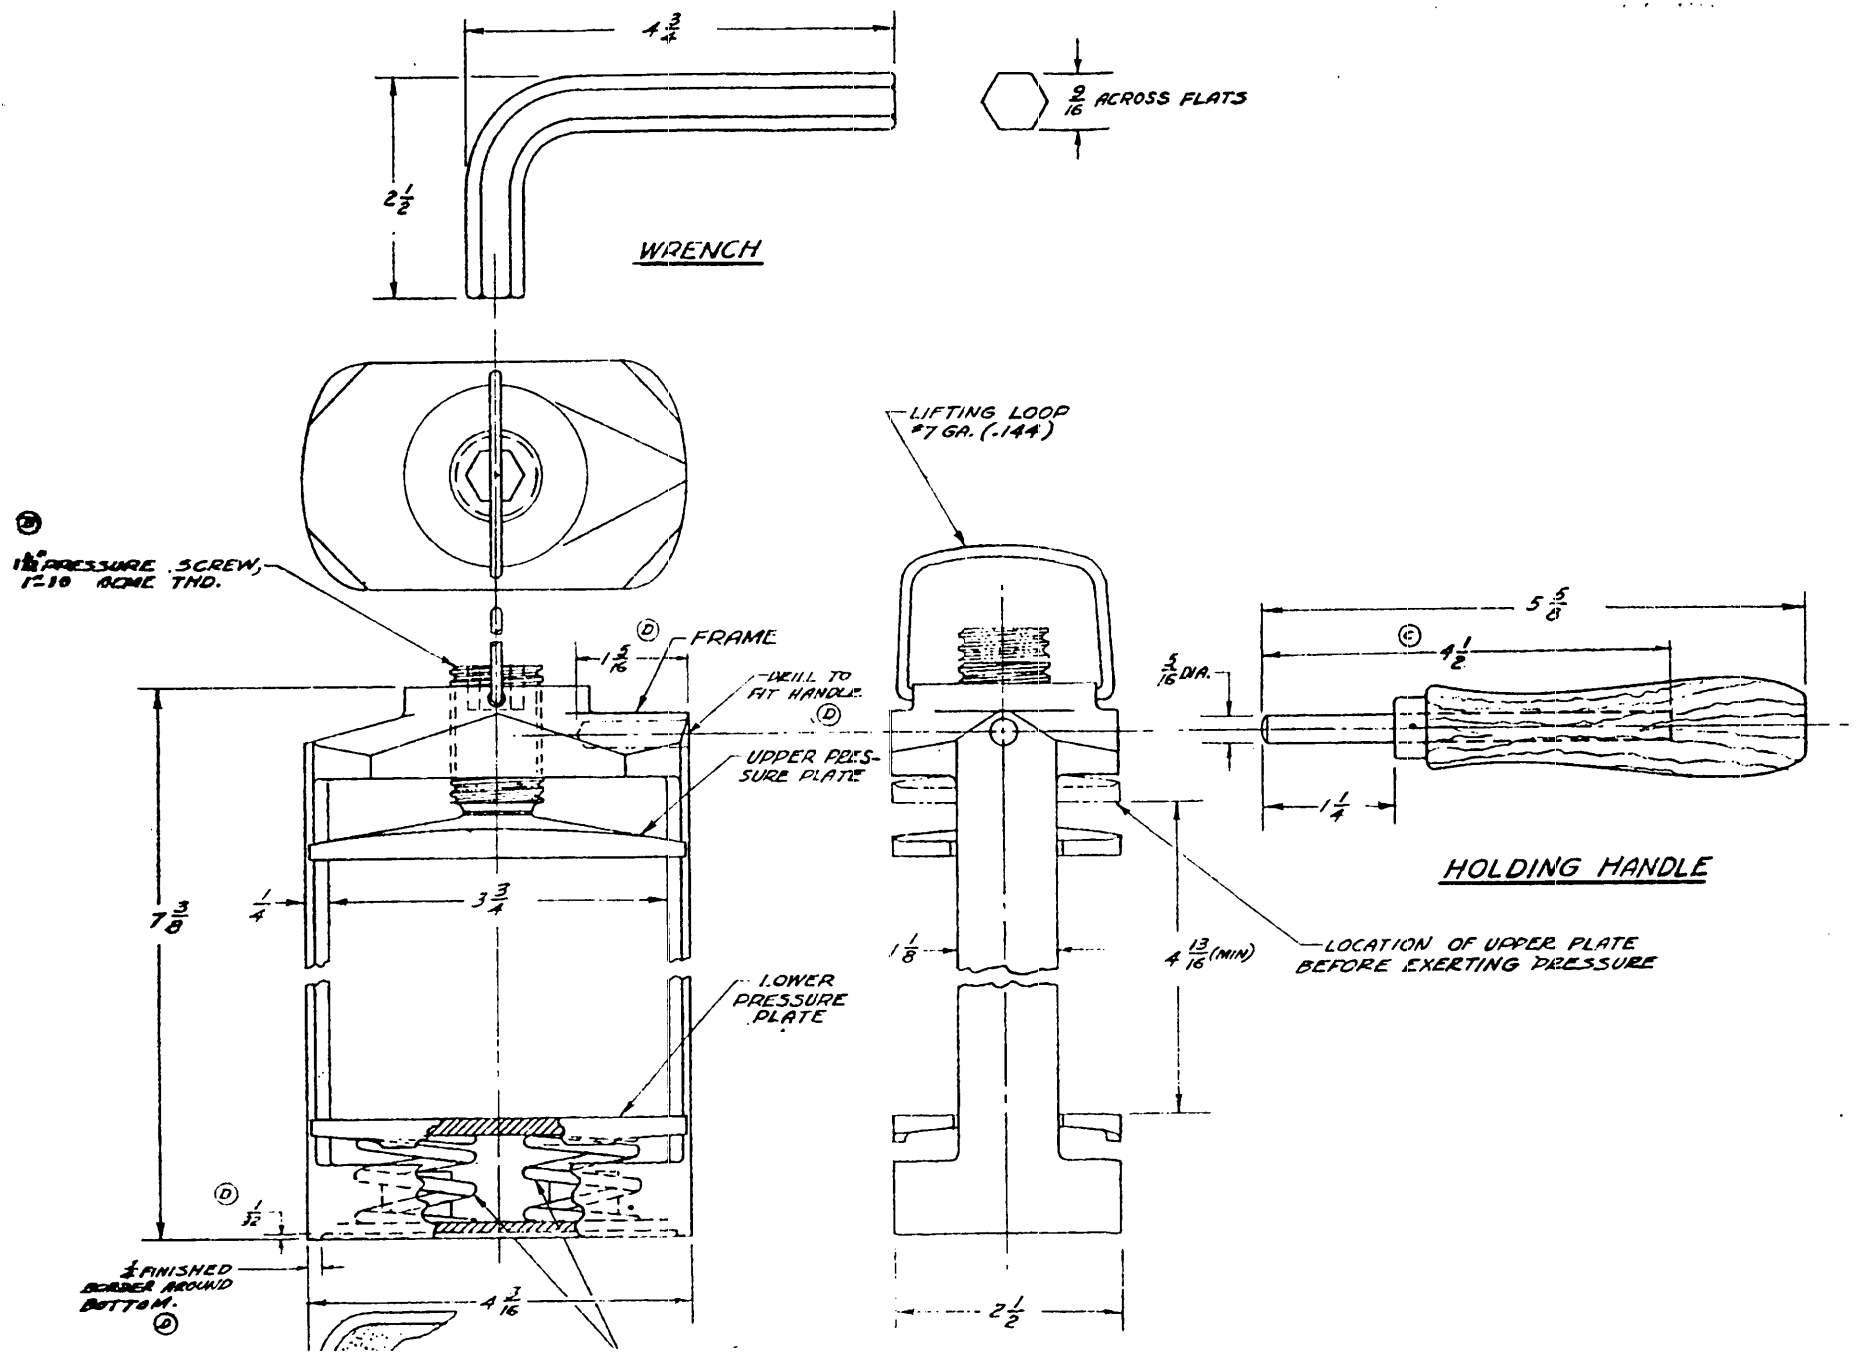

Source: https://assist.dla.mil -- Downloaded: 20260-26T11:52Z
Check the source to verify that this is the current version before use.

3.2.7 *Springs.*—The springs shall be made of stainless steel, of the coil type, located in the base of the frame, and shall engage the lower pressure plate. Springs shall be replaced by removing the two screws from the base of the frame. The pressure exerted by the springs shall be not less than 400 pounds and shall be well distributed.

3.3 Identification marking.—Flask press shall be stamped or cast with the name or registered trade-mark of the manufacturer.

3.4 Finish.—All steel parts shall be suitably plated to prevent corrosion.

3.5 Workmanship.—Workmanship shall be first class in every respect. Flask press shall be free from defects which detract from its appearance or may impair its serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.—Unless otherwise specified, at least one press shall be taken at random from each 100, or fraction thereof delivered.

4.2 Inspection.—Each press shall be inspected for material, workmanship, dimensions, component parts, finish, packaging, packing and marking.

5. PREPARATION FOR DELIVERY

5.1 Packaging.—Unless otherwise specified, the press shall be packaged in accordance with accepted commercial practice.

5.2 Packing. — The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Packages.*—Unless otherwise specified, packages shall be marked with the name and size of the commodity, the quantity contained therein, and the names of the manufacturer and contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 Ordering data.—Purchasers should exercise any desired options offered herein. (See 3.2.2, 4.1, 5.1, 5.3, 6.2, and 7.2.6.)

6.2 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.3 This specification covers the following item appearing in the Armed Services Catalog of Medical Matériel:

5–155–150—Clamp, Flask.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., normally procured for Federal Government requirements.

6.5 Transportation description.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

6.5.1 *Transportation description applicable to these items is:*

Presses, not otherwise indexed by name, other than filter, set up.
Less carload or less truckload, in boxes or crates;
Carload or truckload, in packages.
Carload weight 24,000 pounds, subject to Rule 34, Consolidated Freight Classification.
Truckload weight 24,000 pounds.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and standard, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specification and standard.*

Federal Specifications:

NN–B–601—Boxes; Wood-Cleated-Plywood, for Domestic Shipment.
NN–B–621—Boxes; Wood, Nailed and Lock-Corner.
NN–B–631—Boxes; Wood, Wirebound (for Domestic Shipment).
LLL–B–631—Boxes; Fiber, Corrugated (for Domestic Shipment).
LLL–B–636—Boxes; Fiber, Solid (for Domestic Shipment).

Military Specifications:

JAN–P–105—Packaging and Packing for Overseas Shipment—Boxes, Wood, Cleated, Plywood.
JAN–P–106—Packaging and Packing for Overseas Shipment—Boxes; Wood, Nailed.
MIL–B–107—Boxes, Wood, Wirebound (Overseas Type).
JAN–P–125—Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.
MIL–A–140 — Adhesive, Water-Resistant, Waterproof Barrier-Material.

Navy Department Specification:

General Specification for Inspection of Material. [1]

Military Standard:

MIL–STD–129—Marking of Shipments.

(Copies of specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting office.)

7.2.2 *Packaging.*—One (1) clamp constitutes one unit. Each unit shall be packaged in a carton, of appropriate size and design, conforming to the requirements of Federal Specification LLL–B–631 or LLL–B–636. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Each carton shall be adequately secured to prevent accidental opening.

7.2.3 *Packing.*

7.2.3.1 *For domestic shipment.*—Ten unit cartons (10 units) shall be packed in a shipping container conforming to the requirements of Federal Specification NN–B–601, NN–B–621, or NN–B–631.

7.2.3.2 *For overseas shipment.*—Ten unit cartons (10 units) shall be packed in a ship-

[1] Applicable to Navy purchases only.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

ping container designed for type 2 load and conforming to the requirements of Military Specification JAN–P–105, JAN–P–106, or MIL–B–107. Closure and strapping shall conform to the requirements of the appendix to the applicable box specification. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN–P–125, for case liners; seams and closures shall be completely sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Military Specification MIL–A–140.

7.2.3.3 *Packing variation.*—If the number of units in any shipment is not the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in a shipping container of suitable size and design and so constructed as to insure safe delivery to specified destination.

7.2.4 *Marking.*—Each unit carton and each shipping container shall be marked in accordance with Military Standard MIL–STD–129.

7.2.5 *Inspection procedures (Navy only).*—The general inspection procedures shall be in accordance with Navy Department General Specifications for Inspection of Material.

7.2.6 *Ordering data.*—Procurement documents should specify whether the subject commodity is to be packed for domestic or overseas shipment (see 7.2.3.)

NAVY INTEREST: *Md*

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

For sale by the Superintendent of Documents, Washington 25, D. C. Price 5 cents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.