FEDERAL SPECIFICATION

SPECULUM, VAGINAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers vaginal specula suitable for vaginal examination, treatment, and operative procedures.

1.2 Classification.

1.2.1 *Types and sizes.* — Specula shall be of the following types and sizes, as specified (see 6.1):

Type I.—Graves (bivalve).
Size 1. — 3½ inch blade.
Size 2.—4 inch blade.
Size 3.—5 inch blade.

Type II.—Sims (double ended).
Size 2.—2½ and 3 inch blades.
Size 4.—3 and 3¼ inch blades.

Type III.—Auvard (weighted).
Size 1.—2½ inch blade.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 Specifications and standards.—The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

GG-I-526 — Instruments, Dental and Surgical; General Specifications.

QQ-B-626 — Brass, Leaded and Nonleaded; Rods, Shapes, Forgings, and Flat Products with Finished Edges (Bars, Flat Wire and Strips).

Federal Standards:

Fed. Std. No. 102 — Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123 — Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL-P-12902 — Packaging of Surgical, Dental and Veterinary Instruments, Diagnostic Equipment, and Related Items.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL-STD-129—Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 **Other publication.** — The following document forms a part of this specification. Unless otherwise indicated, the issue in effect on date of invitation for bids shall apply.

American Iron and Steel Institute:

Steel Products Manual.

(Application for copies should be addressed to the American Iron and Steel Institute, 150 East Forty-second Street, New York 17, N. Y.)

3. REQUIREMENTS

3.1 **Material.**—Specula shall be fabricated of class and composition steels, as specified in table I, in accordance with Federal Specification GG–I–526.

TABLE I.

Type	Class	Composition
I (Graves)	2 or 5	G, H, or U*
II (Sims)	2	G
III (Auvard)	4 or 5	N, P, or U**

* Material shall be either American Iron and Steel Institute (AISI) 410 or 430 stainless steel, and shall meet the copper sulfate and boil tests requirements as specified in Federal Specification GG–I–526. The hardness for AISI 410 shall be Rockwell C40–C45 and for AISI 430 shall be Rockwell C25–C30

** Material shall be composition 22 of Federal Specification QQ–B–626, chromium plated over nickel, and shall be in accordance with the plating and corrosion tests requirements, of Federal Specification GG–I–526 for class 4, composition N.

3.2 **Style, design, and dimensions.**

3.2.1 *Type I (Graves).*—Type I shall be a bivalve vaginal speculum, Graves design, and shall be as shown in figures 1 and 2.

3.2.2 *Type II (Sims).* — Type II shall be double-ended vaginal speculum, Sims design, with strongly concave blades, and shall be as shown in figure 3.

3.2.3 *Type III (Auvard).* — Type III shall be a weighted (2½ pounds minimum), Auvard design, vaginal speculum, and shall be as shown in figure 4.

3.3 **Finish.**—Finish shall be mirror in accordance with the requirements of Federal Specification GG–I–526.

3.4 **Additional requirements.**—Except as specified herein, the vaginal specula shall comply with applicable requirements and tests of Federal Specification GG–I–526. The requirements of that specification for micrometallographic examination shall not apply.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* — When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 *For examination.* — Sampling for examination shall be conducted in accordance with Military Standard MIL–STD–105.

4.2.2 *For tests.* — Sampling for tests shall be conducted in accordance with Military Standard MIL–STD–105. Requirements applicable for individual unit only (see table II).

4.2.3 *Raw materials.* — Four ounces of each lot of each metal used in the construction of the speculum shall be selected for chemical analysis.

4.2.4 Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination.—The speculum shall be examined to determine compliance with all requirements contained in this specification.

4.4 Tests.—Tests shall be conducted, as necessary, to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

For civil agency procurement only, Federal Standard No. 102 should be referred to for definitions and applications of the various levels of packaging and packing protection for supplies and equipment.

5.1 Packaging and packing.

5.1.1 *Unit of issue.* — One speculum, as specified, constitutes one unit of issue.

5.1.2 *Packaging quantities.* The number of units of issue indicated in table III shall be packaged in each unit package and exterior container, as applicable for the required level of protection specified in the procurement document.

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.* — Packaging and packing shall conform to the requirements of Military Specification MIL–P–12902, Procedure Code No. 35.

5.1.4 *Level B.* — Packaging and packing shall conform to the requirements of Military Specification MIL–P–12902, Procedure Code No. 21.

5.1.5 *Level C.* — The subject commodity shall be packaged and packed in substantial commercial containers of the type, size, and

TABLE II.

Component	Characteristic	Req.	Test procedure	Unit of product	Insp. level	AQL
Speculum	Hardness	GG–I–526	GG–I–526	1-speculum	L3*	**
	Boil test	GG–I–526	GG–I–526	1-speculum	L3*	**
	Copper sulfate	GG–I–526	GG–I–526	1-speculum	L3*	**

* A minimum of three units shall be tested regadless of lot size.
** Acceptance number shall be zero for all sample sizes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

TABLE III. — *Packaging quantities*

Type	Unit package	Intermediate package	Exterior container
I	1	Not required	48
II	1	Not required	48
III	1	Not required	12

kind commonly used for purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2 **Marking.**

5.2.1 *For nonmilitary agencies.*

5.2.1.1 *Intermediate and exterior containers.* — In addition to any special marking specified in the contract or order, containers shall be marked in accordance with Federal Standard No. 123.

5.2.2 *For military agencies.*

5.2.2.1 *Interior packages.* — Marking shall conform to the requirements of Military Specification MIL–P–12902, except that the ASMPA stock number will not be required.

5.2.2.2 *Exterior container.* — Exterior container shall be marked in accordance with Military Standard MIL–STD–129.

6. NOTES

6.1 **Ordering data.**—Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number and date of this specification.

(*b*) Types and sizes, required (see 1.2).

(*c*) Selection of applicable levels of packaging and packing (see 5.1).

(1) Level B preservation and packaging is intended to provide economical but limited protection, and should be specified only when it is determined the speculum will be held in covered storage approximately 12 months from date of initial packaging.

6.2 This specifiction does not include all types, classes grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 **Transportation description.** — Transportation descriptions and minimum weights applicable to this commodity are:

Rail:

Surgical instruments, not otherwise indexed by name.

Carload minimum weight 10,000 pounds, subject to Rule 34 Uniform Freight Classification.

Motor:

Surgical instruments, not otherwise indexed.

Truckload minimum weight (W) 10.6 pounds, (W) subject to Rule 34, National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded, by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

CUSTODIANS:

Army—Army Medical Service
Navy—Bureau of Medicine and Surgery
Air Force.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

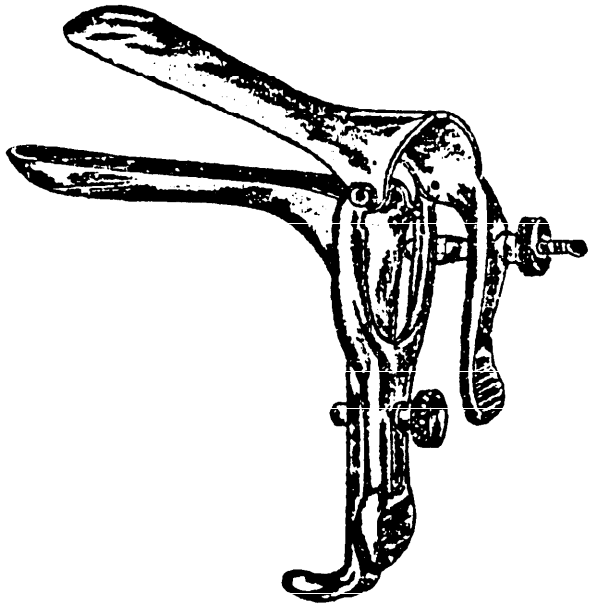


FIGURE 1.—Type I Graves.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

SIZE	A	B	C	D	E	F	G
1	$1\frac{3}{16}\pm\frac{1}{16}$	$3^{+\frac{5}{16}}_{-0}$	$\frac{1}{2}^{+\frac{1}{16}}_{-\frac{5}{64}}$	$4\frac{7}{16}\pm\frac{3}{16}$	$\frac{3}{4}\pm\frac{1}{8}$	$45°\pm5°$	$3\frac{3}{8}^{+\frac{1}{8}}_{-\frac{3}{16}}$
2	$1\frac{3}{16}\pm\frac{1}{8}$	$4^{+\frac{1}{2}}_{-\frac{1}{16}}$	$\frac{11}{16}\pm\frac{1}{16}$	$5\frac{7}{16}^{+\frac{3}{16}}_{-\frac{5}{16}}$	$\frac{7}{8}^{+\frac{1}{8}}_{-\frac{1}{16}}$	$36°\pm5°$	$4\frac{1}{2}^{+\frac{3}{16}}$
3	$1\frac{3}{8}\pm\frac{1}{16}$	$5^{+0}_{-\frac{1}{8}}$	$\frac{3}{4}\pm\frac{1}{16}$	$5\frac{3}{4}\pm\frac{1}{8}$	$1\frac{1}{16}\pm\frac{1}{8}$	$30°\pm5°$	$5^{+\frac{1}{8}}_{-\frac{5}{16}}$

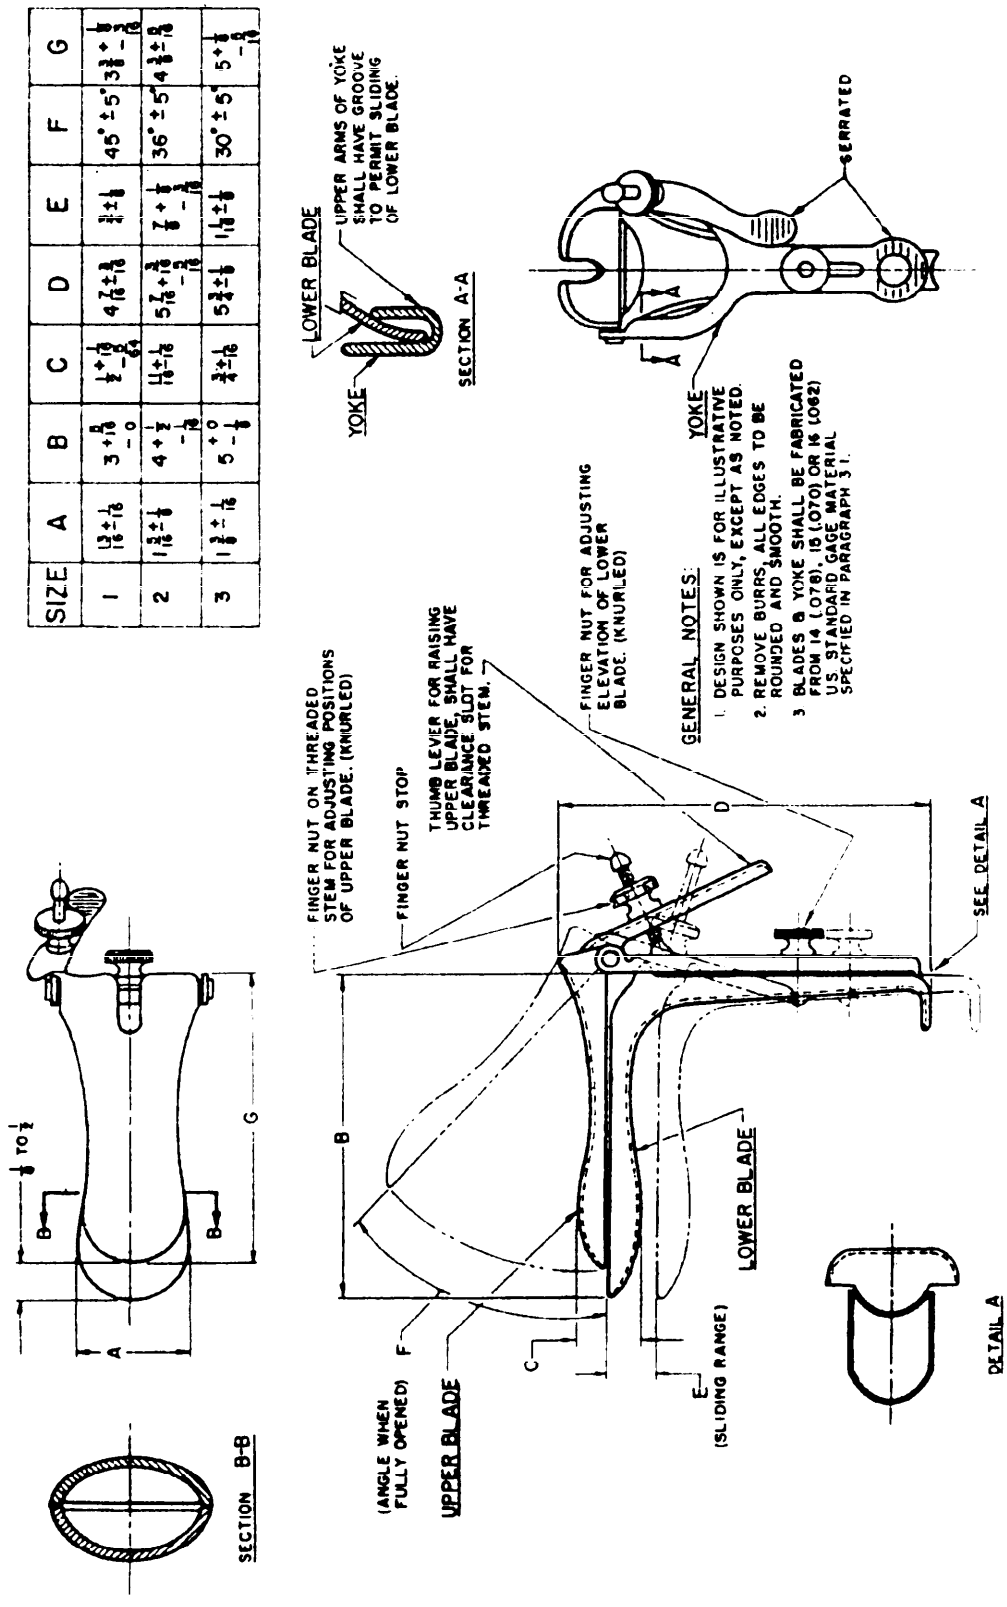


FIGURE 2.—Type I Graves.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

NOTE:

1. SHALL BE FABRICATED FROM No.15 GA (.070) OR No.16 GA (.062) US STANDARD GAGE MATERIAL SPECIFIED IN PARA 3.1.

SIZE	A	B	C	D	E	F	G
2	6 5/8 +1/4	2 3/8 +1/8	3 1/16 +1/8	1 +1/8	1 1/4 +1/16	9/16 +1/16	9/16 +1/16
4	7 1/16 +1/4	3 1/8 +1/8	3 3/8 +1/8	1 3/16 +1/8	1 3/8 +1/8	9/32 +1/16	5/8 +1/16

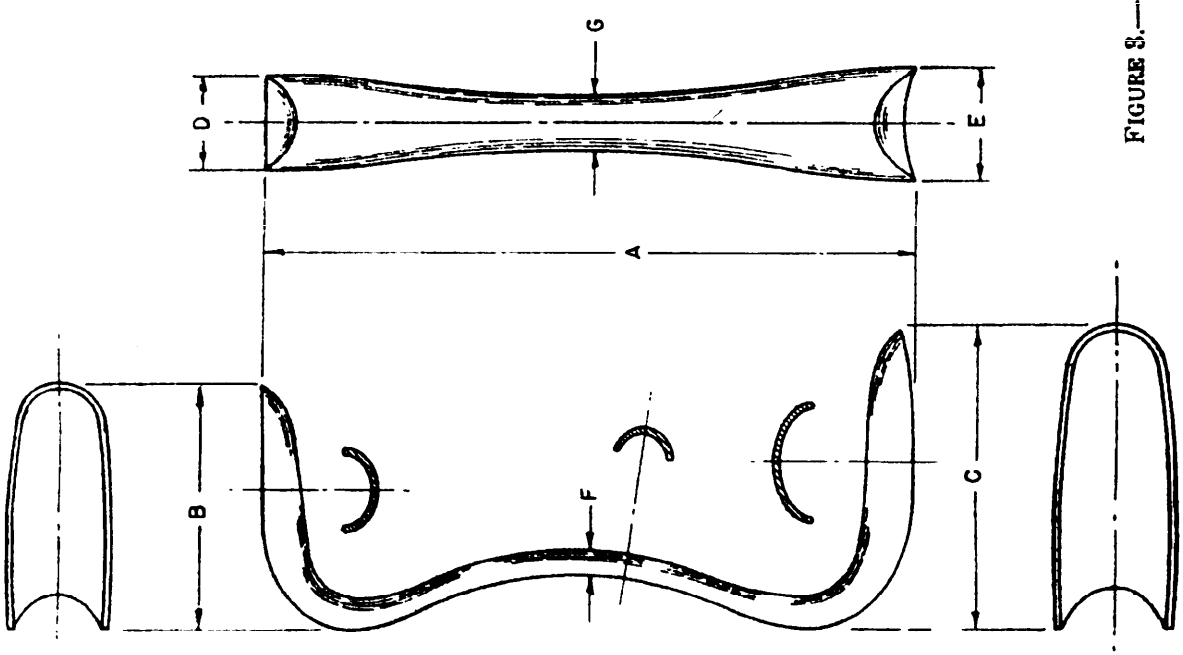


FIGURE 8.—Type II Sims.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

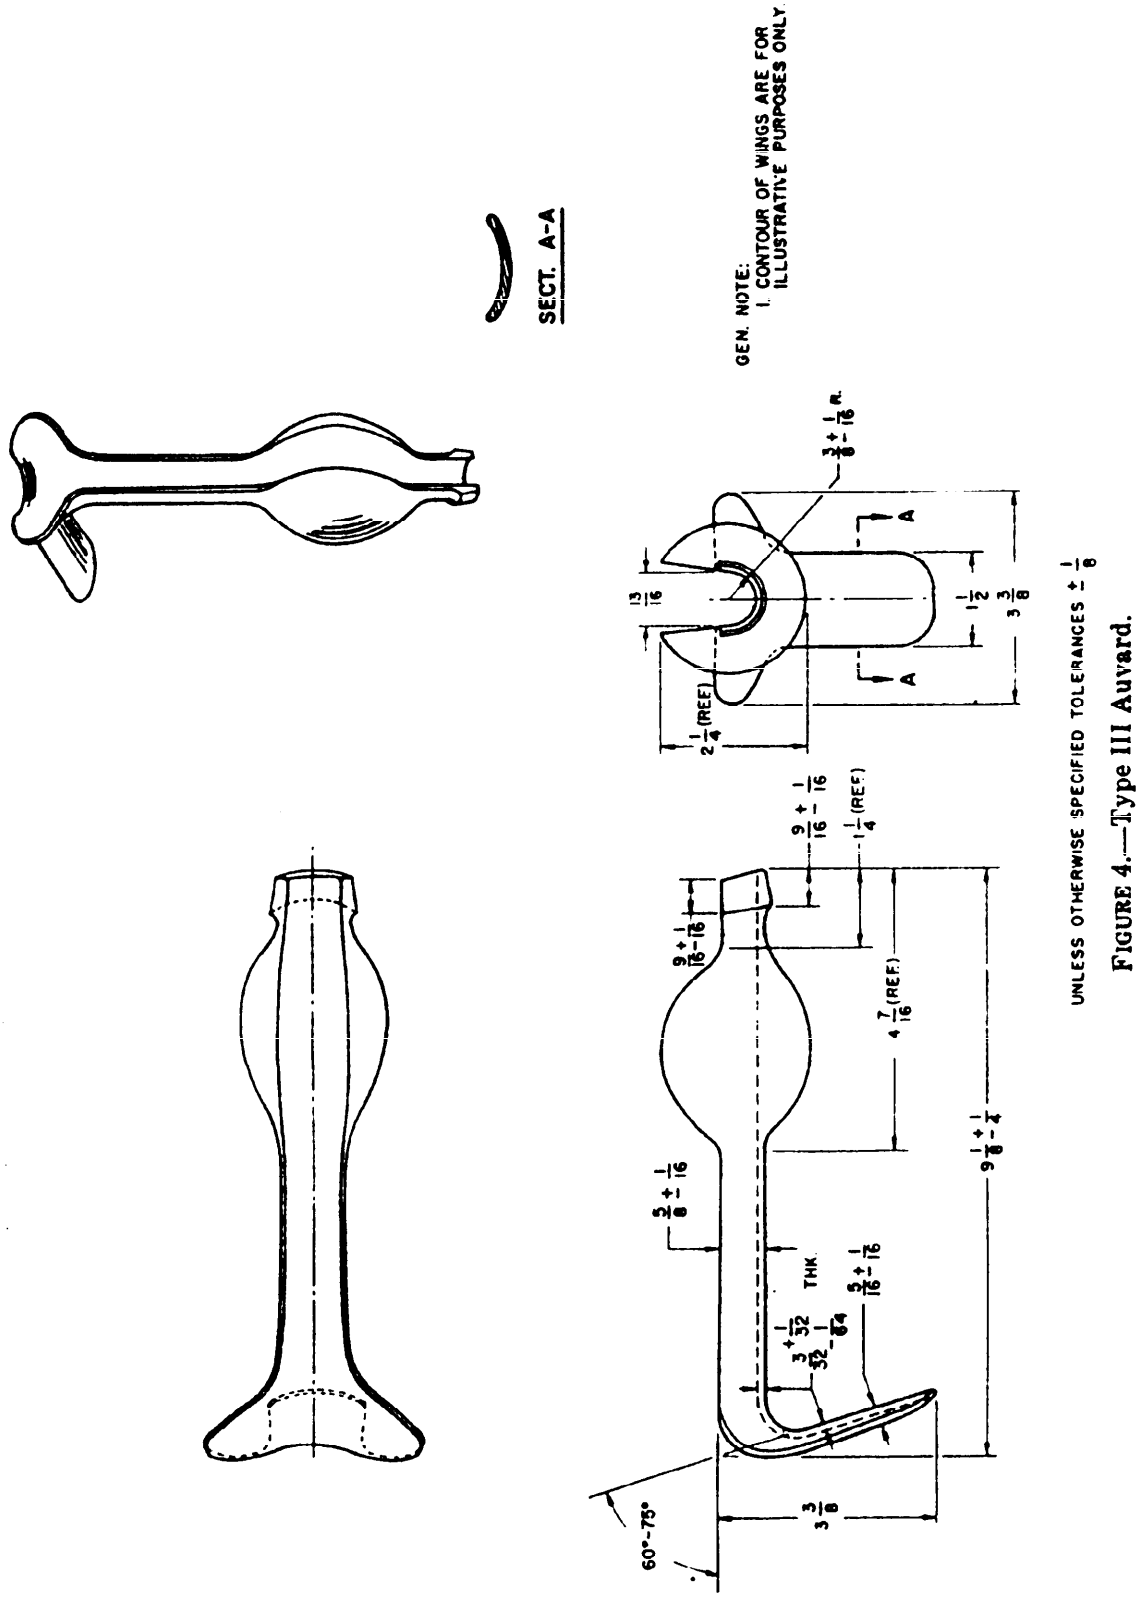


FIGURE 4.—Type III Auvard.

★ U. S. GOVERNMENT PRINTING OFFICE: 1960

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the currentversion before use.

50222 M/

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

NOTICE
OF CANCELLATION

GG-S-604
NOTICE 1
27 September 1991

FEDERAL SPECIFICATION

SPECULUM, VAGINAL

GG-S-604, dated November 8, 1960, is hereby cancelled and superseded by Commercial Item Description A-A-54301, dated December 14, 1990.

Preparing Activity:
DoD-MB
(Project No. 6515-5069)

AMSC N\A
FSC 6515
DISTRIBUTION STATEMENT A. Approval for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.