GG–T–626
MARCH 7, 1955
SUPERSEDING
Int. Fed. Spec. GG–T–00626 (GSA–FSS)
July 28, 1954

FEDERAL SPECIFICATION

TRAYS, IMPRESSION, DENTAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers dental-impression trays suitable for use in taking impressions in the oral cavity.

1.2 Classification.

1.2.1 *Types, classes and sizes.* — Impression trays covered by this specification shall be of the following types, classes and sizes, as specified in the invitation for bids:

Type I.—Trays, impression, crown and bridge.

Type II.—Trays, impression, edentulous.

Class 1.—Upper.

Size No. 41—Large.
Size No. 43—Medium.
Size No. 45—Small.

Class 2.—Lower.

Size No. 17B—Medium, narrow flange.
Size No. 51—Large.
Size No. 53—Medium.
Size No. 56—Small.

Type III.—Trays, impression, hydrocolloid.

Class 1.—Upper.

Sizes:
Large.
Medium-large.
Medium.
Small.

Class 2.—Lower.

Sizes:
Large.
Medium-large.
Medium.
Small.

Type IV.—Trays, impression, orthodontic.

Class 1.—Upper.

Sizes:
Large.
Medium.
Medium-small.
Small.

Class 2.—Lower.

Sizes:
Large.
Medium.
Small.

Type V.—Trays, impression, partial.

Class 1.—Upper (anterior).

Size No. 5A—Medium.
Size No. 6A—Small.

Class 2.—Lower.

Size No. 15A.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following Federal Specification of the issue in effect on date of invitation for bids, forms a part of this specification:

QQ–A–561—Aluminum (AL–2); Plate and Sheet.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

2.2 Specifications and standard applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Material.

3.1.1 *Aluminum.*

3.1.1.1 *Tray Body.*—The body for types I, II, IV, and V trays shall be fabricated of aluminum conforming to condition A of Federal Specification QQ–A–561, except that aluminum for size No. 17B tray of type II, shall conform to condition H of Federal Specification QQ–A–561.

3.1.1.2 *Handle.*—The handle for types I, II, IV, and V trays shall be fabricated of aluminum conforming to condition H of Federal Specification QQ–A–561.

3.1.2 *Brass.*—The body and handle for type III trays shall be fabricated of plain brass, suitable for the purpose.

3.2 Style and design.—The style and design of the various types of trays shall be as shown in figures 1 to 5, inclusive.

3.3 Type I, tray, impression, crown and bridge.

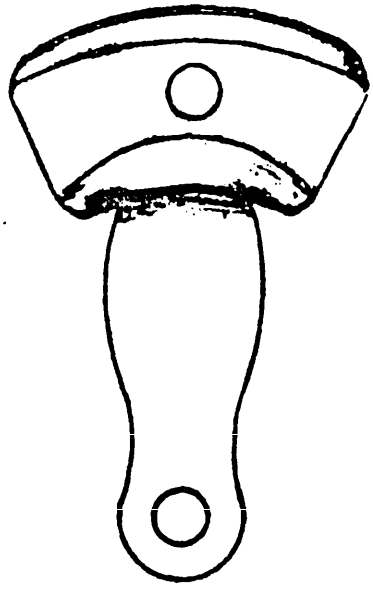


FIGURE 1.—Type I, tray, impression, crown and bridge.

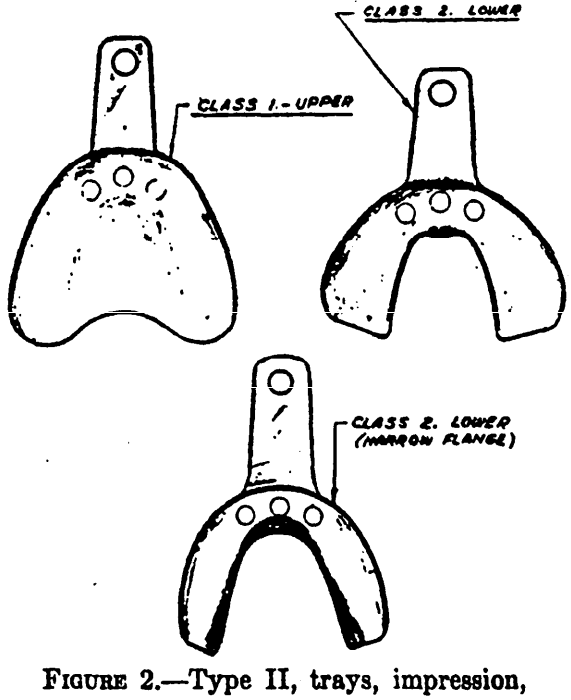


FIGURE 2.—Type II, trays, impression, edentulous.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the current version before use.

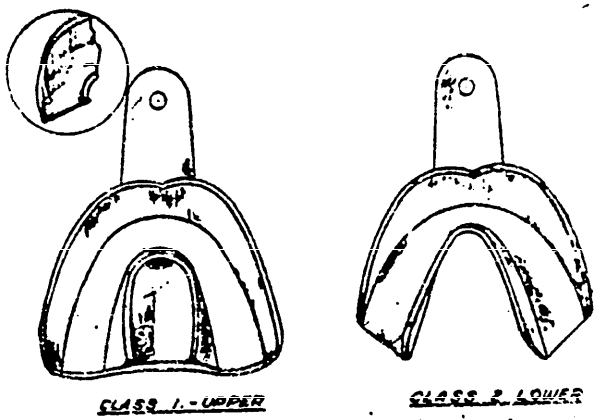


FIGURE 3.—Type III, trays, impression, hydrocolloid.

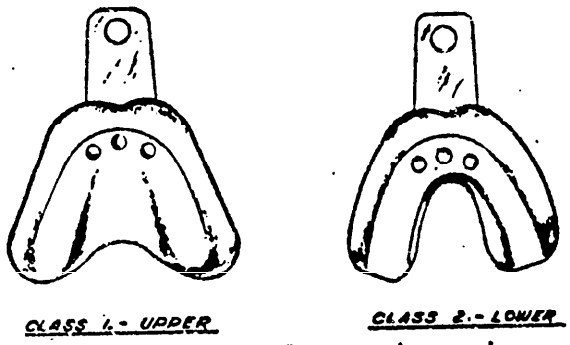


FIGURE 4.—Type IV, trays, impression, orthodontic.

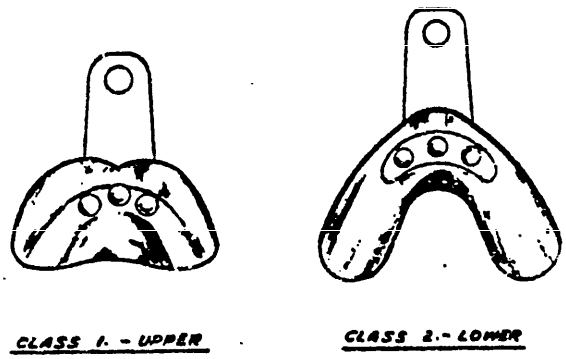


FIGURE 5.—Type V, trays, impression, partial.

3.3.1 *Description.* — The tray shall be suitable for taking impressions in the mouth for crown and bridge work. The handle shall be attached to the tray body by means of a rivet, and shall be of the swivel type. The tray shall conform to the dimensions in inches, as shown in table I.

TABLE I.—*Type I, tray, impression, crown and bridge*

Tray Body		Handle	
	Inches		*Inches*
Width at widest point	1⅞	Over-all length	2⅝
Over-all length	1	Width at widest point	¾
Height of lingual flange	9/16		
Height of labial-buccal flange	½		
Thickness	0.032-.040		

3.4 Type II, trays, impression, edentulous.

3.4.1 *Description.* — The trays shall be suitable for taking compound snap impressions of the edentulous mouth for obtaining study casts over which base-plate trays are made to get final impressions. The body of the trays shall conform to the dimensions for the particular class and size as shown in table II.

3.5 Type III, trays, impression, hydrocolloid.

3.5.1 *Description.* — The trays shall be suitable for taking full impressions of the teeth with elastic hydrocolloids, and shall be of rim-lock design with a solid surface. The handle shall be

TABLE II.—*Type II, trays, impression edentulous*

Class	Size	Tray Body: Width at widest point	Tray Body: Over-all Length	Tray Body: Height at cuspid area	Tray Body: Thickness
		Inches	*Inches*	*Inch*	*Inch*
1	41	3	2½	7/32	0.037-0.040
1	43	2 23/32	2⅜	21/64	0.037-0.040
1	45	2 17/32	2¼	9/32	0.037-0.040
2	17B	3 1/32	1 21/32	17/64	0.037-0.040
2	51	3 3/32	2⅜	21/64	0.037-0.040
2	53	2 31/32	2 9/16	9/32	0.037-0.040
2	56	2 15/16	2¼	5/16	0.037-0.040

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the current version before use.

TABLE III.—*Type III, trays, impression, hydrocolloid*

Class	Size	Tray Body: Width, Base	Width, Top	Length, Base	Length, Top	Lingual Width, Base	Lingual Width, Top	Height at cuspid area	Thickness
		Inches	*Inches*	*Inches*	*Inches*	*Inches*	*Inches*	*Inch*	*Inch*
1	Large	3⅛	3¼	2 7/16	2⅝	....	....	15/16	0.013-0.020
1	Medium large	2 15/16	3	2¼	2 3/16	....	....	15/16	0.013-0.020
1	Medium	2 13/16	2 15/16	2⅛	2 1/16	....	....	15/16	0.013-0.020
1	Small	2 9/16	2¾	2	1 15/16	....	....	15/16	0.013-0.020
2	Large	3⅛	....	2 7/16	2½	1⅝	1 5/16	15/16	0.013-0.020
2	Medium large	3	....	2 5/16	2⅝	1 9/16	1¼	15/16	0.013-0.020
2	Medium	2⅞	....	2 5/16	2¼	1½	1 5/16	15/16	0.013-0.020
2	Small	2¾	....	2 1/16	2⅛	1 7/16	1⅛	15/16	0.013-0.020

soldered to the body of the trays. The body of the trays shall conform to the dimension for the particular class and size as shown in table III. Unless otherwise specified, dimensions are outside or maximum measurements.

3.6 Type IV, trays, impression, orthodontic.

3.6.1 *Description.* — The trays shall be suitable for taking impressions for orthodontic work, and the body of the trays shall conform to the dimensions for the particular class and size as shown in table IV.

3.7 Type V, trays, impression, partial.

3.7.1 *Description.*—The trays shall be suitable for taking individual impressions in difficult cases which cannot be readily obtained with standard rigid trays. The body of the trays shall conform to the dimensions for the particular class and size as shown in table V.

3.8 Handle. — Unless otherwise specified herein, the handle shall be securely attached to the body of the trays by means of three rivets. The handle for all types of trays, except type I, shall taper in width from ⅞ inch at proximal end to 1 1/16 inch at distal end, and shall extend from tray body for a distance of 1⅝ inches. The length and width of handle for type I tray shall be as shown in table I. The handle for all five types of trays shall be 0.048 to 0.052 inch in thickness, and shall have a hole approximately ¼ inch in diameter located in the distal end for hanging the trays on a tray board.

TABLE IV.—*Type IV, trays, impression, orthodontic*

Class	Size	Tray Body: Width at widest point	Over-all length	Height at cuspid area	Thickness
		Inches	*Inches*	*Inch*	*Inch*
1	Large	2 15/16	2 11/16	25/32	0.037-0.040
1	Medium	2⅞	2⅝	¾	0.037-0.040
1	Medium small	2⅞	2 7/16	19/32	0.037-0.040
1	Small	2⅝	2⅛	½	0.037-0.040
2	Large	3 5/16	2⅝	¾	0.037-0.040
2	Medium	3 1/16	2 5/16	19/32	0.037-0.040
2	Small	2 13/16	1 15/16	½	0.037-0.040

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

TABLE V.—*Type V, trays, impression, partial*

Class	Size	Tray Body: Width at widest point	Tray Body: Over-all length	Tray Body: Height at cuspid area	Tray Body: Thickness
		Inches	*Inches*	*Inch*	*Inch*
1	5A	2½	1⅝	⅝	0.032-0.040
1	6A	2¼	1¼	⅝	0.032-0.040
2	15A	2 15/16	2 1/16	⅝	0.032-0.040

3.9 Tolerances.—Unless otherwise specified herein, dimensions on body of trays and handles shall have a tolerance of plus or minus 1/16 inch.

3.10 Bend test.—The body of the trays fabricated of soft temper aluminum (see 3.1.1) shall not crack when subjected to the bend test described in 4.3.1.

3.11 Identification marking.—Each tray shall be permanently and legibly marked on the handle with the respective size or size number as shown in the applicable table, and the name or registered trade-mark of the manufacturer.

3.12 Finish.—Aluminum trays shall be polished to a smooth, bright finish. Brass trays shall be either nickel or chromium over nickel plated, and shall be polished to a bright finish.

3.13 Workmanship.—Workmanship shall be first class throughout. The trays shall be uniform in quality and temper, smooth and free from buckles, seams, cracks, or other defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION AND TEST PROCEDURES.

4.1 Sampling.—Unless otherwise specified, not less than five trays of each type, class, and size shall be taken at random from each delivery for inspection and test.

4.2 Inspection.—Each sample shall be inspected for type, class, size, material, description, style and design, handle, identification marking, finish, workmanship, packaging, packing and marking.

4.3 Tests.—Tests shall be conducted in accordance with the requirements of Federal Specification QQ–A–561.

4.3.1 *Bend test.*—The body of the trays shall be bent flat on itself, either parallel with, or transversely to, the direction of final rolling.

5. PREPARATION FOR DELIVERY

5.1 Packaging.—Unless otherwise specified, trays shall be packaged in accordance with accepted commercial practice.

5.2 Packing.—The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 Packages.—Unless otherwise specified, packages shall be marked with the name and size of the commodity, the quantity contained therein, and the name of the manufacturer and contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 Ordering data.—Purchasers should specify types, classes, and sizes required, and should

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

exercise any desired options offered herein. (See 1.2.1, 3.8, 3.9, 4.1, 5.1, 5.3, 6.3, and 7.2.5.)

6.2 This specification covers the following items appearing in the Armed Services Medical Stock List.

6520–562–2000	Impression Tray, Dental, Crown and Bridge.
6520–562–4150	Impression Tray, Dental, Edentulous, Lower No. 51.
6520–562–4650	Impression Tray, Dental, Edentulous, Lower No. 53.
6520–562–5150	Impression Tray, Dental, Edentulous, Lower No. 56.
6520–562–6150	Impression Tray, Dental, Edentulous, Upper No. 17B.
6520–562–7650	Impression Tray, Dental, Edentulous, Upper No. 41.
6520–562–8150	Impression Tray, Dental, Edentulous, Upper No. 43.
6520–562–9650	Impression Tray, Dental, Edentulous, Upper No. 45.
6520–563–0150	Impression Tray, Dental, Hydrocolloid, Lower, Large.
6520–563–0650	Impression Tray, Dental, Hydrocolloid, Lower, Medium.
6520–563–1150	Impression Tray, Dental, Hydrocolloid, Lower, Medium-Large.
6520–563–1650	Impression Tray, Dental, Hydrocolloid, Lower, Small.
6520–563–2150	Impression Tray, Dental, Hydrocolloid, Upper, Large.
6520–563–2650	Impression Tray, Dental, Hydrocolloid, Upper, Medium.
6520–563–3150	Impression Tray, Dental, Hydrocolloid, Upper, Medium-Large.
6520–563–3650	Impression Tray, Dental, Hydrocolloid, Upper, Small.
6520–563–4150	Impression Tray, Dental, Orthodontic, Lower, Large.
6520–563–5150	Impression Tray, Dental, Orthodontic, Lower, Medium.
6520–563–5650	Impression Tray, Dental, Orthodontic, Lower, Small.
6520–563–6000	Impression Tray, Dental, Orthodontic, Upper, Large.
6520–563–8000	Impression Tray, Dental, Orthodontic, Upper, Medium.
6520–563–9000	Impression Tray, Dental, Orthodontic, Upper, Medium-Small.
6520–564–0000	Impression Tray, Dental, Orthodontic, Upper, Small.
6520–564–1150	Impression Tray, Dental, Partial, Anterior, Medium.
6520–564–1650	Impression Tray, Dental, Partial, Anterior, Small.
6520–564–2150	Impression Tray, Dental, Partial, Lower.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine conformance to the requirements of this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 Federal specifications do not include all types, classes, grades, sizes, etc., of the commodities indicated by the titles of the specifications, or which are commercially available, but are intended to cover the types, etc., which are suitable for Federal Government requirements.

6.5 Transportation description.—Transportation description applicable to this item is:

Dental goods, not otherwise indexed by name.

Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Truckload minimum weight 12,000 pounds.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:52Z
Check the source to verify that this is the current version before use.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications and standards, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications and standard.*

Federal Specifications:

NN–B–621—Boxes, Wood, Nailed and Lock-Corner.
NN–B–631—Boxes; Wood, Wirebound (for Domestic Shipment).
PPP–B–601—Boxes, Wood, Cleated-Plywood.
PPP–B–676—Boxes, Set-Up, Paperboard.

Military Specifications:

JAN–P–106—Packaging and Packing for Overseas Shipment—Boxes; Wood Nailed.
MIL–B–107—Boxes, Wood, Wirebound (Overseas Type).
JAN–P–120—Packaging and Packing for Overseas Shipment — Cartons, Folding, Paperboard.
MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.
MIL–L–10547—Liners, Case, Waterproof.

Military Standard:

MIL–STD–129—Marking for Shipment and Storage.

(Copies of specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

7.2.2 *Packaging.*

7.2.2.1 *Unit of issue.*—One tray, of the stock number specified, constitutes one unit.

7.2.2.2 *Unit packaging.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with the requirements of Military Specification JAN–P–120 or Federal Specification PPP–B–676. Each carton shall be adequately secured to prevent accidental opening.

7.2.2.3 *Intermediate packaging.* — Twelve unit cartons either shall be packaged in a carton of appropriate size and design, or be completely wrapped with kraft paper of suitable weight. Carton and wrapping shall be adequately secured to prevent accidental opening.

7.2.3 *Packing.*

7.2.3.1 *For domestic shipment.* — Twenty-four intermediate packages (288 units) of one stock number shall be overpacked in an exterior container. Construction, closure, and strapping (when required) shall be in accordance with the requirements of Federal Specification NN–B–621, NN–B–631, or Military Specification MIL–B–10377 (table I), for type 2 load; or Federal Specification PPP–B–601 (table I, type III, class 1 plywood).

7.2.3.2 *For overseas shipment.*—Twenty-four intermediate packages (288 units) of one stock number shall be overpacked in an exterior container designed for type 2 load and constructed in accordance with the requirements of Military Specification JAN–P–106, MIL–B–107, or MIL–B–10377 (table II); or Federal Specification PPP–B–601 (table II, type III, class 1 plywood).

7.2.3.2.1 *Case liner.* — Each overseas box shall be lined with a waterproof case liner conforming to the requirements of Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

7.2.3.2.2 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

NOTE: Strapping will not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

7.2.3.3 *Packing variation permitted.*—If the number of units in any shipment is less than the specified number of units to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design which will insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:52Z
Check the source to verify that this is the current version before use.

7.2.4 *Marking.*

7.2.4.1 *Unit carton.*—Each unit carton shall be marked with the stock number, nomenclature, unit, quantity, and name of the contractor.

7.2.4.2 *Intermediate packages and shipping containers.*—Each intermediate package and each shipping container shall be marked in accordance with Military Standard MIL–STD–129.

7.2.5 *Ordering data.*—Requests, requisitions, schedules, and contracts or orders should specify whether the subject commodity is to be packed for domestic or overseas shipment. (See 7.2.3.1 and 7.2.3.2.)

MILITARY INTEREST:
Navy—Md
Army—M
Air Force—USAF.

Copies of this specification may be purchased for 10 cents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.