A-A-53713
30 September 1988

COMMERCIAL ITEM DESCRIPTION

STONE, SHARPENING (Soft Arkansas)

The General Services Administration has authorized the use of this Commercial Item Description.

Salient characteristics.

This commercial item description covers a natural stone suitable for sharpening dental instruments.

The stone shall be a round edge, slip style soft Arkansas sharpening stone composed of natural, abrasive Novaculite in soft(super fine) grit. The stone shall be quarried from high quality deposits, shall be precision sawed to size, and shall contain no flaws or substandard material. The stone shall be capable of producing a final, finished edge after prior sharpening with aluminum oxide abrasives. Specific gravity of the stone shall be 2.30 (minimum) to 2.50 (maximum). Style, design, and dimensions shall be in accordance with figure 1.

Identification marking. Each stone shall be prominently marked with the manufacturer's name or registered trademark. The stone or immediate container shall be marked or labeled to indicate that, when using the stone, lubrication with oil is required.

Workmanship. The sharpening stone shall possess sufficient strength to withstand normal service without chipping, breaking, or otherwise becoming damaged. The stone shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One sharpening stone, as specified, constitutes one unit.


Quality Assurance Provisions

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the contractor may use his own or any other facilities for the performance of the inspection requirements specified herein, unless disapproved by the Government.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

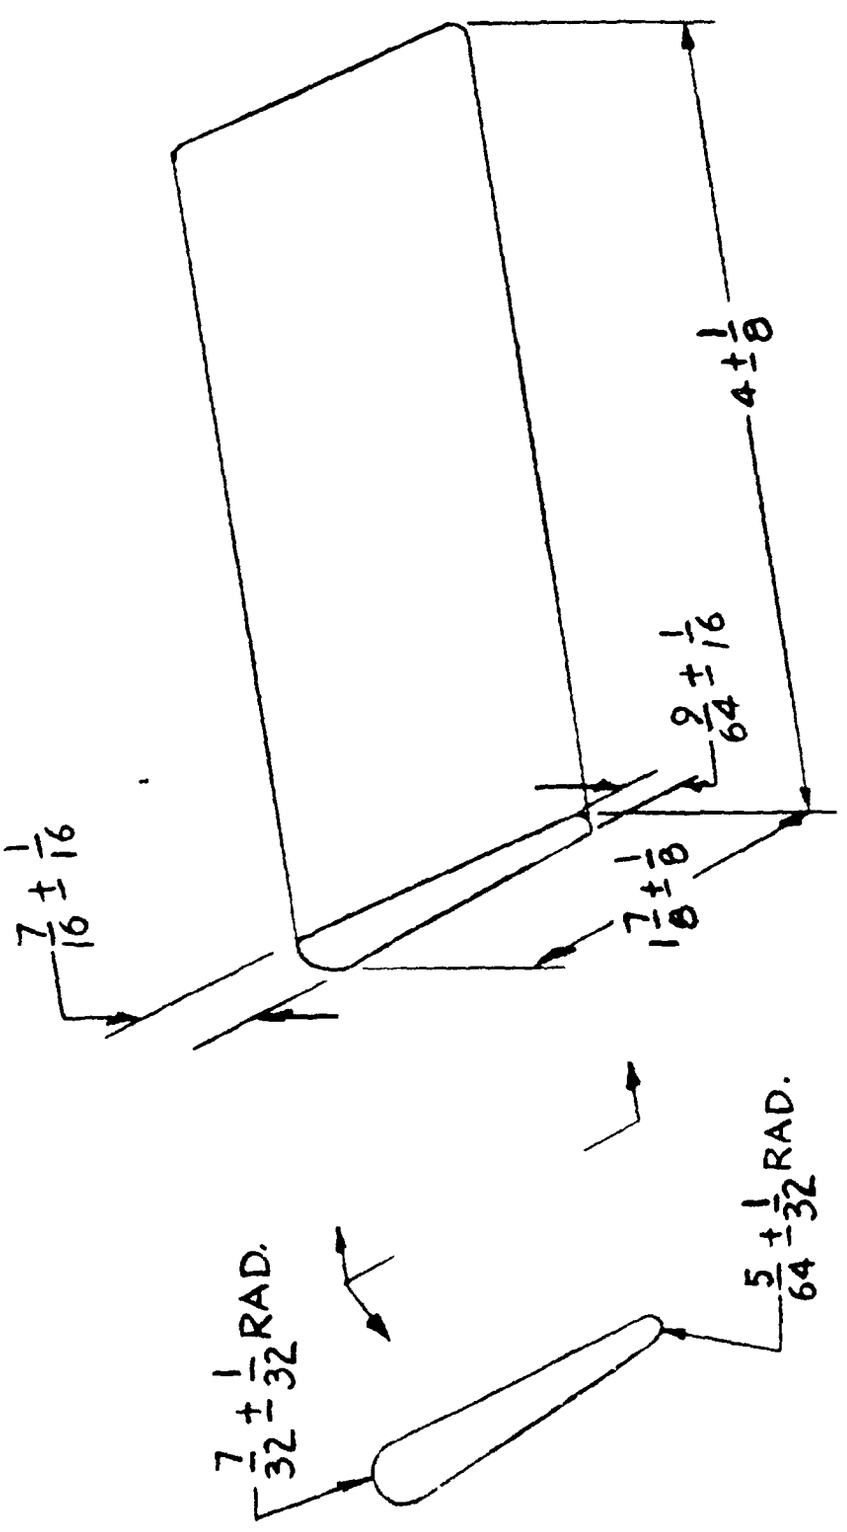


NOTE:
UNLESS OTHERWISE SPECIFIED
ALL DIMENSIONS ARE IN INCHES.

FIGURE 1 STONE, SHARPENING



Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government.

Sampling.

For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 with an AQL of 2.5 (percent defective) and an inspection level of S-2. The unit of product for examination purposes shall be one stone.

For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 at inspection level S-1, AQL 1.0 (percent defective). The unit of product for test purposes shall be one stone.

Examination. The stones shall be examined to determine compliance with specification requirements. The stones shall be examined for defects including, but not limited to those listed below.

Defects

Style or design of stone not as specified.
Stone has cracks, breaks, chips, or other defects affecting function or serviceability.
Dimensions of stone not as specified.
Identification marking or labeling not as specified.

Tests. Tests shall be conducted to determine compliance with specification requirements.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

Specific gravity. Weigh a dry sample of stone. Dip sample in molten paraffin wax, until completely coated, and weigh again. Reweigh coated sample under water. Calculate the specific gravity of the stone as follows:

$$\text{Specific gravity} = \frac{A}{B-\left(\frac{B-A}{S}+C\right)}$$

A = Weight of sample
B = Weight of coated sample
C = Weight of submerged sample
S = Specific gravity of paraffin

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to contents and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

| National Stock Number | Item Identification |
|---|---|
| 6520-01-264-1329 | STONE, SHARPENING, Dental Instrument, Soft Arkansas, Novaculite, Round Edge, Slip Style, 4 inch (10.2 cm) Long, 1.9 inch (4.8 cm) Wide |

Ordering data. Intermediate/exterior package quantities and labeling and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-2178

LOCATION: NCR Disk No. 7

61311



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1 DOCUMENT NUMBER | 2 DOCUMENT TITLE |
|---|---|
| A-A-53713 | STONE, SHARPENING (Soft Arkansas) |

| 3a NAME OF SUBMITTING ORGANIZATION | 4 TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR |
| | ☐ USER |
| b ADDRESS *(Street City State ZIP Code)* | ☐ MANUFACTURER |
| | ☐ OTHER *(Specify)* |

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

| 7a NAME OF SUBMITTER *(Last First MI)* – Optional | b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c MAILING ADDRESS *(Street City State ZIP Code)* – Optional | 8 DATE OF SUBMISSION *(YYMMDD)* |

*(TO DETACH THIS FORM CUT ALONG THIS LINE.)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS** In a continuing effort to make our standardization documents better the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

*NOTE* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

*(Fold along this line)*

*(Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

**BUSINESS REPLY MAIL**
FIRST CLASS PERMIT NO 4966 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:23Z
Check the source to verify that this is the current version before use.