MIL-S-16297A
10 APRIL 1961
SUPERSEDING
MIL-S-16297(BUMED)
1 MAY 1951

MILITARY SPECIFICATION

STAND, SHELF, CORROSION-RESISTING STEEL

This specification has been approved by the Department of Defense and is mandatory for use by the Departments of the Army, the Navy, and the Air Force.

1. SCOPE

1.1 This specification covers one type of corrosion-resisting steel shelf stand, suitable for use in surgical operating rooms to hold various operating room equipment and supplies.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

UU-P-271 — Paper, Wrapping, Waterproofed Kraft.
PPP-B-585 — Boxes, Wood, Wirebound.
PPP-B-601 — Boxes, Wood, Cleated-Plywood.
PPP-B-621 — Boxes, Wood, Nailed and Lock-Corner.

STANDARDS

FEDERAL

Fed. Std. No. 66 — Steel: Chemical Composition and Hardenability.
Fed. Test Method Std. No. 151 — Metals; Test Methods.

MILITARY

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 — Marking for Shipment and Storage.

(Copies of specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. All sheet and tubing used in the manufacture of the stands shall conform to AISI 302 or 304 corrosion-resisting steel of Federal Standard 66. Commercial tolerances on gage sizes shall apply.

3.2 Construction. Stand shall conform to figure 1, and shall consist of a tubular framework for holding four equally spaced shelves.

3.2.1 *Frame.* Frame shall consist of 1-inch-outside-diameter, 0.0625-inch-thick (No. 16, United States Standard (U.S.S.) gage) tubing, mounted on adjustable corrosion-resisting-steel or cadmium-plated carbon steel glides. The two rear legs forming the back supports shall be straight. The two front legs shall be curved diagonally inward, midway between the second and third shelves to allow for the reduced width

FSC 6530

871074—61—(X-122)

Source: https://assist.dla.mil -- Downloaded: 20261O-18T08:34Z
Check the source to verify that this is the current version before use.

of the two upper shelves. All tubing shall be closed flush at the top by welding.

3.2.2 *Shelves.* There shall be four shelves of 0.0625-inch-thick (No. 16, U.S.S. gage) corrosion-resisting steel. All shelves shall be closely welded to the uprights with all joints ground smooth. Corners shall be notched on a ½-inch radius to fit the contour of the legs, so that no opening remains. All edges of the shelves shall be flanged downward 1 inch and hemmed not less than ⅝ inch. Welding shall be as shown on figure 1. All exposed welds shall be ground and polished to blend with the adjacent areas.

3.2.3 *Guardrails.* Guardrails of ⅜-inch rod shall be welded to the tubular frame uprights as shown on figure 1.

3.3 Finish. All exposed surfaces shall be finished in a No. 4 commercial grind polish.

3.4 Identification marking. Each stand shall be permanently and legibly marked with the name or registered trademark of the manufacturer, the contract or purchase order number, and the letters U.S.

3.5 Workmanship. Workmanship shall be first class throughout. Stands shall be free from any defects which affect their appearance or may impair their serviceability. Forming shall be neatly done without scratches or tears.

3.5.1 *Welding.* The welding shall be electric arc or oxyacetylene, continuous on all contact surfaces, using welding rod of composition similar to the parent metal. Welds shall be thorough, nonporous, cleaned, ground, and finished smooth to match adjoining surfaces. Welds shall be free from pit marks and imperfections. All surfaces shall be free from sharp edges.

4. QUALITY ASSURANCE PROVISIONS

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform all the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 *For examination.* Sampling for examination shall be conducted in accordance with Standard MIL-STD-105.

	Inspection level	*AQL (defects per hundred)*
For visual examination		
Major defects	II	1.0
Total (Major and Minor A combined) defects	II	4.0
Minor B defects	L5	2.5
For dimensional examination	L5	2.5

4.2.2 *Raw materials.* Four ounces of each lot of metal used in the construction of the stands shall be selected for chemical analysis.

4.3 Examination. The stands shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 *Classification of defects.* Examination shall be conducted in accordance with the following classification of defects:

Categories and defects *
Major
101. Components not properly aligned and fitted.
102. Metal parts not free of cracks, tears, ruptures, and deformed surfaces.
103. All edges of shelves not flanged and hemmed as specified.

Source: https://assist.dla.mil -- Downloaded: 20261O-18T08:34Z
Check the source to verify that this is the current version before use.

Minor A

201. Exposed and accessible edges, corners, and surfaces not free of burs, sharpness, and sharp projections.
202. Finish not uniform and not free of coarse grind marks and scratched areas.
203. Welds not continuous, not sound, and not free of pitting, splatter, and discoloration.
204. Welds not ground smooth to blend with adjacent surfaces.
205. Uprights not closely fitted to notched shelf corners.
206. Unit not clean.

Minor B

251. Design and construction not in accordance with figure 1.
252. Unit not complete with all component parts.
253. Glides not adjustable in height.
254. Identification marking not complete, not legible, and not permanently attached.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 *Dimensional examination.* The stands shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 *Chemical composition.* Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard 151.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 *Level A.*

5.1.1.1 *Unit of issue.* One (1) stand, as specified, constitutes one unit of issue.

5.1.1.2 *Unit preparation.* Exterior finished surfaces shall be protected by wrapping with kraft paper or by a kraft paper shroud, and by cushioning at points of contact of interior braces or interior faces of container with flexible corrugated fiberboard or other suitable materials. Wrapping and cushioning material shall be secured in position. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit.

5.1.2 *Level C.* Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.* Each unit shall be overpacked in an exterior container designed for type 3 load, and constructed in accordance with Specification PPP-B-585, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; or PPP-B-621, table IV. Closure and strapping shall comply with appendix of applicable specification. Each unit shall be protected with a shroud fabricated of waterproof barrier material conforming to Specification UU-P-271, class E-2, M-2, or M-3. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, blocks, or other suitable devices to insure against shifting and breakage, or marring of surfaces.

5.2.2 *Level B.* Each unit shall be overpacked in an exterior container designed for type 3 load, and constructed in accordance with Specification PPP-B-585, style 3, for class 2 use; PPP-B-601, table I, using type III, class 1 plywood; or PPP-B-621, table II. Closure shall comply with appendix of applicable specification. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, blocks, or other suitable devices to insure against shifting and breakage, or marring of surfaces.

5.2.3 *Level C.* The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or order.

5.3 Marking. Exterior container shall be marked in accordance with Standard MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 202640-18T08:34Z
Check the source to verify that this is the currentversion before use.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

6.3 Transportation description applicable to this item is:

Stands, NOIBN, set up in packages

Carload minimum weight varies as spec. in Uniform Freight Classification.

Truckload minimum weight 12,000 pounds per National Motor Freight Classification.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Custodians:

Army—Med
Navy—BuMed
Air Force—AFCSG

Preparing activity:

Navy—BuMed (MMSA)

Source: https://assist.dla.mil -- Downloaded: 2026-10-18T08:34Z
Check the source to verify that this is the current version before use.

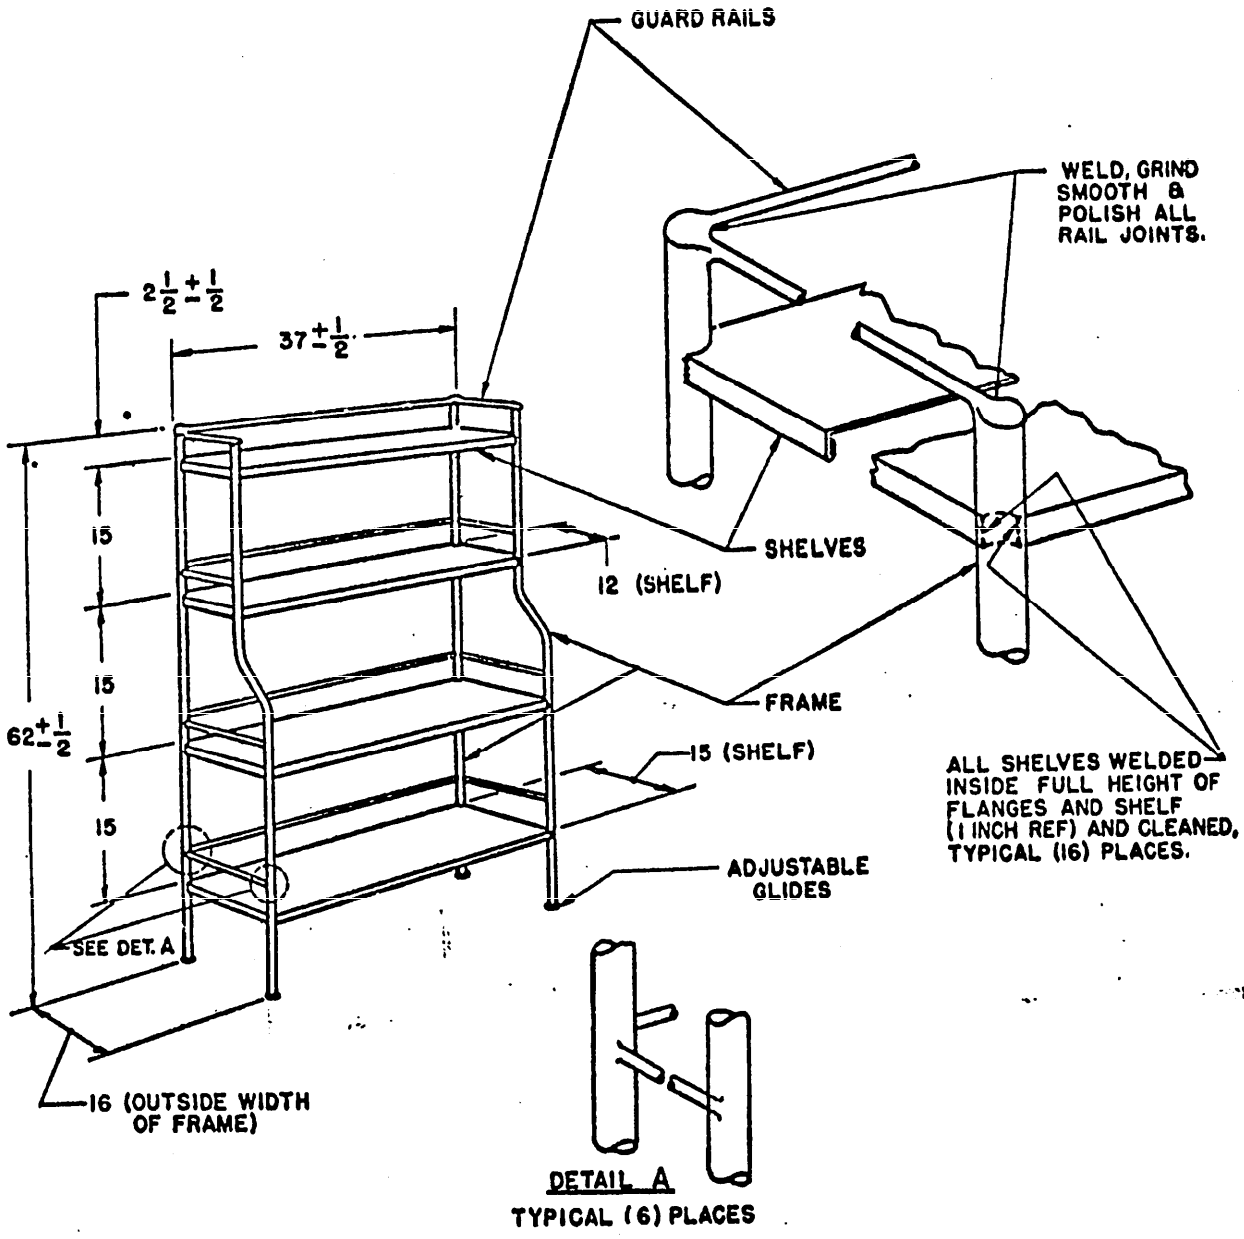


FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 2026l0-18T08:34Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-18T08:34Z
Check the source to verify that this is the current version before use.