MILITARY SPECIFICATION

FORCEPS, LUNG GRASPING, COLLIN, 8 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers a lung grasping forceps of the Collin design, suitable for use in grasping the lung during thoracic surgery.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The forceps shall be in accordance with the applicable requirements of GG-I-526, and the following option exercises under that specification.

3.2 Material. The forceps shall be fabricated from Class 4, Type 410 or Type 420 material.

3.3 Hardness. After proper stress relieving, the Rockwell hardness for the forceps shall be C-40 to C-45.

3.4 Style, design and dimensions. Shall be a lung grasping forceps, of the Collin design. The style, design and dimensions of the forceps shall conform to Figure 1.

3.4.1 Locks. Shall be box lock type. Forceps of box lock construction shall have shanks tested for lock stiffness in accordance with GG-I-526.

3.5 Finish. Shall be mirror finish.

3.6 Identification marking. Instruments of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 20260-21T09:56Z
Check the source to verify that this is the current version before use.

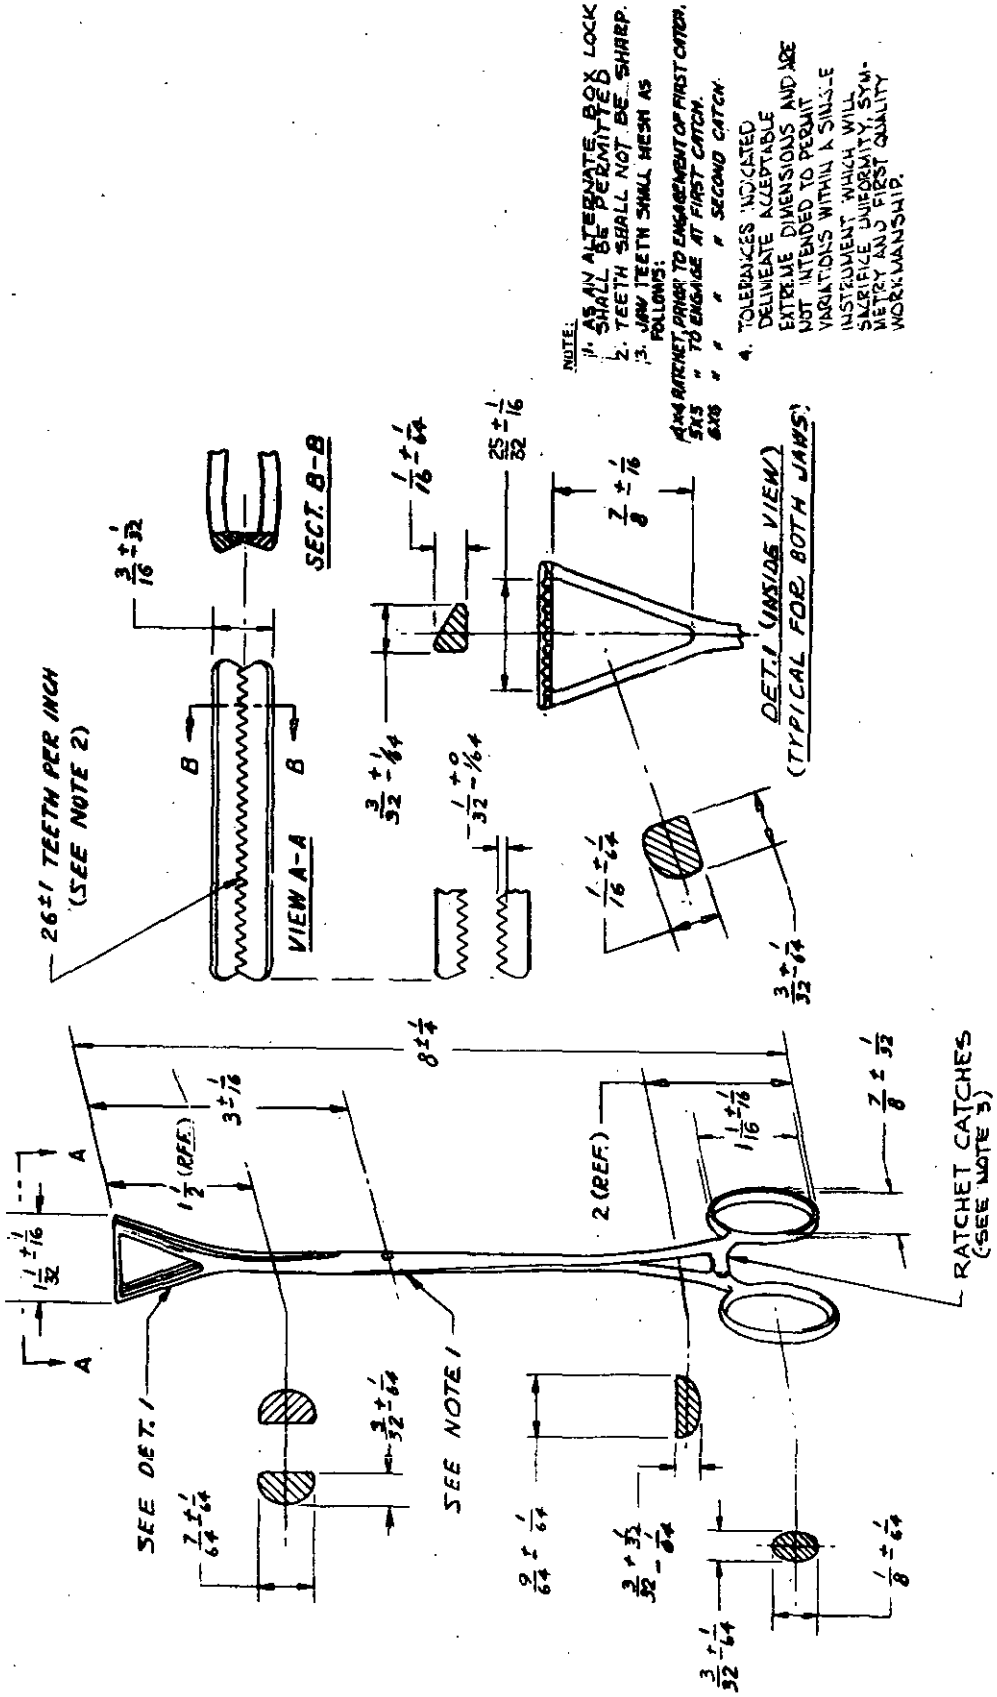


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:56Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Shall be in accordance with GG-I-526.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection level and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one forceps.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Table II. Sampling for tests

Unit of product	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Entire forceps	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*
	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.0
	Dimensions	3.4	---	S-1	2.5
	Copper sulfate	GG-I-526	GG-I-526	S-2	1.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0
	Box lock test	3.4.1	GG-I-526	S-2	1.0

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:56Z
Check the source to verify that this is the currentversion before use.

* Acceptance number shall be zero for all sample sizes.
** Sufficient amount from each lot of each metal used in the construction of the forceps shall be selected for composition analysis.

4.3 Examination. The forceps shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Instrument not constructed as specified.
103	Instrument not free from sharp edges, rough areas, burrs, cracks, grind marks or overlaps.
104	Serrations not free of foreign matter.
105	Ratchet teeth not uniform or function poorly.
106	Forceps of box lock design not free from excessive play in box lock area.
Minor	
201	Finish not as specified.
202	Instrument not permanently and legibly marked with either the name or trademark of the contractor.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of defects per hundred units.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.

Table IV. Examination of preparation for Delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted; incorrect; illegible; improper size, location, sequence, or method of application.
Materials	Component missing or damaged.
Workmanship	Bulging or distortion of containers.
	Cushioning inadequate, improper or missing.

4.5.1 Examination of closure and reinforcement for containers. When shipping containers are required to comply with PPP-B-636, examination for defects in closure and reinforcement shall be in accordance with the appendix to that specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. Each forceps, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable methods as outlined in MIL-P-116.

5.1.2.2 Preservative. Preservative shall not be utilized.

5.1.2.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.2.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.2.5 Intermediate package. Twelve unit packages shall be packaged in a snug fitting intermediate package constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be levels A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Forty eight intermediate packages (576 units) shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Fiberboard boxes shall conform to the special requirements as specified in PPP-B-636.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberbaord boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Forty eight intermediate packages (576 units) shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1, PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Fiberboard boxes shall conform to special requirements specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2.4 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package, and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The forceps are intended for use in grasping the lung during thoracic surgery.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-335-9100	FORCEPS, LUNG GRASPING, COLLIN, 8 INCH

It does not include all types or sizes as indicated by the title or all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 7 dated 26 June 1967 for FSN 6515-335-9100, Forceps, Lung Grasping, Collin, 8 inch.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1861

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:56Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
hiladelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:56Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:56Z
Check the source to verify that this is the current version before use.