MILITARY SPECIFICATION

FORCEPS, OBSTETRICAL, SIMPSON

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers one type of an obstetrical forceps of the Simpson design, suitable for use in obstetrical procedures.

1.2 Classification. The obstetrical forceps of the Simpson design shall be of the following sizes:

Size 1 - 12 inch
Size 2 - 14 inch

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up.

Military

MIL-P-116	Preservation, Methods of.
MIL-I-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:57Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The obstetrical forceps shall be in accordance with the applicable requirements of GG-I-526, and the following option exercises under that specification:

3.2 Material. The obstetrical forceps shall be fabricated from Class 4, Type 410 or Type 420 material.

3.3 Hardness. After proper stress relieving, the Rockwell hardness of the obstetrical forceps shall be C40 to C45.

3.4 Style, design, and dimensions. Shall be an obstetrical forceps, Simpson standard sliding type, with curved, hand forged blades and smooth, hollowed out handles. The style, design, and dimensions of the obstetrical forceps shall conform to Figure 1.

3.5 Finish. The finish shall be mirror, or mirror and satin.

3.6 Identification Marking. Instruments of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:57Z
Check the source to verify that this is the currentversion before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Shall be in accordance with GG-I-526.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the stainless steel may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the material, the lot number, the lot size, the sample size the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one forceps.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:57Z
Check the source to verify that this is the current version before use.

Table II. Sampling for Tests

Component (unit of product)	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
1-Forceps	Composition	3.2 and GG-I-526	GG-I-526	**	*
1-Forceps	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.5
1-Forceps	Dimensions	3.4	--------	S-1	3.5
1-Forceps	Copper sulfate	GG-I-526	GG-I-526	S-2	1.5
1-Forceps	Boil test	GG-I-526	GG-I-526	S-2	1.5

* Acceptance number shall be zero for all sample sizes.

**Sufficient amount from each lot of each metal used in the construction of the obstetrical forceps shall be selected for composition analysis.

4.3 Examination. The obstetrical forceps shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but shall not be limited to the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Instrument not constructed as specified.
103	Instrument not free from sharp edges, rough areas, burrs, cracks, grind marks, or overlaps.
Minor	
201	Finish not as specified.
202	Instrument not permanently and legibly marked with either the name or trademark of the contractor.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:57Z
Check the source to verify that this is the current version before use.

4.5 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of section 5. Defects shall be scored as specified in table II. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of defects per hundred units.

Table IV. Examination of preparation for delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted; incorrect; illegible; improper size, location, sequence, or method of application.
Materials	Component missing or damaged.
Workmanship	Bulging or distortion of containers.
	Cushioning inadequate, improper or missing.

4.5.1 Examination of closure and reinforcement for containers. When shipping containers are required to comply with PPP-B-636, examination for defects in closure and reinforcement shall be in accordance with the appendix to that specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Unit of issue. Each forceps, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.2.2 Preservative. Preservative shall not be utilized.

5.1.2.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.2.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-2.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree or protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:57Z
Check the source to verify that this is the current version before use.

5.2.1 Level A. Twenty four unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification. In addition, fiberboard boxes shall conform to the special requirements as specified in PPP-B-636.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B. Twenty four unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Fiberboard boxes shall conform to the special requirements as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2.4 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.3 Marking.

5.3.1 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:57Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The obstetrical forceps are intended for the delivery of the after-coming head during obstetrical procedures.

6.2 Ordering data. The procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following items appearing in the Federal Supply Catalog:

NSN	Item
6515-00-336-7500	FORCEPS, OBSTETRICAL, Simpson, 12 inch
6515-00-336-7600	FORCEPS, OBSTETRICAL, Simpson, 14 inch

It does not include all types as indicated by the title nor all types which are commercially available.

6.4 Supersession data. This specification includes requirements of Purchase Description No. 6, dated 29 September 1966 for NSN 6515-00-336-7500 Forceps, Obstetrical, Simpson, 12 inch and NSN 6515-00-336-7600 Forceps, Obstetrical, Simpson, 14 inch.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DH

Project No. 6515-1863

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.


Source: https://assist.dla.mil -- Downloaded: 202610-21T09:57Z
Check the source to verify that this is the current version before use.

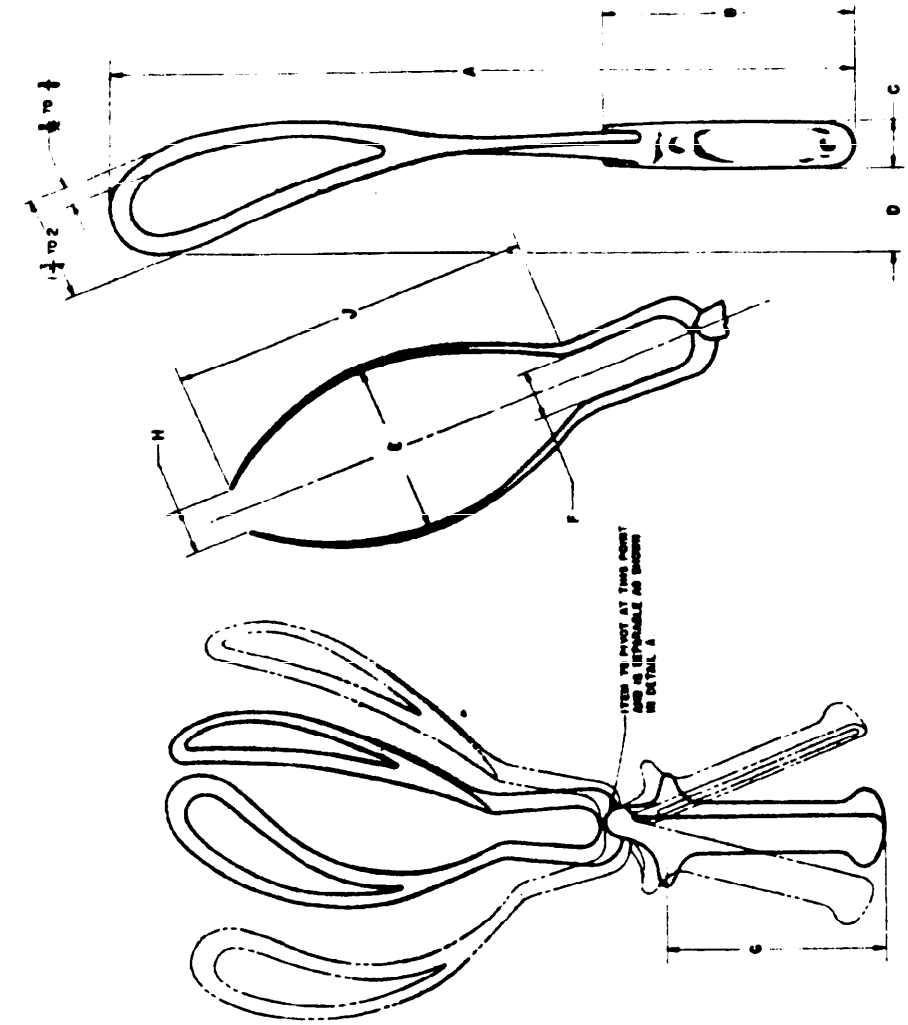


STOCK NO.	A	B	C	D	E	F	G	H	J (REF)
8315-336-7800	12 ± 1/8	4 ± 1/8	1 ± 1/8	11 to 11 1/2		10 to 10 1/2	2 ± 1/8	1 ± 1/8	8 ± 1
8315-336-7800	14 ± 1/8	4 1/2 ± 1/8	1 1/2 ± 1/8	11 to 11 1/2		10 to 10 1/2	2 1/2 ± 1/8	1 1/2 ± 1/8	8 ± 1

NOTE
TOLERANCES INDICATED ARE INTENDED TO DELINEATE THE EXTREME DIMENSIONS THAT ARE CONSIDERED ACCEPTABLE AND ARE NOT TO BE CONSTRUED AS PERMITTING THESE VARIATIONS WITHIN A SINGLE INSTRUMENT SO AS TO SACRIFICE PROPER UNIFORMITY, SYMMETRY, AND FIRST CLASS WORKMANSHIP.

FIGURE 1

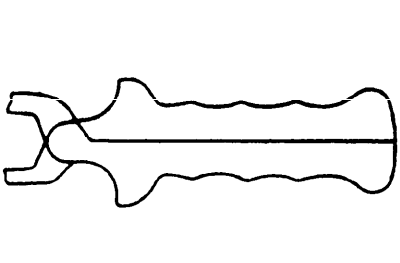

ALTERNATE MANHOLE DESIGN



DETAIL A

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:57Z
Check the source to verify that this is the current version before use.