MIL-S-37052A
19 December 1974
SUPERSEDING
MIL-S-37052
22 April 1974

MILITARY SPECIFICATION

SPECULUM, NASAL, VIENNA, 5-3/4 inch

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a Vienna style, adult model, bivalve, nasal speculum.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instrument, Dental and Surgical; General Specifications.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case and Sheet, Overwrap; Watervaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The speculum shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The speculum shall be fabricated from Class 3, type 302, 303, or 304 material.

3.3 Hardness. The speculum shall have a Rockwell hardness of B75 to B80.

3.4 Style, design and dimensions. Shall be a nasal speculum, Vienna type, adult model, bivalve, designed for visual examination and treatment of the nose. Handles shall possess indentations or serrations for gripping purposes. Speculum shall be capable of easy opening when normal hand pressure is applied, and shall close freely without binding or setting when hard pressure is released. Speculum shall be in accordance with Figure 1, for style, design and dimensions.

3.5 Locks. Lock shall be of the modified screw-type as shown on the figure.

3.6 Finish. Finish shall be mirror, or mirror, and satin. Finish of all surfaces, including inside surface of the blades, shall be smooth and uniform.

3.6.1 Passivation. The speculum shall be properly passivated.

3.7 Identification marking. In addition to GG-I-526 requirements, specula of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.


Source: https://assist.dla.mil -- Downloaded: 202610-21T09:52Z
Check the source to verify that this is the currentversion before use.

GENERAL NOTES:

1 - TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY, AND FIRST QUALITY WORKMANSHIP.

2 - REMOVE BURRS AND BREAK SHARP EDGES.

3 - UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCE IS ± 1/16 INCH

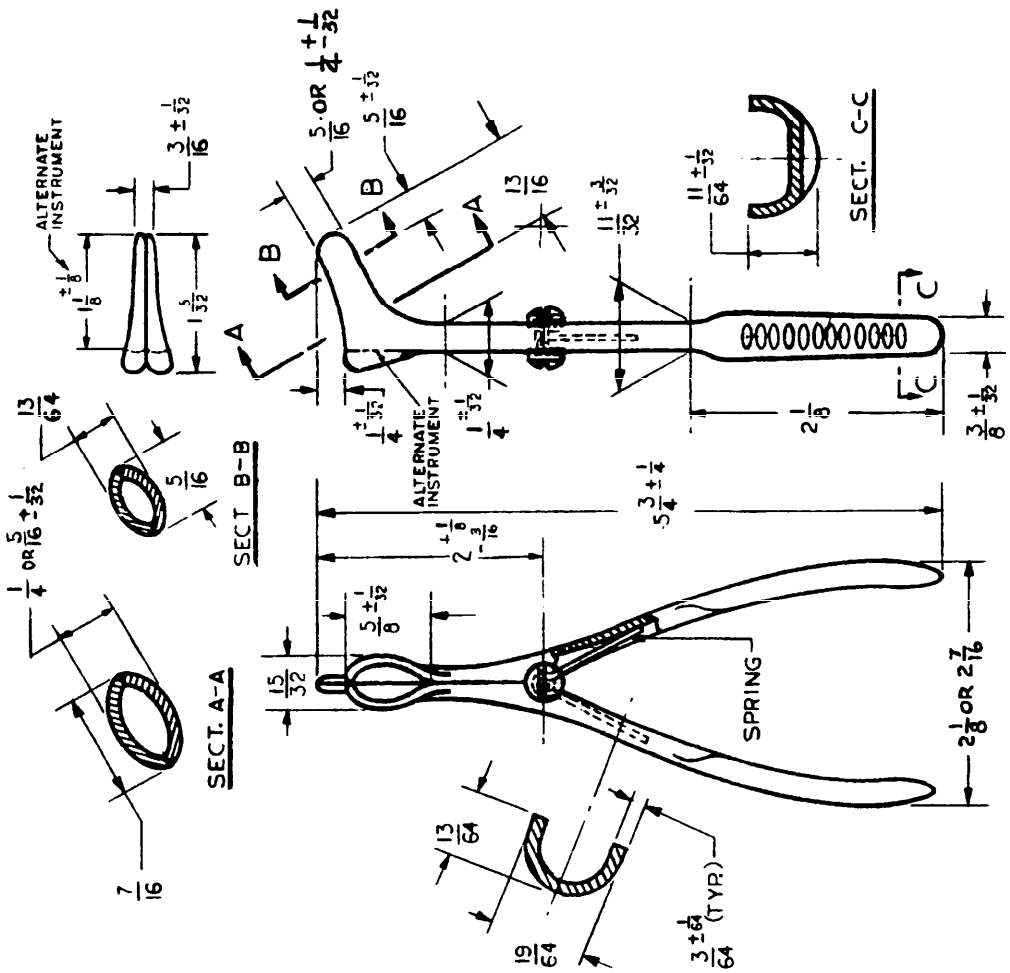

NSN 6515-00-369-9100

SPECULUM, NASAL, VIENNA, 5 3/4 INCH.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:52Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one speculum.

Table I. Sampling Criteria for Examination

Type of Defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Unit of product for test purposes shall be one speculum. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Insp. level	AQL
Speculum	Hardness test	3.3 and GG-I-526	GG-I-526	S-2	1.5
	Dimensions	3.4	-	S-2	4.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0

4.2.3 Raw materials. A sufficient quantity of each lot of metal used in the construction of the speculum shall be selected for chemical analysis.

4.3 Examination. The specula shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Table I and III. Examination, however, shall not be restricted to defects listed in Table III. Any speculum in the sample containing one or more defects shall be rejected, and if the number of defective items in any sample exceeds the acceptance number for test sample, the lot represented by the sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Speculum not free from cracks, pits, dents, scale, corrosion, nicks, sharp edges and burrs.
103	Speculum not free from excessive play in lock area.
104	Speculum is not capable of easy opening and closing.
105	Speculum does not close freely, without binding, sticking and setting of spring.
Minor	
201	Finish not as specified.
202	Identification marking not present, correct, complete or legible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. Each speculum, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit preparation. Each unit shall be cleaned and dried in accordance with the applicable method as specified in MIL-P-116. A preservative shall not be utilized on the item and each item shall be wrapped in neutral tissue or other suitable noncorrosive material.

5.1.2.2 Unit package. Each speculum shall be packaged in accordance with MIL-P-116, method IC-2.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. One hundred forty four (144) unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements as specified in Table II of PPP-B-636 shall apply for fiberboard boxes.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. One hundred and forty four unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. These specula are to be used in examination and treatment of the nose by spreading the nostrils.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Selection of applicable level of packaging and packing required (see 5.1 and 5.2).

6.3 National Stock Number (NSN) coverage. This specification covers the following item listed in the Federal Supply Catalog:

National Stock Number	Item Identification
6515-00-369-9100	SPECULUM, NASAL, Vienna, 5-3/4 inch

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1919

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:52Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-37052A

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:52Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:52Z
Check the source to verify that this is the current version before use.