NOTICE: When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility, nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

DD FORM 672-1
1 OCT 52

| CUSTODIANS | OTHER INT. |
|---|---|
| Navy - BuAer<br>Air Force | A -<br>N -<br>AF - |

PROCUREMENT SPECIFICATION: NONE

SUPERSEDES:

# MILITARY STANDARD

TEST STAND, OXYGEN REGULATOR

# MS33567 (ASG)

SHEET 1 OF 1

(A) CANCELLED - WITH NO SUPERSEDING STANDARD

THIS IS A DESIGN STANDARD. NOT USED AS A PART NUMBER.

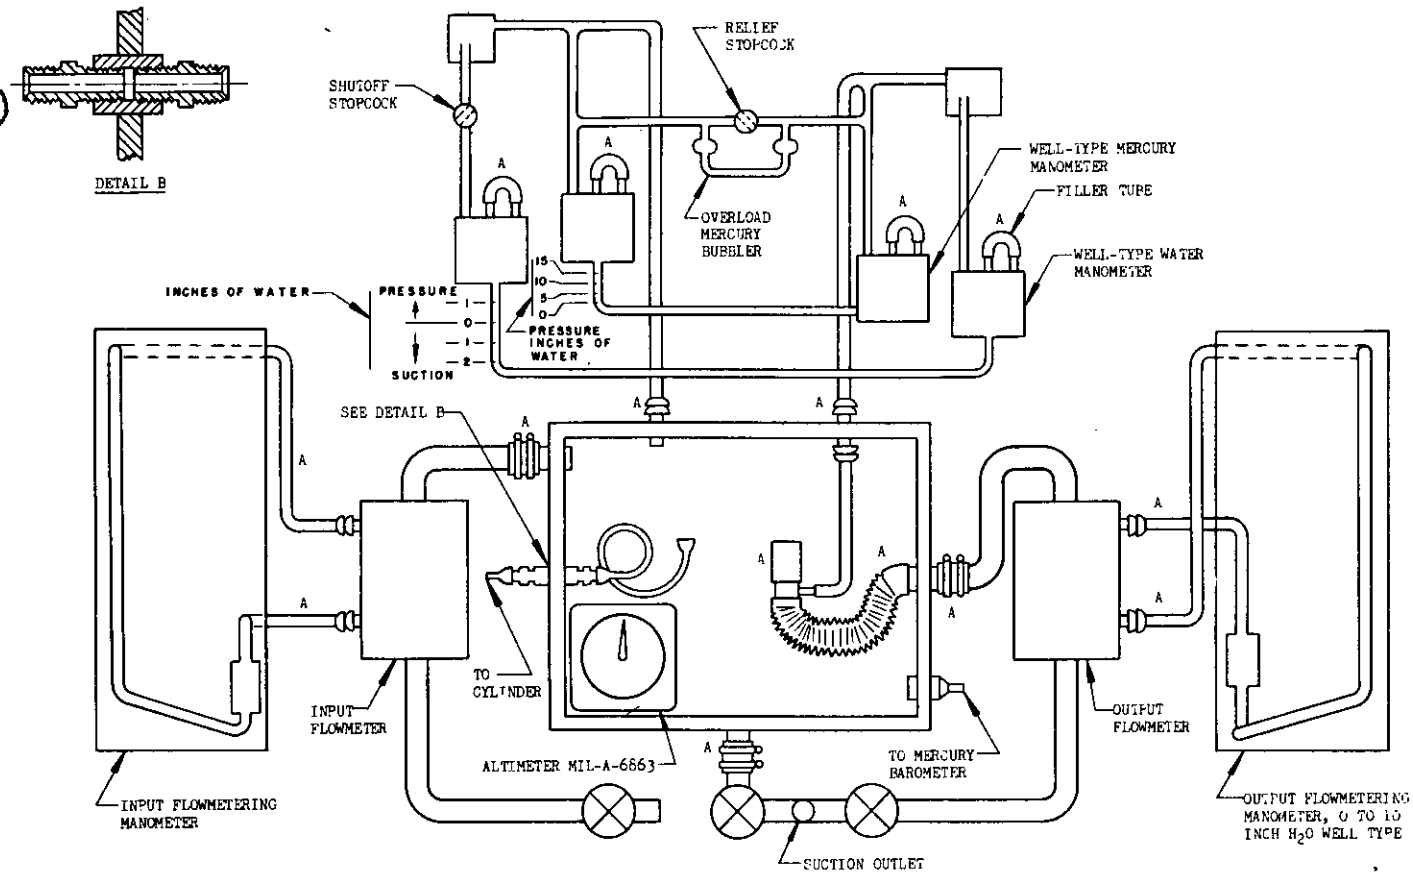


ALL CONNECTORS INTO THE CHAMBER SOULD BE CONTINUOUS THROUGH THE WALL AND PERMANENTLY ASSEMBLED, WELDED OR BRAZED.
CONNECTIONS MARKED A, SHALL BE RUBBER WHICH WILL NOT CONTAMINATE MERCURY OR THE METAL TUBES.
ALL OTHER SUBASSEMBLIES SHALL BE PERMANENTLY JOINED.
ALL WELLS SHALL HAVE FLOAT TYPE CHECKS AGAINST OVERLOAD.

THIS STANDARD TAKES PRECEDENCE OVER DOCUMENTS REFERENCED HEREIN.
REFERENCED DOCUMENTS SHALL BE OF THE ISSUE IN EFFECT ON DATE OF INVITATIONS FOR BID.
THIS DOCUMENT HAS BEEN PROMULGATED BY THE DEPARTMENT OF DEFENSE AS THE MILITARY STANDARD TO LIMIT THE SELECTION OF THE ITEM, PRODUCT, OR DESIGN COVERED HEREIN IN ENGINEERING, DESIGN, AND PROCUREMENT. THIS STANDARD SHALL BECOME EFFECTIVE NOT LATER THAN 90 DAYS AFTER THE LATEST DATE OF APPROVAL SHOWN.

FED. SUP CLASS. NONE

APPROVED 5 Oct 55 REVISED (A) 31 July 1978

Source: https://assist.dla.mil -- Downloaded: 20240-23T17:05Z
Check the source to verify that this is the current version before use.