A-A-54235A
20 November 1991
SUPERSEDING
A-A-54235
15 August 1990

COMMERCIAL ITEM DESCRIPTION

SURGICAL PREPARATION KIT, Disposable, Pre-Surgical Shave Type, Nonsterile

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a disposable surgical preparation kit containing the materials necessary to shave a patient prior to surgery.

Salient characteristics.

The surgical preparation kit shall consist of the following components:

Component	Quantity Required
Soap impregnated sponge	1
Disposable razor	1
Type I towel (Clean-up)	2
Type II towels (Underpad)	1 (minimum)
Cotton-tipped applicators a/	2
Double-compartmented water tray or Single-compartmented water tray	1 or 2

a/ The use of a paper or plastic envelope or bag for containing the applicators is optional.

Material.

Applicator, cotton tipped.

Plastic. The plastic used for the applicator shall be high

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

grade suitable for sterilization. The plastic shall conform to the requirements of the applicable Food and Drug Administration (FDA) regulations.

Cotton. The cotton shall be in accordance with the requirements of the U.S.P. for purified cotton, excluding sterility. The cotton shall be free from lumps, oil spots, streaks of dirt, and all other foreign matter.

Safety razor

Razor (without blade). Razor shall be fabricated of polystyrene, polypropylene, or styrene-butadiene, with a minimum average tensile strength of 3000 pounds per square inch (p.s.i.), when tested as specified in ASTM Designation D638. A minimum Izod impact strength of 0.45 foot pound force per inch (ft. lbf./in.) of notch at 23°C, when tested as specified in ASTM Designation D256. As an alternate, razor handle and blade seat shall be fabricated of styrene-butadiene molding and extrusion material, and the blade cover shall be fabricated of polystyrene.

Blade. The blade shall be fabricated from corrosion-resisting steel containing 0.90 to 1.05 percent carbon, 0.15 to 0.25 percent silicon, 0.90 to 1.10 percent manganese, 12.0 to 14.0 percent chromium, and maximums of 0.040 percent phosphorus and 0.040 percent of sulfur. As an alternate, the corrosion-resisting steel shall contain 0.53 to 0.70 percent carbon, 0.15 to 0.50 percent silicon, 0.20 to 0.80 percent manganese, 12.0 to 14.7 percent chromium, and maximums of 0.30 percent phosphorus and 0.25 percent sulfur. The beveled edge shall be treated with a fluorocarbon-telomerized coating such as sintered polytetrafluoroethylene or shall have a fine silicon fluid coating.

Soap impregnated sponge. Sponge shall be fabricated from high quality polyurethane impregnated with good quality potassium soap conforming to the requirements of the U.S.P. for soap, having a minimum of 0.7 gram per pad. The soap shall not contain perfume. The addition of lanolin, U.S.P. grade, is permissible. The sponge shall be furnished either wet or dry.

Towels. Towels shall be furnished in the following two types:

Type I (Clean up). The clean up towel shall consist of 3 or 4 plies of soft, lint-free, facial quality tissue paper treated for wet strength. The physical properties of the tissue shall conform to the requirements shown below. Sufficient quantity of each lot of towels shall be sampled for testing in accordance with the TAPPI Standards referenced below.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Type II (Underpad). The underpad towel shall be 3 or 4 (total) ply towel consisting of 2 or 3 plies of tissue in accordance with Type I, with the addition of a single ply of plastic film firmly and securely laminated to the tissue by overall embossing of the towel. The plastic film shall be 0.0004 inch, minimum thickness polyethylene or polypropylene. The plastic film may be short, up to 1/2 inch, at each end of either the length or width dimension. The plastic film shall be laminated to the outside of the towel, or may be laminated between the second and third tissue ply of a 4 ply towel.

The towel shall be folded by three half folds. The towel shall be overall embossed, or partially embossed for at least two rows. Each row shall be at least 3/4 inch in width.

Physical Properties.

Characteristic	Value	TAPPI Standard
Basis weight, minimum (500 single plies, 24 by 36 inches).	9.5 lbs.*	T410 os-68
Water absorption, maximum 0.01 ml. water.	10 seconds	T432 su-72
Bursting strength, minimum 12 plies of tissue.	15 points	T403 os-76
Wet tensile breaking strength, minimum.		
Cross direction.	0.05 Kg/15 mm	T456 os-68**
Both directions.	0.07 Kg/15 mm	
Brightness, minimum (white towels only).	80 %	T452 os-58

* As an alternate, test may be run on 2 ply or 3 ply tissues, in which case 500 tissues would be 19.0 lbs. for 2 ply and 28.5 lbs. for 3 ply tissues.

** Test specimen strip shall consist of the actual number of plies in the finished towel (3 or 4 for type I, 2 or 3 for type II).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Tray. The tray shall be fabricated of polystyrene, polypropylene, linear polyethylene, or styrene butadiene. Minimum average tensile strength shall be 3000 p.s.i.

Design and construction. The surgical preparation kit shall be a kit containing items necessary for preparation of patients before surgery. The preparation kit shall be complete (except for water), ready to use, and disposable.

Applicator, cotton tipped. Applicators shall consist of a plastic applicator stick tipped at one or both ends with cotton. The cotton tip shall be securely attached to one or both ends of the applicator stick with heat, without appreciable interference with absorptivity of cotton. The tip shall be pear shaped and shall be smoothly wound, covering the end of the stick to a depth of no less than 1/16 inch. Applicator shall be from 3 to 6-1/2 inches in length. Two applicators shall be furnished in each surgical preparation kit. The two applicators may be furnished, packaged in a sterile condition in a nonresealable envelope, at the manufacturer's option.

Safety razor. The safety razor shall consist of a handle and head (frame and cap) which permanently secure the blade. As an alternate, the razor handle shall be capable of being detached from the razor head by pulling with a force of no less than 4 pounds, when tested as specified herein. The razor shall be the disposable type, as shown in Figure 1 and shall have the following dimensions:

Overall length:	3-5/8 to 4-1/8 inches
Length of handle:	3-1/4 to 3-9/16 inches
Length of head:	1-1/2 to 1-7/8 inch
Width of head:	7/8 to 1-1/8 inch
Handle diameter (when round) or handle width across flats (when rectangular) at smallest cross section:	1/4 inch minimum

The razor shall have a protective cover fitting over the blade. The cover may be the snap-off type or may slide over the head of the razor, and shall be fabricated of either

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:31Z
Check the source to verify that this is the current version before use.

plastic or cardboard. The razor shall have from 9 to 10 teeth on both sides or on one side of the razor head. The teeth shall be spaced and beveled to prevent clogging and to facilitate rinsing. In Figure 1, the teeth on the corners shall be wide enough to prevent scratching of the tissue. The assembly of the head frame, cap, and blade shall be properly oriented with respect to each other, to preclude any movement of the blade cutting edge. The assembly shall not exhibit clearance at the interface of the head frame, cap, and blade. The straight beveled edges of the blade shall be parallel and equidistant from the tips of the razor head teeth. The handle of the razor shall have suitable gripping surface to minimize slippage during use. The gripping surface may be of any design shown in Figure 1. The design shown in Figure 1 is for illustration purposes only and is not intended to preclude acceptance of razors that otherwise comply with the requirements.

Blade. The blade shall be a coated, stainless steel blade, and shall be permanently assembled in the razor. Each cutting edge of the blade shall be 1-7/16 $\pm$ 1/16 inch in length and shall be exposed from beneath the cap of the razor no less than 1/32 inch and no more than 1/20 inch. Thickness of the blade shall be from 0.0036 to 0.0067 inch.

Towels. Both type I and type II towels shall measure no less than 17 inches in length by 12-1/2 inches in width.

Sponge. A soap impregnated sponge shall be furnished either wet or dry. When the sponge is furnished wet, it shall be hermetically sealed in an aluminum foil packet measuring no less than 0.007 inch thick and capable of passing the general vacuum chamber, and submersion leakage test. When the sponge is furnished dry, no protective package is required. The sponge shall be suitable for generating lather for shaving the patient prior to surgery.

The sponge shall be 3 to 3-7/8 inches long by 2 inches wide, minimum, by 1/8 inch thick minimum, when the sponge is furnished wet, or 3/16 inch thick, minimum, when the sponge is furnished dry.

Tray. The tray shall be furnished either as a double-compartmented, single tray, or as two individual trays. Tray or trays shall not leak water, when tested as specified herein.

Double-compartmented, single tray. When double-compartmented, single tray is furnished, compartments shall be formed either by a discrete divider which extends upward from the bottom level surface of the tray, or shall exist as two separate

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

wells connected only at the top surface of tray. Tray shall have the following dimensions:

Thickness (minimum):	0.020 inch
Depth:	1-1/4 to 2 inches
Length of large compartment:	3-1/4 to 4-1/4 inches
Width of large compartment:	4-5/8 to 5-1/2 inches
Length of small compartment:	2-1/4 to 2-3/4 inches
Width of small compartment:	4-5/8 to 5-1/2 inches

If tray is well-shaped, bottom lengths and widths of compartments may taper down to 1/2 inch less than the top lengths and widths.

Individual trays. When two individual trays are furnished, the individual trays may be rectangular or tub shaped, or one tray may be furnished with a cover such that the cover may be used as a separate tray. The trays may be either of the same size or of different sizes. Trays shall conform to the following dimensions:

Top length:	4-9/16 to 6-1/2 inches
Top Width:	2-9/16 to 5 inches
Bottom length:	4 to 5-1/2 inches
Bottom width:	2 to 4 inches
Depth: 1/	1 to 2 inches
Thickness:	0.020 inch minimum

1/ If trays are such that the cover is used as the smaller tray, the inside depth of the cover shall be 1/2 inch, minimum.

Color. Trays shall be white or natural in color. Color of the razor and sponge shall be at the manufacturer's option. Clean-up and underpad towels shall be white or pastel in color, provided that type I and II towels are of different

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

color to readily distinguish one type from the other for immediate use.

Hardness (blade). The coated blade shall be uniformly hardened to the hardness range indicated below for the applicable composition. The hardness shall be tested in accordance with ASTM Designation E 18 or E 92 and E 140 or an equivalent British Standard method. The hardness reading shall be taken as close as possible to the cutting edge, but not on the beveled portion.

Material	Rockwell Superficial hardness number 30-N Scale 1/	Vickers hardness number 2/
Regular (0.90 to 1.05 % carbon)	68-73	500-600
Alternate (0.53 to 0.70 % carbon	71-76	500-650

1/ using a 30-kilogram force (kgf) load and a superficial diamond penetrator.

2/ using a 5-kgf load.

As an alternate, the uncoated blade shall be uniformly hardened during fabrication to a hardness range of 500 to 650 (Vickers hardness number) using a 1 kgf load or 70-76 (Rockwell superficial hardness number 30-N scale) using a 30 kgf load and a superficial diamond penetrator.

Finish (uncoated blade). The cutting edges of the blade shall be bilaterally ground and honed to razor sharpness. The final hone bevels shall be flat, smooth and continuous throughout the entire length of the blade. Except for the extreme 1/8 inch at either end, the cutting edge shall be free from micro-cracks, and no more than 5 percent of the edge length shall show nicks, notches, or unhoned portions when viewed microscopically, as specified herein. The remainder of the blade shall have a smooth, bright polished finish. The entire blade shall show no evidence of corrosion.

Marking. When the sponge is furnished in a foil packet, the packet shall be suitably marked to indicate its contents. Razor or blade shall be permanently and legibly marked with the name or trademark of the manufacturer or supplier.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Individual package. Each surgical preparation kit shall be packaged in paperboard or heat-sealed plastic bags.

Workmanship. All components shall be free from disagreeable odor. Preparation kit and all components shall be clean and shall be packaged clean. Preparation kit and all components shall be free from defects which may detract from their appearance or impair their serviceability.

Unit. Package (PG). One package containing forty eight (48) individually packaged surgical preparation kits, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Manufacturer's protocol. A manufacturer's protocol, that lists the inspection characteristics with specification requirements and which states that inspection results comply with said requirements, is acceptable, providing the actual inspections results are made readily available to Government representatives upon request.

Certificates of quality for raw materials. Certificates of quality, supplied by the manufacturer of the following raw

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

materials, may be furnished in lieu of actual performance of such testing by the contractor, provided that the lot identity has been maintained and can be demonstrated to the Government:

raw sponge material (not impregnated with soap).
liquid soap.

Certificates of quality for end item (finished component). Certificates of quality, supplied by the manufacturer of the applicators (including compliance with applicable F.D.A. regulation for plastic applicator stick and towels, may be furnished in lieu of actual performance of such testing by the contractor, provided that lot identity has been maintained and can be demonstrated to the Government.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection, examination, and test characteristics. The unit of product for inspection, examination, and test purposes shall be one preparation kit (end item). Unless otherwise specified, sampling for examination shall be conducted at inspection level II, except for dimensions which shall be conducted at inspection level S-1, AQL 1.5 (percent defective) and sampling for tests (when applicable) shall be conducted at inspection level S-3, except that the acceptance number shall be zero (0) for all sample sizes.

Microscopic in-process examination. Sampling shall be conducted in accordance with MIL-STD-105, inspection level S-1. Oil, grease and lint shall be removed from the cutting edges of the blade (prior to coating) by any suitable means which will not damage the blade edge. The blade edge shall then be placed in the microscopic field and adequately illuminated by two 15-watt fluorescent lamps for clear vision. The nicks in the blade edge shall be examined by a field micrometer eye piece with one-hundredth millimeter graduations in a one-hundred power microscope.

Examination. Examination shall include, but shall not be limited to the following:

Defects.

Surgical preparation kit not complete, one or more components missing.
Design and construction of components of surgical preparation kit not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Defects (con't).

Nine to ten teeth not present on at least one side of the razor head.
Trays not free from defects such as breaks, cracks and blisters.
Finish of components not as specified.
Razor broken, or head and handle not securely attached.
Cover (if provided on tray) not secured.
Cotton does not adhere firmly to applicator stick.
Cotton does not cover end of stick by 1/16 inch minimum.
Color of components not as specified.

Tests.

Tray leakage. The tray shall be filled to 3/4 inch (for cover used as tray, fill to 3/8 inch) with water containing sufficient dye to produce a distinct color. The tray shall then be set on a level surface at room temperature. After one hour has elapsed, the tray and surface shall be visually examined for leakage.

Solids content of impregnated sponge. Solids content of the sponge shall be determined by the following method:

Sponge shall be weighed. Soap shall be extracted in hot water by repeated squeezing of the sponge until no foam is expelled. Sponge shall then be dried again at 220° to 230° Fahrenheit for one hour, cooled in a desiccator, and then weighed. The difference in weight (first and second weighings) is the solids content.

Razor breakage . When the razor provided is constructed such that the razor handle is capable of being detached from the razor head by exerting a pulling force, the following test shall apply:

One end of the razor shall be held in position on a spring balance, and loads of one pound and greater (in increments of 1/2 pound) shall be applied until the head and handle of the razor break apart. The load (in pounds) at which the razor breaks apart shall be recorded.

Contract certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

National Stock Number	Item Identification
6515-00-103-6659	SURGICAL PREPARATION KIT, Disposable, Pre-surgical shave type, Nonsterile

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DOD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQHS

PROJECT NO.6515-5360
LOCATION KD#2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

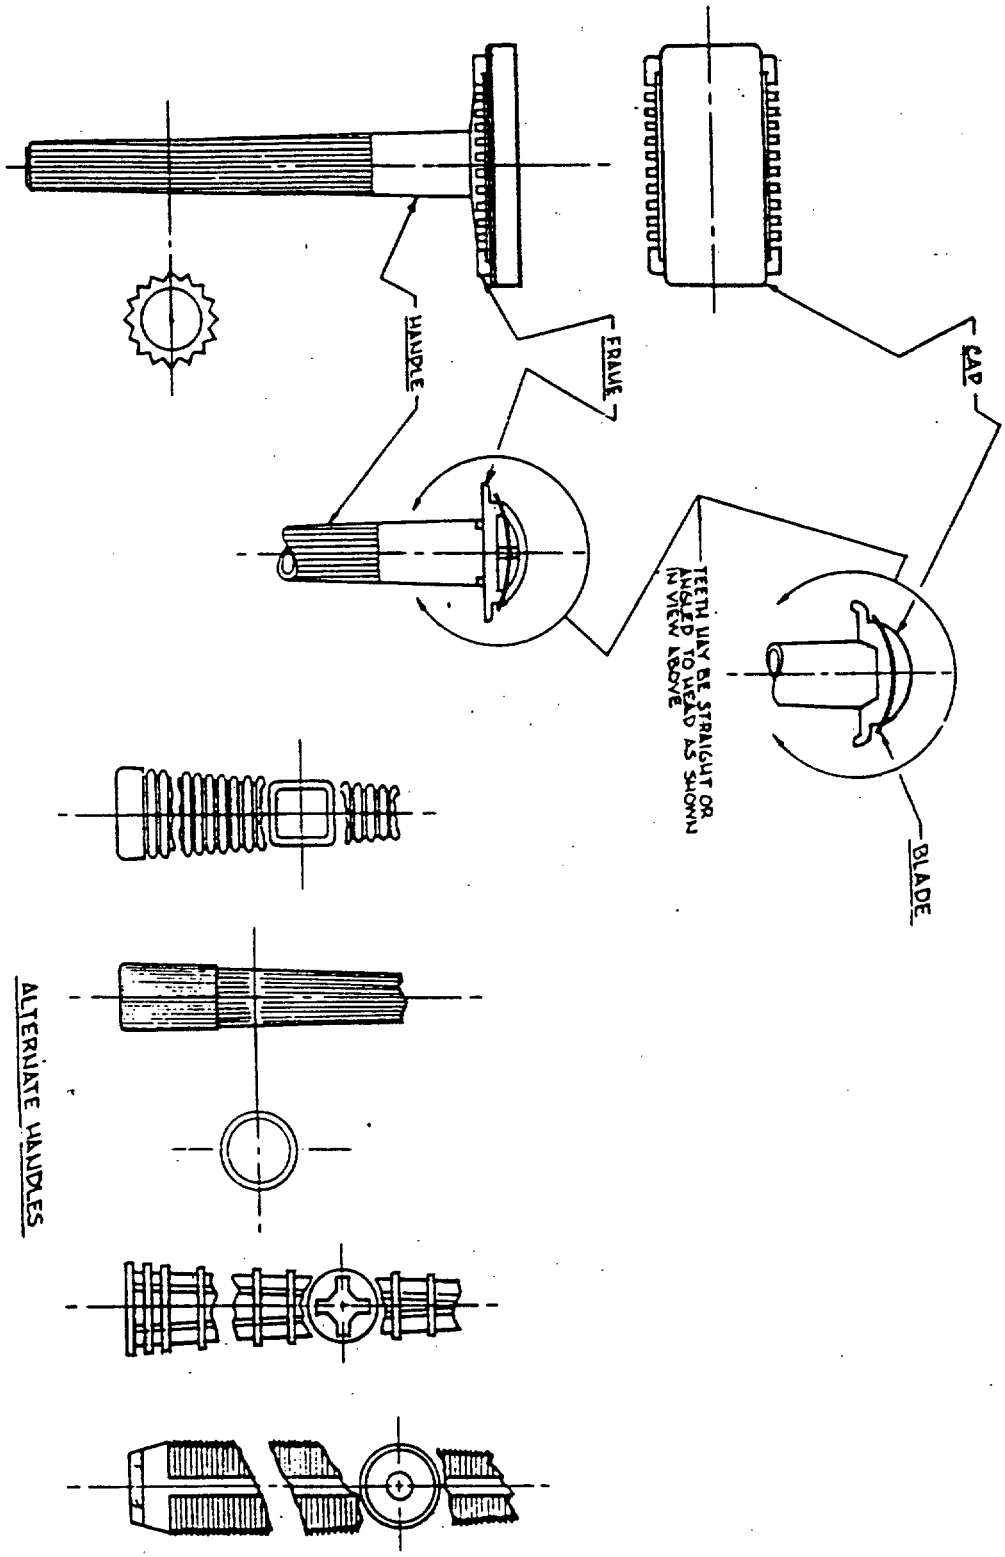

NOTE:
THE ILLUSTRATIONS SHOWN ABOVE ARE TYPICAL FOR THE TYPES IN THIS SPECIFICATION.

FIGURE 1. RAZOR AND BLADE ASSEMBLY

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.