O-P-46E
November 9, 1976
SUPERSEDING
Int. Fed. Spec. O-P-0046D(DSA-DM)
November 21, 1969 and
Fed. Spec. O-P-46B
November 6, 1952

FEDERAL SPECIFICATION

PAD, HEATING, CHEMICAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 Scope. This specification covers one type of chemical heating pad, and refill, suitable for medical field use where electricity is not available.

1.2 Classification.

Class I - Pad, Heating, Chemical
Class II - Refill, Chemical Heating Pad

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

Federal Specifications:

CCC-C-419 - Cloth, Cotton, Duck, Unbleached, Plied-yarns, Army and Numbered.
CCC-D-950 - Dyeing and Aftertreating Processes for Cotton Cloths.
PPP-B-636 - Boxes, Shipping, Fiberboard.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

Federal Standards:

Fed. Std. No. 123	- Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 191	- Textile Test Methods.
Fed. Std. No. 751	- Stitches, Seams and Stitchings.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Forth Worth, Denver, San Francisco, Los Angeles and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.

Military Specifications:

MIL-P-116	- Preservation, Methods of.

Military Standards:

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Material.

3.2.1 Cotton duck. Cotton duck shall conform to type III, 9.85 ounces per square yard, of CCC-C-419. The cotton duck shall be vat dyed yellow or olive drab No. 7 in accordance with type I of CCC-D-950 or shall be mineral dyed khaki in accordance with type II of CCC-D-950. Aftertreating of the material shall be in accordance with class B, table II of CCC-D-950 using one of the listed copper-8-quinolinolate treatments.

3.2.2 Sheeting. The basic sheeting shall be dyed olive drab No. 7 in accordance with type I of CCC-D-950. Cotton sheeting shall meet the following minimum requirements, when tested as specified in 4.4.3.

Yarns per inch:
  Warp 50
  Filling 50

Weight (ounces per square yard) ..3.5

3.2.3 Coated fabric. The basic fabric (see 3.2.2) shall be uniformly coated on one side with neoprene or other suitable synthetic rubber. The finished fabric shall meet the following minimum requirements, when tested as specified in 4.4.3.


Breaking strength:
  Warp .....40 pounds
  Filling .....40 pounds

Hydrostatic resistance (Mullen),
  (coated side down).....50 pounds per square inch

Weight of coating ..... 9 ounces per square yard

Weight of finished fabric .....12.5 ounces per square yard

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

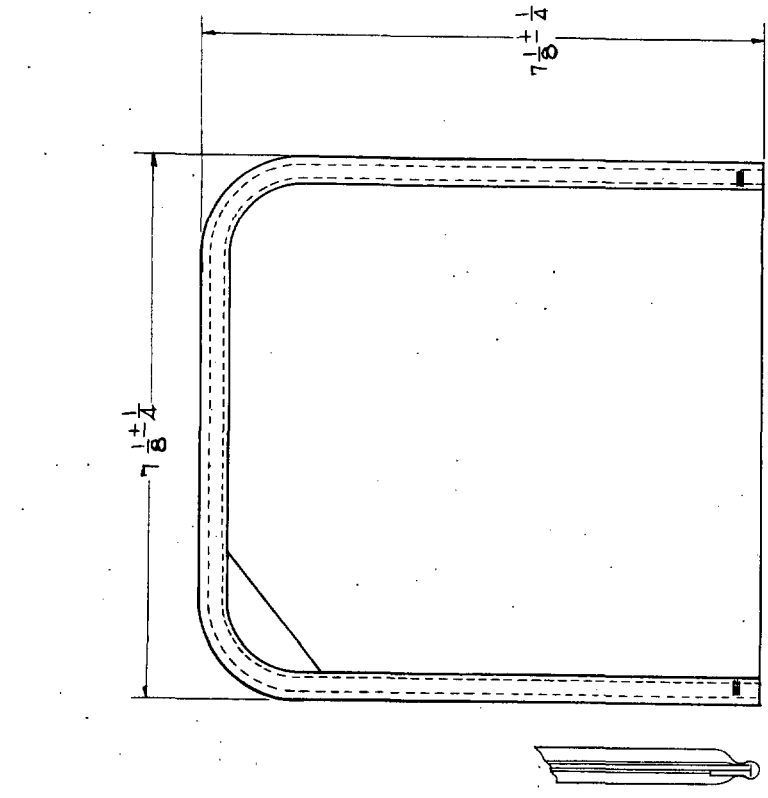

ALTERNATE DESIGN

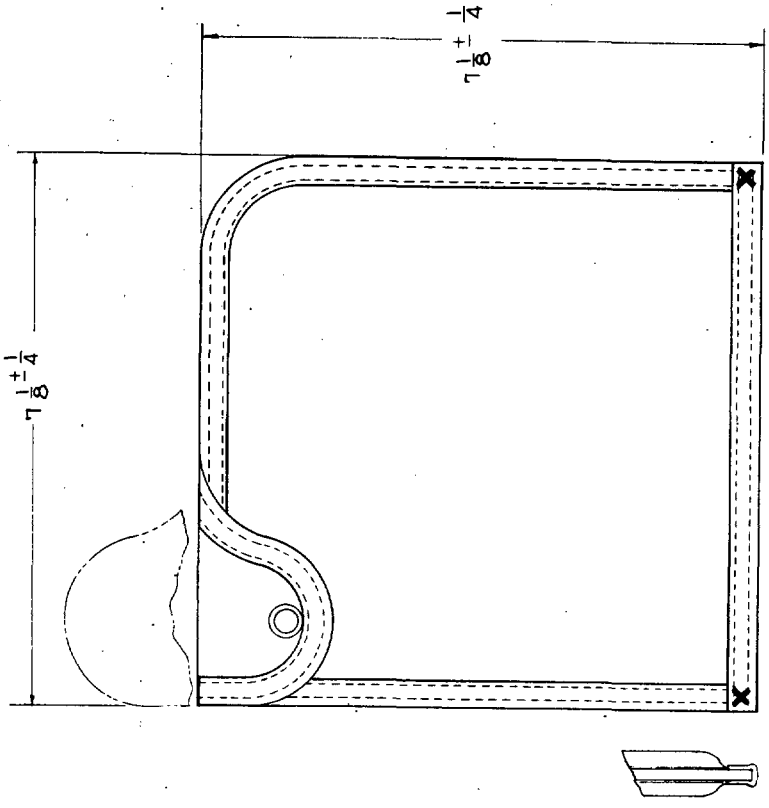


Figure 1 - inner case

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

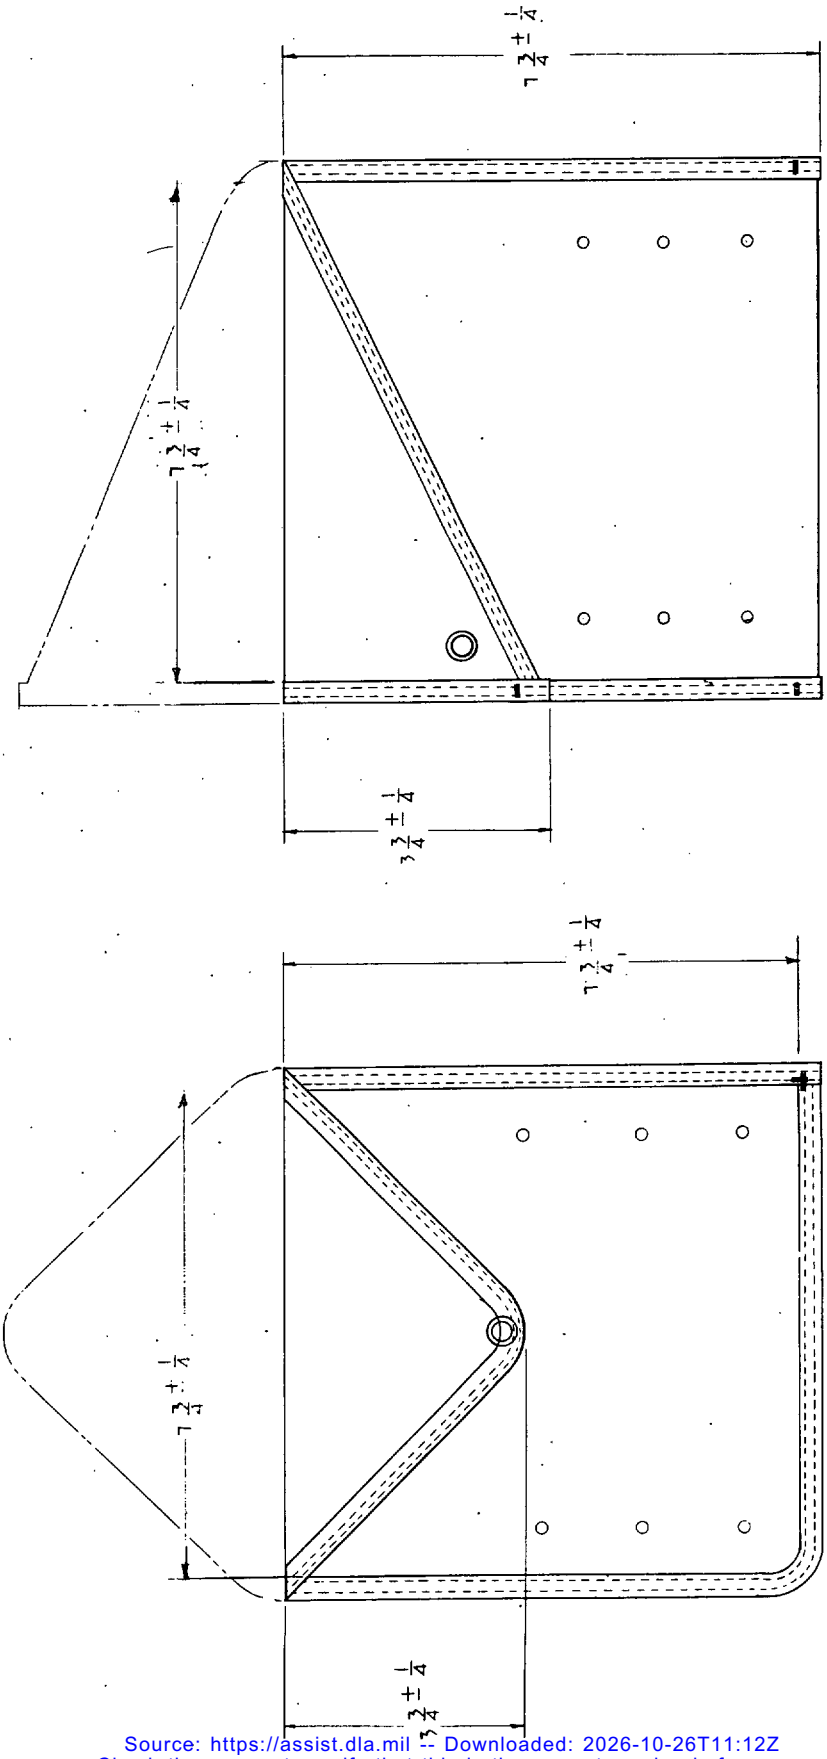


Figure 2 - outer case

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

3.2.3.1 Adhesion. The surfaces of the coated fabric shall show no signs of adhesion to each other when tested as specified in 4.4.2.1.

3.2.3.2 Tackiness and cracking. The coating on the fabric shall show no signs of tackiness or cracking when tested as specified in 4.4.2.2.

3.2.4 Heating mixture. The chemical heating mixture shall be of the quality and quantity necessary to meet the performance requirements specified herein. The heating mixture shall not be harmful to human skin. Filled pad shall not emit toxic fumes in quantities sufficient to cause harm to a human.

3.3 Construction. The class I chemical heating pad shall consist of an inner case which shall contain the heating mixture, and an outer case which shall completely enclose the inner case. The class II refill shall consist of an inner case containing heating mixture. Inner and outer cases shall be in accordance with figures 1 and 2, respectively.

3.3.1 Inner case. The inner case shall be made of cotton duck as specified in 3.2.1. Edges shall be bound with cotton tape or bias binding of a matching or harmonizing shade of olive or brown and of adequate strength which shall be attached with double stitching. The inner case shall not permit sifting through of the heating mixture. The case shall be provided with an opening for introducing water, and an adequate means of closing the opening to prevent escape of contents. A nylon fabric or rubber coating on the inside surface of the inner case in the area of the opening only, shall be acceptable. The inner case shall be printed with, at least, the information specified below:

DIRECTIONS

1. UNSNAP AND SLOWLY POUR TWO TABLESPOONS OF WATER INTO OPENING. SHAKE OR KNEAD UNTIL WARM: THEN PUT INTO POCKET OF OUTER CASE.

2. FOR MAXIMUM HEAT, PLACE TOWEL OR COVER OVER HEAT PAD. WHEN USED IN BED, IT IS NOT NECESSARY TO COVER: IF TOO HOT, WRAP IN TOWEL.

3. WHEN THROUGH USING, REMOVE INNER CASE AND SET ASIDE TO COOL AND DRY. CAUTION - NEVER PLACE HOT UNIT ON ANY SURFACE DAMAGED BY HEAT.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4. EACH APPLICATION IS SUFFICIENT FOR APPROX. 8 HOURS OF CONTINUOUS HEAT IF PAD REMAINS COVERED. EACH SUBSEQUENT USE WILL TAKE A LITTLE LONGER TO REACH HIGHEST TEMPERATURE. ALLOW FOR WARM-UP PERIOD. DO NOT USE EXCESS WATER.

5. TO REHEAT, REPEAT AS DIRECTED ABOVE. AFTER 40 HOURS USE, INCREASE WATER TO 3 FULL TABLESPOONS. CRUSH OR KNEAD OUT ANY LUMPS PRIOR TO ADDITION OF WATER. SHAKE OCCASIONALLY TO KEEP PAD AT HIGHEST TEMPERATURE.

For closures without a snap, Direction 1 above shall read as follows:

1. SLOWLY POUR TWO TABLESPOONS OF WATER INTO OPENING. SHAKE OR KNEAD UNTIL WARM: THEN PUT INTO POCKET OF OUTER CASE.

All variations of wording shall be approved by the contracting officer before application. Lettering shall be legible and permanent, and shall be of sufficient size to permit easy reading of instructions even when the inner case becomes water spotted after one or more uses.

3.3.2 Outer case. The outer case shall be made from coated fabric as specified in 3.2.3. The coated side of the fabric shall be the inner surface of the outer case. The outer case shall be closed on three sides, with the fourth side open and provided with a triangular shaped flap as specified in figure 2. All edges of the case and flap shall be bound with cotton tape, dyed olive-drab No. 7, and secured with a double row of stitching. The free edge of the open side of the case shall be hemmed or bound with tape. A snap fastener assembly located on the flap and the body of the outer case shall be furnished. The snap fastener assembly shall secure the flap to the degree necessary to retain the inner case when the outer case is suspended from two corners of the outer case with the flap end down. The snap fastener assembly shall operate without undue force such as would make opening or closing of the fastener difficult. The flap side of the outer case shall be provided with six ventilation holes.

3.3.3 Stitching. All stitches on both the inner and outer cases shall be machine stitches conforming to stitch type 301 of Fed. Std. No. 751. The inner case shall be stitched with a minimum of eight stitches per inch, and the outer case shall be stitched with six to eight stitches per inch. When machine stitching is not a continuous thread, it shall be backstitched not less than 1 inch or bartacked at each break. All stitching shall be backstitched or bartacked at the ends.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

3.4 Heating requirements. The chemical heating pad or refill, as specified, shall give off heat as a result of a chemical reaction, upon the addition of water. The pad or refill shall perform as required in 3.4.1, 3.4.2 and 3.4.3. The chemical heat pad refills shall be tested in outer cases manufactured as specified herein.

3.4.1 Initial temperature. When tested as specified in 4.4.1, the initial temperature for the first reaction cycle shall not be less than 145° Fahrenheit (F.). The initial temperatures for each of the succeeding seven cycles shall not be less than 120°F.

3.4.2 Minimum temperature. When tested as specified, in 4.4.1, the temperature shall, at no time during the 56 hours of testing, drop below 110°F.

3.4.3 Maximum temperature. When tested as specified in 4.4.1, the temperature shall, at no time during the 56 hours of testing, rise above 190°F.

3.5 Identification marking. The manufacturer's name or registered trademark, contract or purchase order number, and national stock number (NSN) shall be legibly and permanently marked in black letters on both the inner and outer cases, for the class I pad and the case for the class II refill.

3.6 Workmanship. Workmanship shall be first class throughout. Heating pads shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the pad or refill, as applicable, when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and test of 4.4.1.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and test(s) of 4.4.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling. The unit of product for sampling for inspection purposes shall be the pad or refill, as applicable (see 1.2), for end item tests. For the sheeting and coated fabric, an inspection lot size shall be expressed in units of one linear yard of each material and shall consist of all the sheeting and coated fabric received by the pad manufacturer at one time. The sample unit for inspection shall be two linear yards each.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and table I.

TABLE I. Sampling for examination

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	2.5
Minor defects	II	4.0
For dimensional examination	S-1	6.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II. The acceptance number shall be zero for material and end item testing.

4.2.2.1 Sheeting and coated fabric. Sampling for the testing of the sheeting and coated fabric shall be in accordance with 4.2.1 and as follows:

Lot Size (Yards)	Sample Size
80 or less	2
81 up to and including 220	3
221 or over	5

The samples shall be taken from the beginning of each roll.

4.2.2.2 Heating mixture. The test for heating requirements (4.4.1) shall be performed at least once for each lot of heating mixture. An inspection lot shall be all material produced under the same conditions and controlled to the degree that uniformity of product within the designated lot can be assured. Lot identification of the raw material by the manufacturer is one method of control, as cited above, which is considered acceptable.

TABLE II. Sampling for tests

Component	Characteristic	Requirement	Test procedure	Inspection level
Sheeting	Weight	3.2.2	4.4.3	1/
	Yarns per inch	3.2.2	4.4.3	1/
Coated fabric	Breaking strength	3.2.3	4.4.3	1/
	Hydrostatic resistance	3.2.3	4.4.3	1/
	Weight of coating	3.2.3	4.4.3	1/
	Weight of finished fabric	3.2.3	4.4.3	1/
	Adhesion	3.2.3.1	4.4.2.1	1/
	Tackiness and cracking	3.2.3.2	4.4.2.2	1/
Pad or refill	Initial temperature	3.4.1	4.4.1	S-2
	Minimum temperature	3.4.2	4.4.1	S-2
	Maximum temperature	3.4.3	4.4.1	S-2

1/ See 4.2.2.1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4.3 Examination. The pads shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in table III. Examination shall not be restricted to the classified possible defects listed below.

TABLE III. Classification of defects

Categories	Defects
Major:	
101	Inner case perforated, cut, torn, or ruptured.
102	Inner case fabric fails to prevent sifting through of heating mixture.
103	Pad and inner case not complete with all component parts.
104	Bound edges not seamed with a double row of stitches.
105	Stitches not stitch type 301.
106	Stitching at ends not backstitched or bartacked to prevent raveling.
107	Stitching has breaks or improper tension; not suitably repaired by backstitching.
108	Instructions for use not present on inner case, legible, permanent, and complete.
109	Rubber coating on outer case shows tack, blisters, cracks, or uncoated areas.
110	Stitching not a minimum of eight per inch on inner case.
111	Outer case shows unauthorized perforations, cuts, tears, or ruptures.
112	Stitching not six to eight per inch, on outer case.
113	Six ventilation holes not present on outer case.
Minor:	
201	Identification marking not present, legible, complete and permanent.
202	Color not as specified.

4.3.2 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of percent defective.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

TABLE IV. Examination of preparation for delivery

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible: improper size, location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distortion of containers.

4.3.2.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

4.4 Tests. Tests shall be conducted in accordance with the applicable material specifications cited in section 3 and as specified herein.

4.4.1 Heating requirements. Heating pads shall be tested for compliance with the heating requirements specified in 3.4 as specified herein.

4.4.1.1 Equipment and Conditions.

a. Strip chart recorder with one channel for each pad being tested.
b. Type I 30 AWG thermocouples iron-constantan with each junction crimped to a Thomas and Betts (T & B) No. A-2 terminal or equivalent. The junction shall make mechanical and electrical contact with the bottom of the terminal cavity. One thermocouple assembly shall be used with each pad tested and shall be calibrated to an NBS thermometer prior to the test.
c. A 3 to 3-1/2 pound wool blanket prepared by folding in half twice in the same direction then folding it in thirds in the other direction to give a resultant thickness of 12 layers. The blanket pack shall then be placed in a confined area such as a drawer. One blanket for each pad being tested is required.
d. Ambient temperature shall be between 70° and 85°F.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4.4.1.2 Procedure.

a. The heating pad shall be activated by introducing 30 milliliters of tap water into the funnel or opening of the pad. The pad shall be vigorously agitated or kneaded for one minute and then put in its outer case and vigorously agitated for an additional three minutes.
b. The thermocouple shall be attached to the top surface of the pad, at the geometric center, between the pad and the outer case. Method of attachment shall not cover the connector. The pad shall not be folded. The pad assembly shall be placed at the center of the packet formed by the fourth and fifth layers of the blanket pack.
c. Temperatures shall be continuously recorded on the strip chart recorder over the entire test period of seven hours after reading initial temperature.
d. An initial temperature shall be recorded. This initial temperature is determined when the rate of change in the recorded temperature is 1°F. or less per minute. The time to reach 110°F. shall not exceed ten minutes after the final agitation.
e. The pad shall be subjected to seven more 7-hour reaction cycles, in between which the pad shall be allowed to cool and dry thoroughly. The procedure shall be the same as for the first cycle, except that after adding water, agitating for 1 minute, placing in the outer case and agitating for 3 more minutes, the pads shall be placed in the blanket pocket for 5 additional minutes for each successive cycle (i.e., second cycle 5 minutes; third cycle, 10 minutes; fourth cycle, 15 minutes) after which the initial temperature shall be recorded. Starting with the sixth cycle, 45 milliliters of distilled water shall be added (see Direction 5, 3.3.1). The time to reach 110°F. shall not exceed 10 minutes plus the additional time increment listed above for each cycle.

4.4.2 Temperature resistance of outer case material. The finished material for the outer case shall be subjected to the tests described below.

4.4.2.1 High-temperature resistance. A sample of the material, measuring 2 by 4 inches, shall be folded with the coated side inside and placed between two glass plates under a weight of 1 pound. The specimen and plates with weight applied shall be placed in an oven at 200°F. ± 5°F. for 2 hours. The specimen shall then be removed from the oven and allowed to cool for 15 minutes. The plates shall then be removed and the specimen examined for adhesion.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

4.4.2.2 High-temperature aging resistance. A specimen of the material shall be immersed in boiling water for 1 hour followed by subjection to circulating air at a temperature of 200°F. to 212°F. for 500 hours, and then another 1-hour immersion in boiling water. After this test, the material shall be flexed back and forth several times and shall be visually examined for signs of cracking and tackiness.

4.4.3 Physical properties of outer case material. The outer case material shall be tested in accordance with the following methods described in Fed. Test Method Std. No. 191 to determine compliance with the minimum physical requirements specified in table V.

TABLE V. Physical properties of outer case material

Test	Method
Breaking strength	5100
Yarns per inch	5050
Weight of base and coated fabric	5041
Hydrostatic resistance (coated side down)	5512

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit package. Each class I (pad, heating chemical) or each class II (refill, chemical heating pad) shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.1.2 Intermediate package. Twelve class I pads or twelve class II refills shall be packaged in a box constructed in accordance with PPP-B-636 type CF, class domestic. Closure shall be adequate to prevent accidental opening.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

5.2.1 Level A. Four intermediate packages (48 units) containing class I pads or six intermediate packages (72 units) containing class II refills shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-636, class weather-resistant. Closure, waterproofing and banding, shall be as specified in appendix of PPP-B-636.

5.2.2 Level B. Four intermediate packages (48 units) containing class I pads or six intermediate packages (72 units) containing class II refills shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-636, class domestic. Closure shall be as specified in the appendix of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers at point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Military activities.

5.3.2.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The chemical heating pad is suitable for medical field use where electricity is not available.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. Class required (see 1.2).
d. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 This specification covers the following items appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-786-4635	PAD, HEATING, CHEMICAL
6530-00-786-4640	REFILL, CHEMICAL HEATING PAD

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Civil Agency Coordinating Activities:

GSA-FSS
VA-DMS

Project No. 6530-1381

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 35 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
O-P-46E PAD, HEATING, CHEMICAL

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

☆ GPO 1974— 603-680/6126 2-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:12Z
Check the source to verify that this is the current version before use.