MILITARY SPECIFICATION

FILE, PULP CANAL, DENTAL, OGEE

This specification is approved for use within Defense Personnel Support Center (DM), and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specifiction covers standardized pulp canal files of the Ogee design for use in endodontic procedures.

1.2 Classification. Ogee files shall be of the following classes and sizes as indicated.

Class I. - 21 millimeter, operative end.

Class II. - 25 millimeter, operative end.

Class III. - 30 millimeter, operative end.

Sizes

10	60
15	70
20	80
25	90
30	100
35	110
40	120
45	130
50	140
55	

FSC 6520

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DoDISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard
PPP-B-636	Box, Fiberboard
PPP-B-676	Box, Setup

Military

MIL-P-116	Methods of Preservation

STANDARDS

Federal

FED-STD-66	Steel, Chemical Composition and Hardenability
FED-STD-151	Metal, Test Methods

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	Marking for Shipment and Storage
MIL-STD-147	Palletized Unit Loads
MIL-STD-794	Parts and Equipment, Procedures for Packaging of

(Copies of specifications and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.

2.2 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

3.1 Materials.

3.1.1 Operative end. The operative end of the Ogee files shall be fabricated of AISI 302 stainless steel in accordance with FED. STD. No. 66, with a minimum tensile strength of 270,000 pounds per square inch (psi) for sizes 10 through 80 files and 237,000 psi for sizes 90 through 140 files, when tested as specified in 4.2.2.

3.1.2 Handle. The handle of the files shall be fabricated of plastic material which is rigid and of a quality suitable to withstand normal operative procedures. Handles shall be capable of being autoclaved or dry heat sterilized without losing the shape of the handle or leaching out of color, when tested as specified in 4.4.6.

3.2 Design and dimensions. The design and dimensions of the Ogee file shall be of the standardized system conforming to the requirements of figure 1 and table I, when tested as specified in 4.2.2. The files shall be suitable for use as cutting instruments for gaining access to, clearing, enlarging, and smoothing the walls of a root canal during endodontic procedures. Ogee files shall be of two-piece construction, comprised of an operative end and a handle. Files shall be furnished in classes I, II, and III, sizes 10 through 140, as specified, (see 6.1).

TABLE I. Dimensions.

Diameter (Tolerance ± 0.02 mm)

Size	D_1 mm	D_2 mm	D_3 mm	Number of Flutes ± 2
10	0.10	0.16	0.42	37
15	0.15	0.21	0.47	37
20	0.20	0.26	0.52	24
25	0.25	0.31	0.57	24
30	0.30	0.36	0.62	20
35	0.35	0.41	0.67	20
40	0.40	0.46	0.72	20
45	0.45	0.51	0.77	18
50	0.50	0.56	0.82	18
55	0.55	0.61	0.87	18
60	0.60	0.66	0.92	16
70	0.70	0.76	1.02	16
80	0.80	0.86	1.12	16
90	0.90	0.96	1.22	11
100	1.00	1.06	1.32	11
110	1.10	1.16	1.42	11
120	1.20	1.26	1.52	11
130	1.30	1.36	1.62	11
140	1.40	1.46	1.72	11

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

3.2.1 Operative end. The operative end shall consist of a conical distal tip; a uniformly tapered, helicoidal cutting section consisting of two spirals diametrically opposed with an ogee-shaped cross-section; and a non-tapered, calibrated shank. The cutting edge shall have a positively raked flute capable of removing dentin by means of cutting rather than a scraping action. The cutting edge angle (c, figure 1) shall be between 35° and 55°. Spirals forming the cutting edge shall be formed by machine grinding rather than twisting. The spirals shall be right hand and shall extend to the tip. The upper shank shall be marked at specific distances from the tip to facilitate gauging depth. The markings shall be legible, sharply defined lines, of uniform width and depth and shall extend around the periphery of the shank. The markings shall be calibrated in accordance with figure 2.

3.2.1.1 Taper. The taper of the cutting portion of the Ogee file shall be 0.02 mm per millimeter of cutting length as specified in 4.4.2.2.

3.2.1.2 Flute depth. The Ogee files shall have a constant flute depth of 0.06 mm plus or minus 0.01 mm. The uniform taper of the spiralled section of the file along with a constant flute depth shall result in an increasing ratio of flute depth to surface area towards the tip yielding increasing flexibility near the tip.

3.2.1.3 Tip. The tip length of the instrument shall be no greater than twice the diameter of D1 of the respective size number, when tested as specified in 4.4.2.3. The tip of the instrument shall be sharply pointed.

3.2.2 Handles. Operative ends of files shall be securely and permanently affixed in the handle with no movement of operative end within the handles permitted. Color shall be incorporated in the plastic composition. Handles shall be in accordance with figure 1 for dimensions.

3.2.3 Figures. The figures forming a part of the specification are specification control figures. The supplier shall be responsible for preparing his own shop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide tolerances within those prescribed on the figure to insure correct function, fit, assembly and operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.

3.3 Resistance to fracture by twisting. The torsional load or torque at various angular deflections for each instrument shall not be less than that given in Table II for each size when tested as specified in 4.4.3.

3.4 Stiffness. The stiffness of all instruments shall not be greater than that given in Table III for each size when tested as specified in 4.4.4.

3.5 Corrosion resistance. The operative ends of the files shall not show evidence of corrosion on their surface when subjected to the corrosion tests as specified in 4.4.5.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

3.6 Finish. Spiralled section of operative ends of the files shall have a bright and smooth finish. Handles shall be longitudinally serrated or shall have cross cut serrations. The entire handle may be serrated or only the finger-gripping portion need be serrated. Handles shall be suitable for proper finger-gripping.

Table II.

Torque and Angular Deflection (Minimum Values) Twisted in Clockwise Rotation.

Size	Torque (gm.cm.)	Angular Deflection (Degrees)
10	5.0	180
15	8.0	180
20	12.0	180
25	20.0	180
30	35.0	180
35	50.0	180
40	65.0	180
45	90.0	180
50	120.0	180
55	160.0	90
60	250.0	90
70	350.0	90


TABLE III.

Stiffness (Bending Movement) Maximum Values at 45° Bend.


Size	Bending Torque (gm. cm.)
10	5
15	16
20	16
25	26
30	34
35	72
40	77
45	108
50	108
55	108
60	108
70	190
80	288

3.7 Identification marking. Handles shall be color coded and numbered with the respective size for identification of instrument as specified in Table IV.


Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

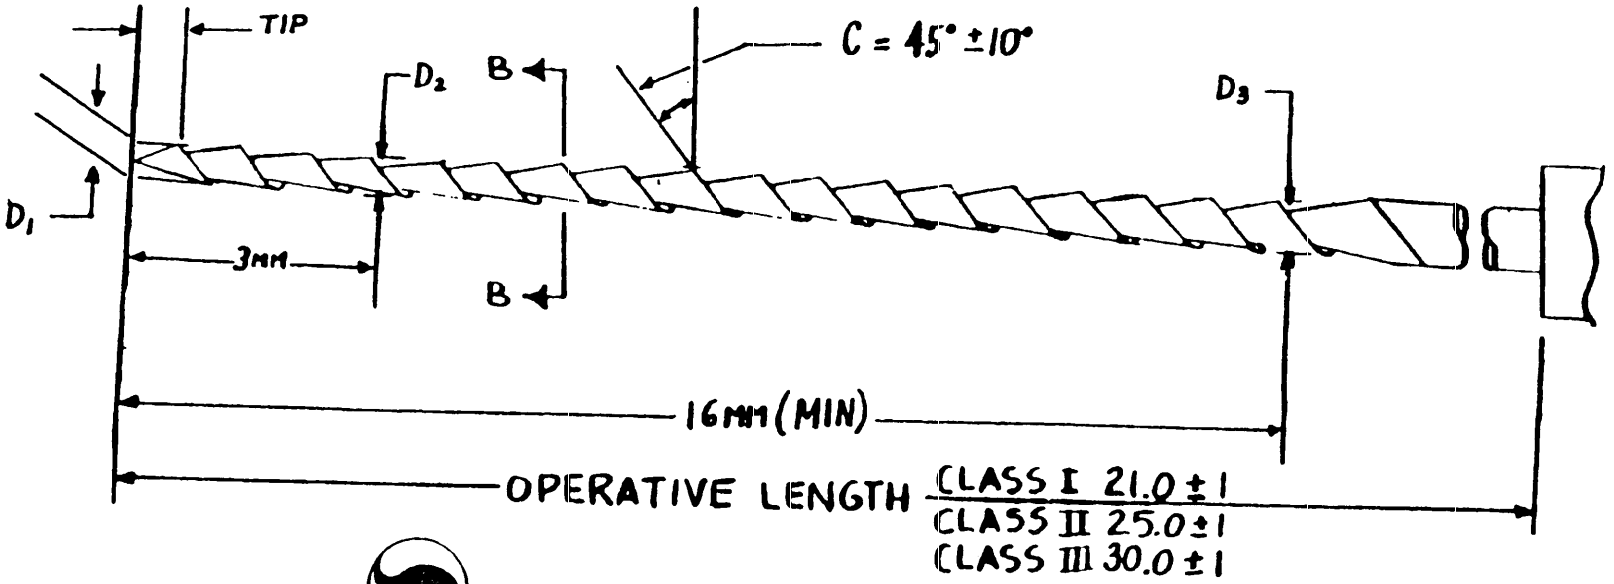

SECTION B-B
OGIVAL CROSS-SECTION

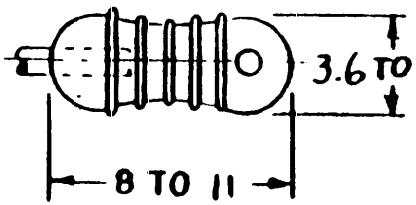


HANDLE

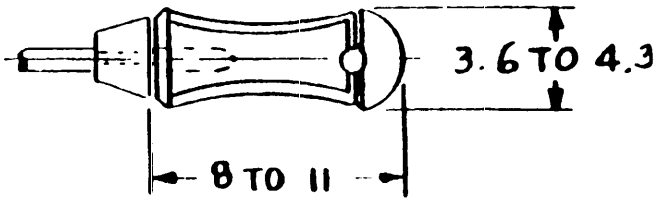


ALTERNATE HANDLE

NOTES:

1. HANDLES SHALL BE IN ACCORDANCE WITH THIS FIGURE FOR DIMENSIONAL REQUIREMENTS; SHAPE OF HANDLES SHOWN ARE TYPICAL AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF FILES WHICH ARE OTHERWISE IN ACCORDANCE WITH THIS SPECIFICATION.
2. HOLE IN HANDLE SHALL BE OPTIONAL.
3. ALL DIMENSIONS ARE IN MILLIMETERS.




SECTION A-A

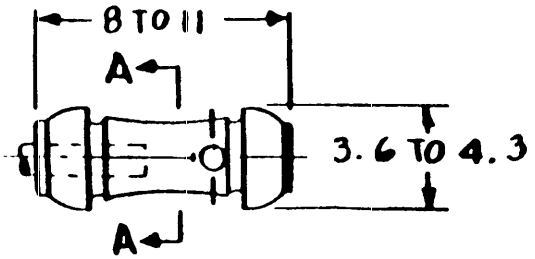

ALTERNATE HANDLE

FIGURE 1 - FILE, PULP CANAL, OGEE

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T11:47Z
Check the source to verify that this is the current version before use.

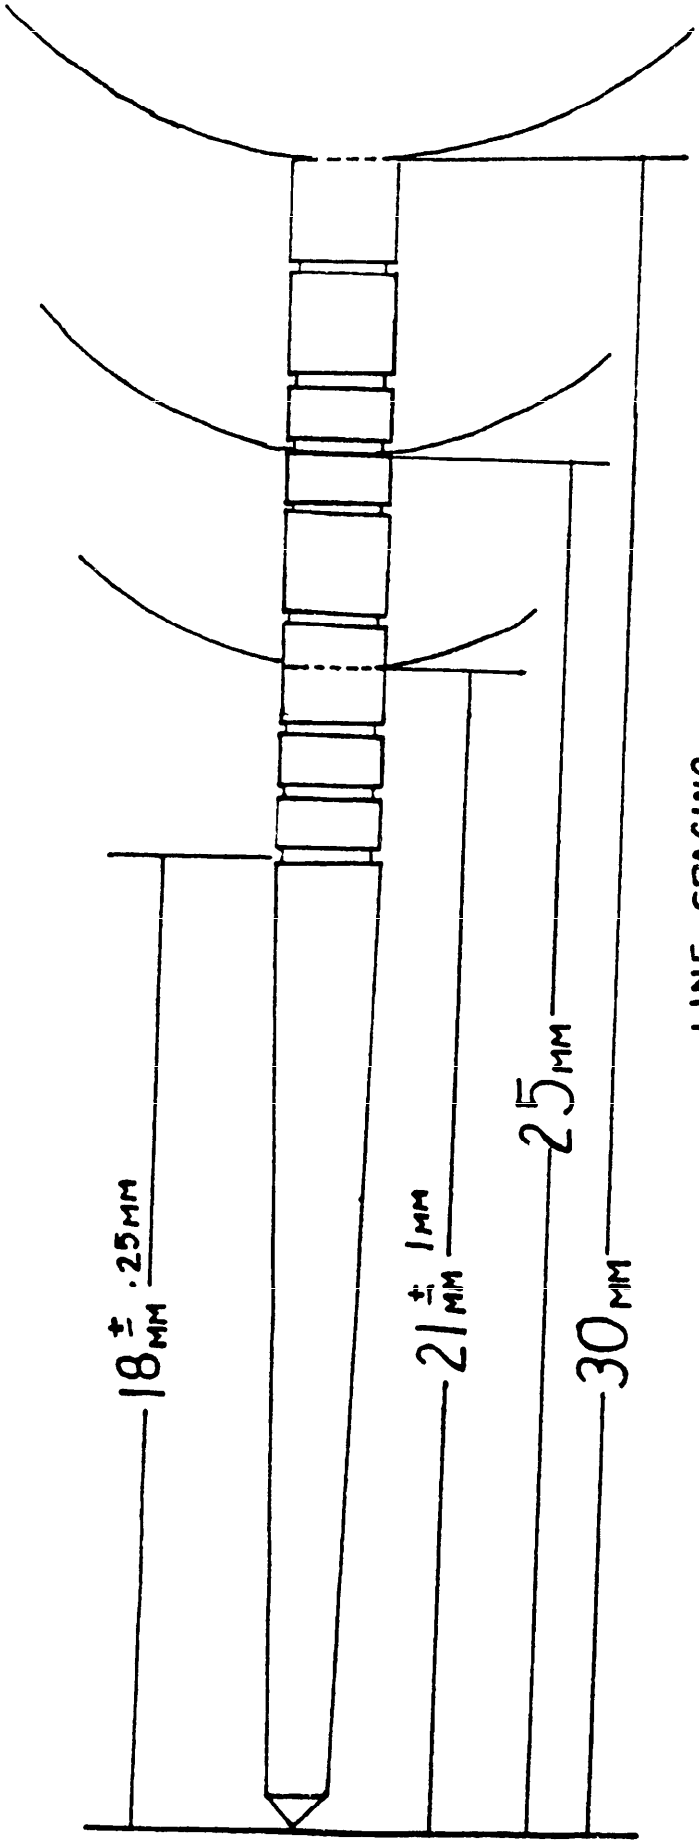

LINE SPACING	± .25 MM	MAX ERROR FROM FIRST TO LAST LINE ± .025 MM
1 MM		
1 MM		
2 MM		
2 MM		
1 MM		
1 MM		
2 MM		
2 MM		

FIGURE 2 - LINE SPECIFICATION

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

3.8 Workmanship. The files shall be free from laminations, cracks, gouges, chips, broken areas or other defects which detract from theirappearance or impair their serviceability.

Table IV. Color Coding.

SIZE	COLOR	ABBREVIATION
10	Purple	Pur
15	White	Wh
20	Yellow	Yel
25	Red	Red
30	Blue	Blu
35	Green	Grn
40	Black	Blk
45	White	Wh
50	Yellow	Yel
55	Red	Red
60	Blue	Blu
70	Green	Grn
80	Black	Blk
90	White	Wh
100	Yellow	Yel
110	Red	Red
120	Blue	Blu
130	Green	Grn
140	Black	Blk

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables V, VI, and VII (see 4.2.1, 4.2.2 and 4.3) and 4.3.1.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be as indicated in table V. Unit of product for examination purposes shall be the unit of issue.

TABLE V. Sampling for examination.

Type Defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-2	1.5
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table VI. Unit of product for test purposes shall be as indicated in table VI.

TABLE VI. Sampling for tests.

Component	Characteristic	Requirement	Test procedure	Unit of product	Inspection level	AQL (percent defective)
Operative ends	Tensile strength	3.1.1	4.4.2	Lot of steel stock	*	---
	Resist. to frac. by twisting	3.3	4.4.3	One file	S-2	**
	Stiffness test	3.4	4.4.4	One file	S-2	**
Entire Instrument	Corrosion Resistance	3.5	4.4.5	One file	S-2	**
Handles	Sterilization	3.1.2	4.4.6	One file	***	**

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:47Z
Check the source to verify that this is the currentversion before use.

*Average of a minimum of three specimens from each lot of steel stock.
**Acceptance number shall be zero for all sample sizes.
***Separate S-2 level quantities for both autoclave and dry heat tests.

4.2.3 Raw materials. Sufficient material from each lot of metal used in the construction of the files shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be tested for the determination of two or more test characteristics.

4.3 Examination. The files shall be examined for defects including, but not limited to, those listed in table VII.

TABLE VII. Classification of Defects.

Categories	Defects
Major A:	
101	Class and size not as specified.
102	Style and design not as specified.
103	Handles not properly color coded.
104	Operative ends do not have a bright smoothly-honed finish.
105	Cutting edges not sharp.
106	Operative ends not firmly affixed in the handles.
107	Laminations or cracks present.
108	Operative end bent, deformed, or otherwise damaged.
Major B:	
151	Number of flutes not as indicated for size number.
152	Dimensions of operative end not as specified.
153	Calibrations not as specified.
Minor A:	
201	Finish of handles not as specified.
202	Label or instruction sheet giving color code system not included in unit package.
203	Packaging and packing not as specified.
Minor B:	
251	Dimensions of handles not as specified.

4.3.1 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:47Z
Check the source to verify that this is the currentversion before use.

4.4.1 Chemical analysis and tensile strength of the metals. In the absence of certificates of quality for the raw material, the samples selected in accordance with 4.2.3 shall be analyzed in conformance with methods 111 or 112 of Fed. Test Method Std. No. 151. In case of dispute, method 111 shall be used for referee analysis. Tensile strength shall be performed in a tension tester on an 8-inch sample of steel stock used to produce the files.

4.4.2 Equipment. The diameter and tip length of an instrument shall be measured using an optical comparator, shadowgraph, or other suitable device capable of measuring the diameter and length with the accuracy specified in 3.2.1.2 and Table I.

4.4.2.1 Diameters. The Ogee file to be measured shall be inserted into an optical comparator, shadowgraph, or other suitable device and the diameters D1, D2, and D3 shall be measured.

4.4.2.2 Taper. An Ogee file to be measured shall have its diameter determined at 1 mm increments along the cutting section beginning 1 mm from the tip point up to 6 mm from the tip point.

4.4.2.3 Tip. The tip length of the instrument shall be determined by a suitable measuring device.

4.4.3 Resistance to fracture by twisting. Samples of a given size shall be tested for resistance to fracture by twisting as follows:

4.4.3.1 Equipment. The testing equipment shall be capable of measuring torque with an accuracy of $\pm$ 1 gm. cm. and angular deflection with an accuracy of $\pm$ 2°. The equipment described below shall be used for compliance testing and is presented as the preferred type of equipment for all purposes. The equipment as shown in Figure 3 shall consist of: a reversible geared motor revolving at a speed of 2 RPM which drives a test instrument by means of a separate hardened steel chuck; a torque measuring device fixed on two linear ball bearings, mounted to the shaft of the device is the chuck with jaws made of brass (70% copper-35% zinc) used to clamp the test instrument at the tip along a length of 3 mm. See Figure 4. A separate amplifier and digital display controls the operation of the motor and records the torque and angular deflection. The circuitry of the amplifier should include the feature of retaining for display the maximum torque 1 mm from the tip point up to 6 mm from the tip point.

4.4.3.2 Procedure for twist test. Calibrate the device for the torque range of the test instrument size to be tested. The Ogee file to be tested shall have its handle removed with a suitable wire cutter at the point at which the handle is attached to the instrument shaft. Set the test instrument shank into the driving chuck leaving a maximum of 1 mm of the unground portion of the shank out of the chuck. Tighten the chuck. Slowly slide the torque device along the linear ball bearing until the tip of the test instrument enters 3 mm into the brass jaws. Check to assure that the test instrument is straight and

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:47Z
Check the source to verify that this is the currentversion before use.

centered into the jaws. Tighten the chuck. Since clamping will probably induce a pre-stress of the test instrument, the gear motor must be activiated in steps until the torque digital display or the strip chart recorder shows a zero reading. After insuring that the geared motor is set for clockwise rotation as viewed from the test instrument shank end, activiate the device. The test device will cease operation when the test instrument fails. The maximum torque and angular deflection shall be recorded for each Ogee file tested.

4.4.4 Stiffness. Sample of a given size shall be tested for stiffness as follows:

4.4.4.1. Equipment. The equipment as described in 4.3.3.1 shall be used with the modification of the clamping jaws and the bending device or catch pin as shown in Figure 5. The amplifier of the device must be capable of obtaining a pre-selected angular deflection (45°) at which point the test stops. The testing equipment shall be capable of measuring torque with an accuracy of $\pm$ 1 gm. cm.

4.4.4.2. Procedure for stiffness test. Calibrate the device for the torque range of the test instrument size to be tested. The Ogee file to be tested shall have its handle removed with a suitable wire cutter at the point where the handle is attached to the instrument shaft. Set the device to stop the angular deflection at 45°. Place the chuck onto the shaft of the torque meter device. Set the tip of the test instrument into the jaws of the chuck perpendicular to the axis of the motor. When the tip enters 3 mm into the brass jaws, tighten the chuck. Mount the catch pin into the gear motor shaft. Slide the torque device along the linear ball bearing until the test instrument is located above the rotating pin. By rotating the gear motor in the proper direction in steps, adjust the catch pin until it is lightly touching the test instrument. The torque reading must show zero. Activiate the test device. The test will automatically cease when the angular deflection has reached 45°. The torque at 45° shall be recorded for each Ogee file tested.

4.4.5 Corrosion tests. Files shall be tested for corrosion resistance by one of the following procedures:

4.4.5.1 Sample and preparation. Files of each size shall be scrubbed with soap and water, rinsed in hot water, followed by a dip in ethyl alcohol (95%), or isopropyl alcohol (isopropanol; 2-propanol) NF, and dried.

4.4.5.2 Copper sulfate test. A copper sulfate solution is made up as follows: Copper sulfate ($CuSO_4$, 5 H_2O) 4.0 g, Sulfuric acid (H_2SO_4, sp gr 1.84) 10.0 g, and Water (H_2O) 90.0 milliliters (ml). The instruments selected and prepared shall be immersed in the copper sulfate solution at a temperature of 65° Fahrenheit (F) for 6 minutes and then wiped off with a cloth saturated with fresh water. The instrument shall then be examined under a magnification of at least 5X for the presence of brown stains indicating corrosion.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:47Z
Check the source to verify that this is the currentversion before use.

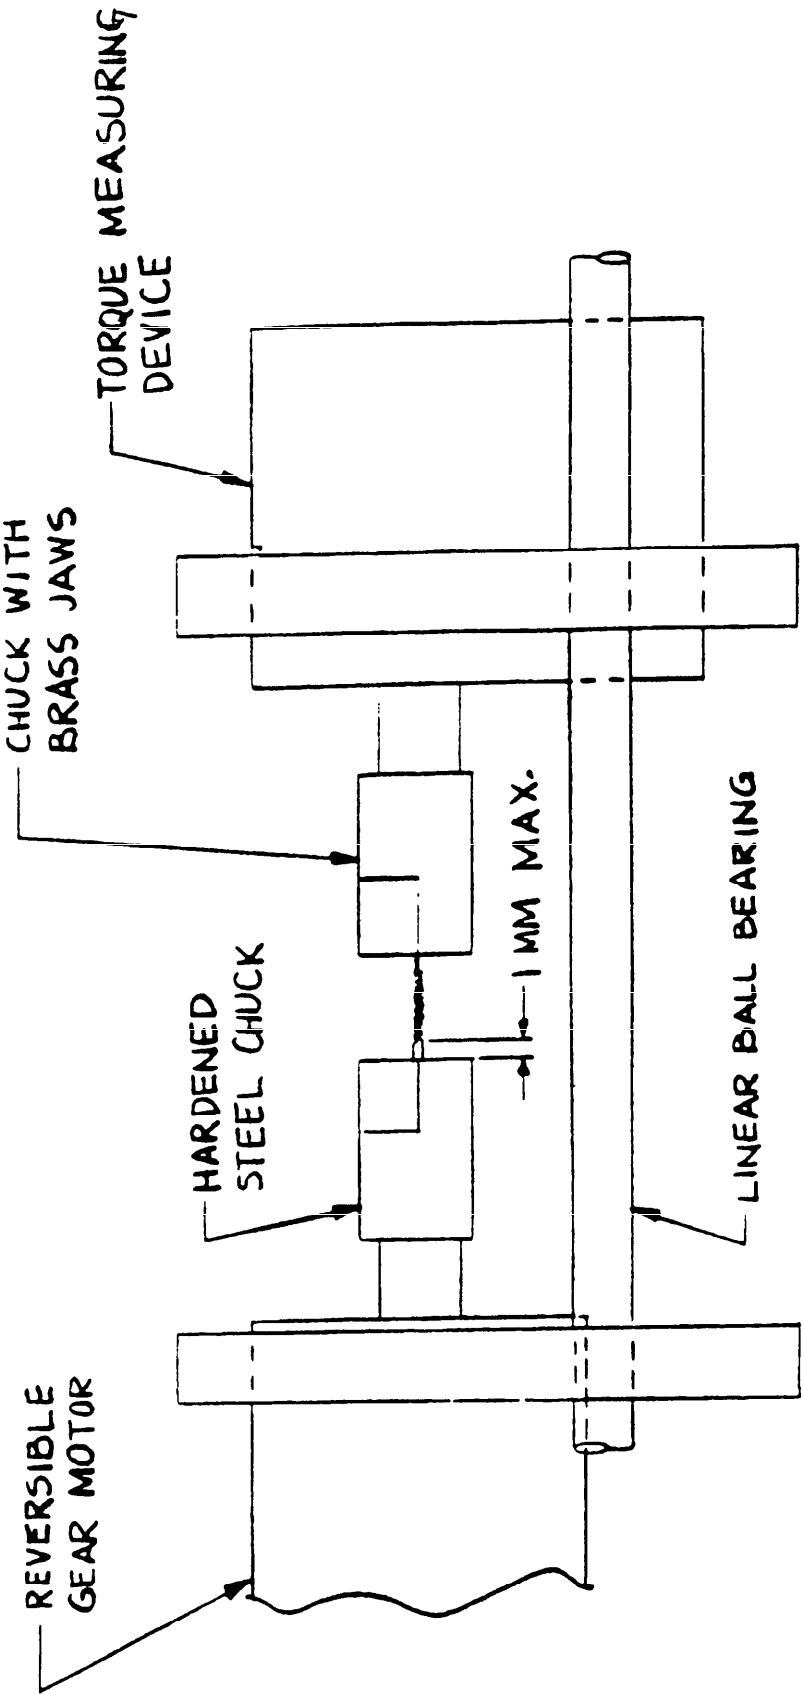


FIG. 3 - TEST EQUIPMENT FOR TORQUE TESTING

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

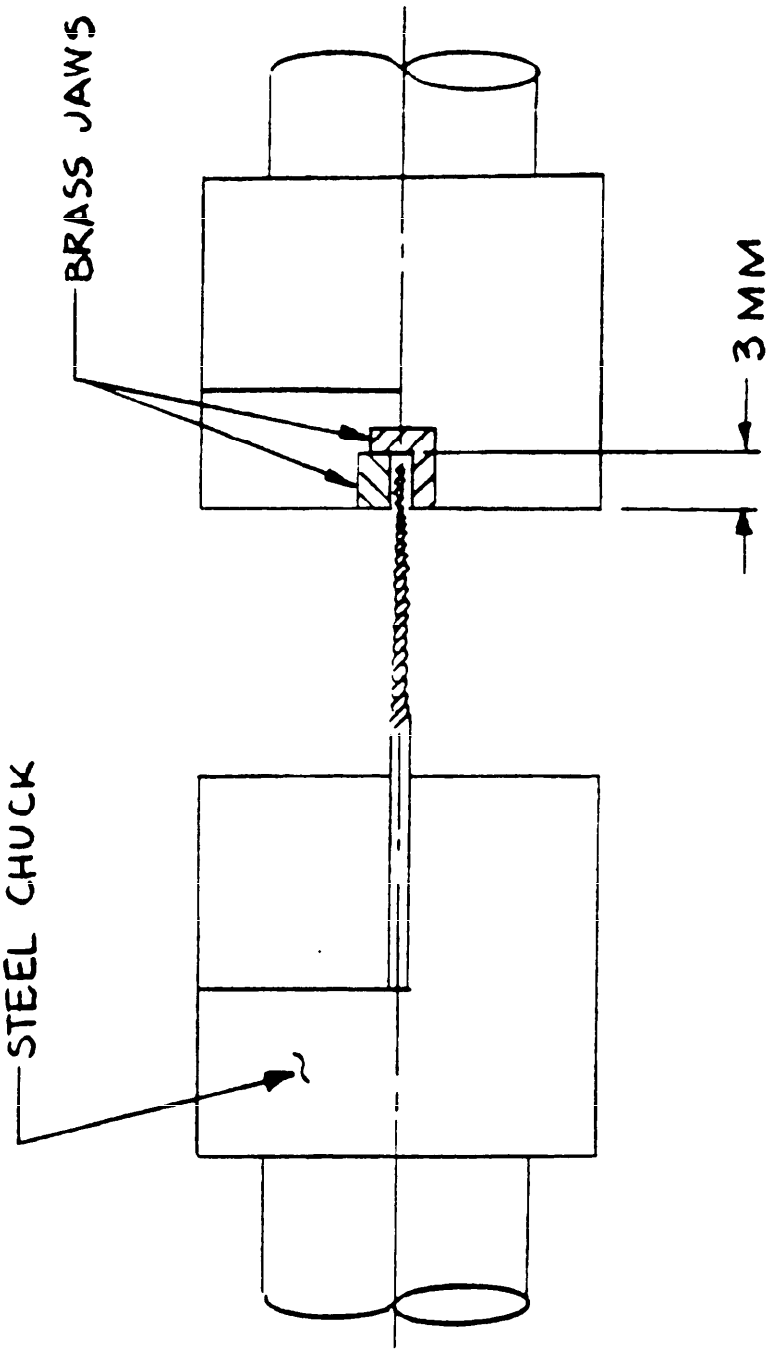


FIG. 4 - TWIST TEST CHUCK DETAIL

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

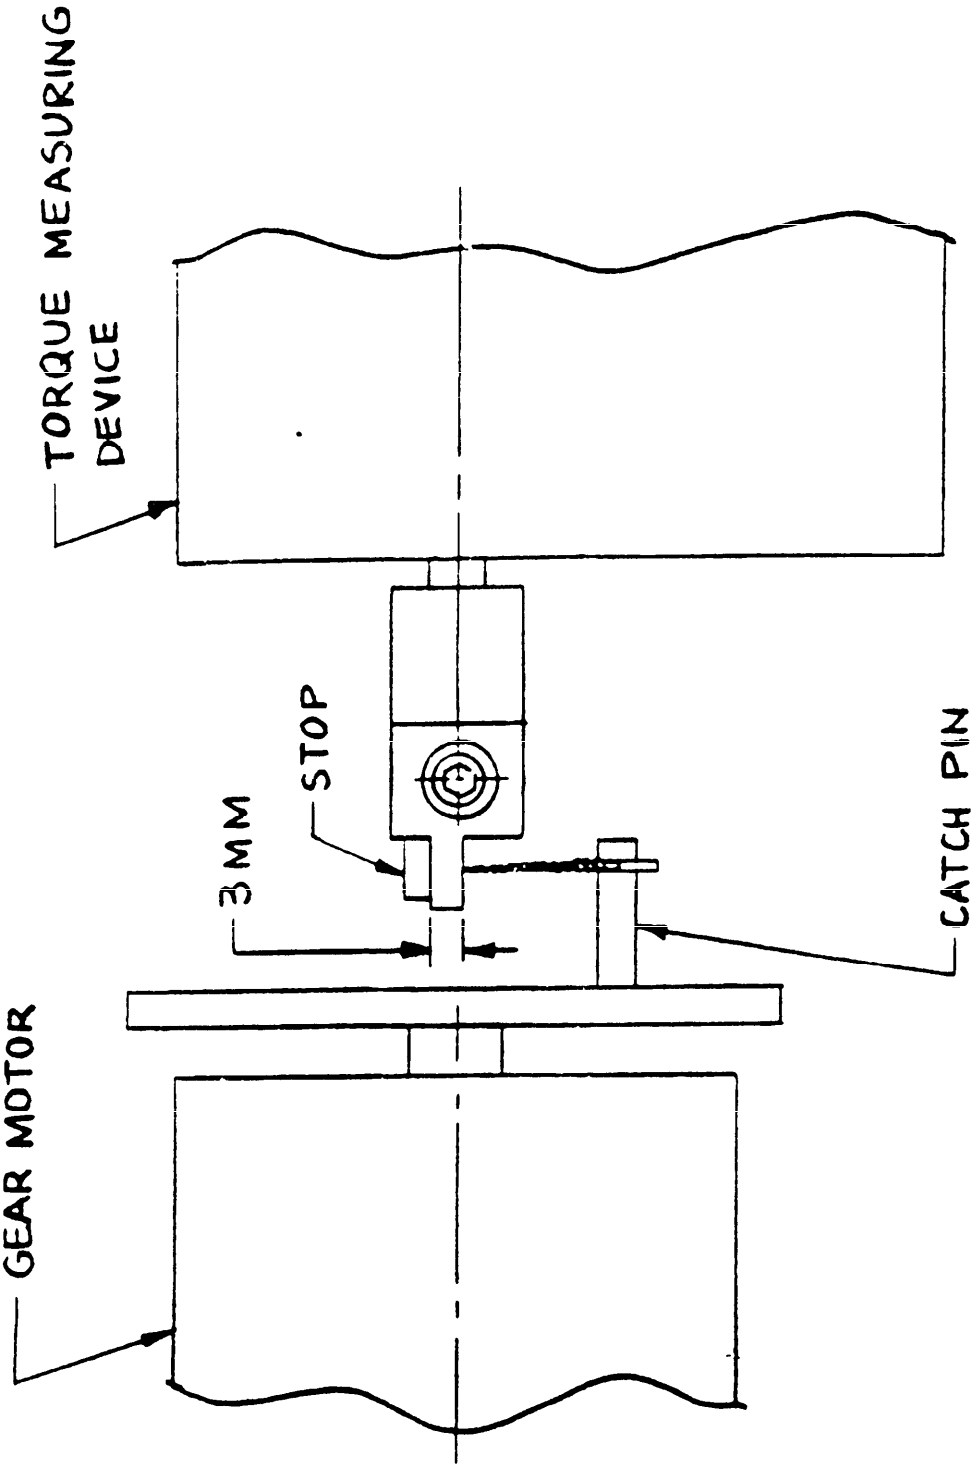


FIG. 5 - STIFFNESS TEST

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

4.4.5.3 Agar ion test. An agar ion gel is made up as follows: Potassium ferricyanide ($K_3Fe(CN)_6$) 0.2 g, Sodium chloride (NaCl) 1.0 g, Water (H_2O) 100 ml, Agar-agar 1.5 g. The agar sol shall be poured into a transparent container. The instruments selected and prepared are inserted into the gel ($37^{\circ} \pm 2^{\circ}$ Celsius (C)) at intervals of not less than 10 mm and at a distance of 10 mm from the periphery of the container. The instruments are inserted to a depth of approximately 20 mm. Visual examination of the instruments while in the gel shall be made for the presence of blue precipitates on the instrument, indicating corrosion.

4.4.6 Sterilization tests. The finished Ogee files shall be autoclaved under 27 ± 3 pounds of pressure at 132 ± 5°C (270 ± 9°F) for twenty (20) minutes and dry heat sterilized at 160 ± 5°C (320 ± 9°F) for one hundred and twenty (120) minutes. The handles of the files shall then be examined for compliance with specification requirements.

5. PACKAGING.

5.1 Preservation. Preservation shall be level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.1. Cleaning. Files shall be cleaned in accordance with MIL-P-116.

5.1.1.2. Drying. Files shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative applications. Preservatives shall not be used.

5.1.1.4 Unit package. Ten files of one class and size of sizes 10 thru 80 or five files of one type and size of sizes 90 thru 140 shall be packaged in a plastic tray having a slip-over cover or a hinged cover having a friction type closure. The tray shall be designed with cavities or inserts to hold each file in an individual cell to prevent movement and damage to the operative end. The cover shall be secured with a strip of pressure-sensitive tape. The plastic container shall be further packaged in accordance with MIL-P-116, method IC-1.

5.1.1.5 Intermediate package. Ten unit packages containing files of one class and size only shall be packaged in a box conforming to PPP-B-566 or PPP-B-676. Closure shall be as specified in the applicable box specification.

5.1.2 Level C. The level C preservation for files shall conform to MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B, or C, as specified (see 6.1).

5.2.1 Level A. Ten intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class weather-resistant. Closure, strapping, and waterproofing shall be as specified in the appendix of the box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. Ten intermediate packages (576 units) containing files of one class and size only shall be packed in a shipping container designed for a type 2 load and constructed in accordance with PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The level C packing for files shall conform to MIL-STD-794 requirements for this level.

5.2.4 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Quantities less than 40 cubic feet need not be unitized. Unitized loads shall beuniform in size and quantities to the greatest extent practicable.

5.2.4.1 Level A and B. Files, packed as specified in 5.2.1 and 5.2.2, shall be unitized on pallets conforming to MIL-STD-147.

5.2.4.2 Level C. Files packed as specified in 5.2.3, shall be unitized on pallets in conformance with MIL-STD-794.

5.3 Marking.

5.3.1 Levels A, B and C. Each unit pack, intermediate package, exterior container, and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2 and 5.2.3) shall be of minimum tare cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.3.1.

6. NOTES

6.1 Ordering data.

6.1.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number, and date of this specification.
b. Class and size required (see 1.2).
c. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 National Stock Number (NSN) coverage. This specificaiton covers the following items listed in the Federal Supply Catalog.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

NSN	ITEM IDENTIFICATION
	FILE, PULP CANAL, DENTAL, 21 mm End Length
6520-01-181-6852	Ogee, Standardized, Size 10, 10s
6520-01-182-9503	Ogee, Standardized, Size 15, 10s
6520-01-182-9502	Ogee, Standardized, Size 20, 10s
6520-01-182-9504	Ogee, Standardized, Size 25, 10s
6520-01-181-6853	Ogee, Standardized, Size 30, 10s
6520-01-181-7016	Ogee, Standardized, Size 35, 10s
6520-01-181-7017	Ogee, Standardized, Size 40, 10s
6520-01-181-7019	Ogee, Standardized, Size 45, 10s
6520-01-181-7012	Ogee, Standardized, Size 50, 10s
6520-01-184-1581	Ogee, Standardized, Size 55, 10s
6520-01-181-7020	Ogee, Standardized, Size 60, 10s
6520-01-182-8661	Ogee, Standardized, Size 70, 10s
6520-01-182-2020	Ogee, Standardized, Size 80, 10s
6520-01-181-6854	Ogee, Standardized, Size 90, 5s
6520-01-182-9505	Ogee, Standardized, Size 100, 5s
6520-01-181-7013	Ogee, Standardized, Size 110, 5s
6520-01-181-7014	Ogee, Standardized, Size 120, 5s
6520-01-181-7015	Ogee, Standardized, Size 130, 5s
6520-01-182-1953	Ogee, Standardized, Size 140, 5s
	FILE, PULP CANAL, DENTAL, 25 mm End Length
6520-01-182-8662	Ogee, Standardized, Size 10, 10s
6520-01-181-7021	Ogee, Standardized, Size 15, 10s
6520-01-181-7022	Ogee, Standardized, Size 20, 10s
6520-01-181-7023	Ogee, Standardized, Size 25, 10s
6520-01-181-7018	Ogee, Standardized, Size 30, 10s
6520-01-181-7024	Ogee, Standardized, Size 35, 10s
6520-01-182-3924	Ogee, Standardized, Size 40, 10s
6520-01-181-7025	Ogee, Standardized, Size 45, 10s
6520-01-184-1582	Ogee, Standardized, Size 50, 10s
6520-01-184-1583	Ogee, Standardized, Size 55, 10s
6520-01-184-6713	Ogee, Standardized, Size 60, 10s
6520-01-182-8665	Ogee, Standardized, Size 70, 10s
6520-01-182-8666	Ogee, Standardized, Size 80, 10s
6520-01-182-4635	Ogee, Standardized, Size 90, 5s
6520-01-182-4636	Ogee, Standardized, Size 100, 5s
6520-01-182-3926	Ogee, Standardized, Size 110, 5s
6520-01-182-3927	Ogee, Standardized, Size 120, 5s
6520-01-182-3928	Ogee, Standardized, Size 130, 5s
6520-01-182-1954	Ogee, Standardized, Size 140, 5s

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

FILE, PULP CANAL, DENTAL, 30 mm End Length

6520-01-182-9506	Ogee, Standardized, Size 10, 10s
6520-01-182-1955	Ogee, Standardized, Size 15, 10s
6520-01-185-4050	Ogee, Standardized, Size 20, 10s
6520-01-182-9507	Ogee, Standardized, Size 25, 10s
6520-01-182-9508	Ogee, Standardized, Size 30, 10s
6520-01-182-4637	Ogee, Standardized, Size 35, 10s
6520-01-182-3925	Ogee, Standardized, Size 40, 10s
6520-01-182-8667	Ogee, Standardized, Size 45, 10s
6520-01-181-7026	Ogee, Standardized, Size 50, 10s
6520-01-181-7027	Ogee, Standardized, Size 55, 10s
6520-01-185-3315	Ogee, Standardized, Size 60, 10s
6520-01-185-3316	Ogee, Standardized, Size 70, 10s
6520-01-183-9807	Ogee, Standardized, Size 80, 10s
6520-01-183-9808	Ogee, Standardized, Size 90, 5s
6520-01-184-6712	Ogee, Standardized, Size 100, 5s
6520-01-182-8663	Ogee, Standardized, Size 110, 5s
6520-01-182-1956	Ogee, Standardized, Size 120, 5s
6520-01-182-8664	Ogee, Standardized, Size 130, 5s
6520-01-182-1957	Ogee, Standardized, Size 140, 5s

MILITARY CUSTODIANS:
Army-MD
Navy-MS
Air Force - 03

Preparing Activity:
DoD-MB

Agent:
DLA-DM

Project No. 6520-1872

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:47Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

TRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in nitting comments and suggestions for improvements. All users of military standardization documents are invited to provide estions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and ed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the blems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an nowledgement will be mailed to you within 30 days to let you know that your comments were received and are being sidered.

TE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of ification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

ISE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

:IAL BUSINESS
LTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
MIL-F-37992	File, Pulp Canal, Dental, Ogee

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil – Downloaded: 2026-10-21T11:47Z
Check the source to verify that this is the current version before use.