
FED. SUP CLASS
6640

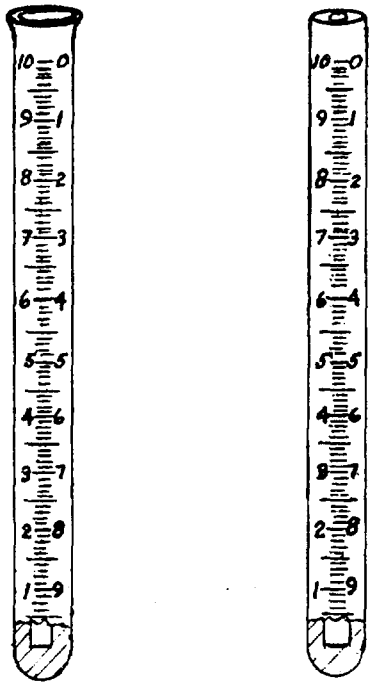

PART NUMBER	DIMENSIONS mm		
	INSIDE DIAMETER	OUTSIDE DIAMETER	OVERALL LENGTH
MS36184-1	2.87 to 3.35	6.5 to 8	110 to 117
MS36184-2	2.90 to 3.50	5 ± 0.25	110 to 117

MATERIAL: Tubes shall be of borosilicate glass in accordance with ASTM E438. MS36184-1 shall be type I, Class A; MS36184-2 shall be Type I or Type II.

DESIGN: Each tube shall bear sharp, distinct graduations, from 1 to at least 100 mm, upward from flat inner bottom, using a single double-numbered scale. Scale shall be numbered from 1 to 10 at 10 mm intervals, upward from flat bottom on one side and downward to flat bottom on the other side. Overall graduation scale tolerance is ± 0.25 mm.

MS36184-1 tube shall have a beaded, flared top.

MS36184-2 tube shall have smooth-finish open end, cut square across top, without beading or lip.

Graduations for MS36184-1 tubes shall be either etched and filled with permanent pigment or pigment fired into the glass.

Graduations for MS36184-2 tubes shall be sharp and distinct under ordinary usage, including centrifuging, for at least one use.

NOTES:
1. Procurement document for MS36184-1 is Federal Specification DD-T-200, Type II.
2. Procurement document for MS36184-2 is Military Specification MIL-T-36153.

(C) ENTIRE STANDARD REVISED

APPROVED 30 Dec 1960 REVISED (A) 20 June 1969 (B) 1 Oct 1974 (C) 7 DEC 1983

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
AIR FORCE - 82

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
EA		TEST TUBE, HEMATOCRIT DETERMINATION, WINTROBE TYPE	MS36184
Other Cust MS 99			
Procurement Specifications: See NOTES 1 and 2	SUPERSEDES:		SHEET 1 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1208

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.

FED. SUP CLASS
6640

3. MS36184-1 shall be supplied with a rubber cap.

4. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

5. For design feature purposes, this standard takes precedence over procurement documents referenced herein.

6. Referenced documents shall be of the issue in effect on date of invitations for bid.

7. FSCM: 13134 and 22527.

USER ACTIVITIES:

REVIEWER ACTIVITIES:

APPROVED REVISED

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A. / Other Cust	INTERNATIONAL INTEREST	TITLE: TEST TUBE, HEMATOCRIT DETERMINATION, WINTROBE TYPE	MILITARY STANDARD MS36184
Procurement Specifications: See NOTES 1 and 2	SUPERSEDES:		SHEET 2 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1208

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.