RR-R-0015a(DSA-DM)
29 September 1966
Interim Revision of
Fed. Spec. RR-R-15
11 January 1951

INTERIM FEDERAL SPECIFICATION

RACK, DRYING, BEDPAN AND URINAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania, 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification RR-R-15.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers a wall type drying rack for urinals and bedpans.

1.2 Classification. Type, grade, and size. The drying rack covered by this specification shall be of one type, grade, and size, as hereinafter specified.

2. APPLICABLE DOCUMENTS

2.1 The following specifications and standards of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

SPECIFICATIONS

Federal

QQ-S-766 Steel, Plates, Sheets, and Strips - Corrosion Resisting.
PPP-B-585 Boxes, Wood, Wirebound.
PPP-B-601 Boxes, Wood, Cleated-Plywood.
PPP-B-621 Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 Box, Fiberboard.

Military

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-151 Metals; Test Methods.

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices, in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specification and Standards from established distribution points in their agencies.)

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN WELDING SOCIETY

TYPE E304 Welding Rod.

(Applications for copies should be addressed to United Engineering Center, 345 East 47 Street, New York, New York 10017.)

3. REQUIREMENTS

3.1 First Article. Unless otherwise specified, prior to the start of production of the contract quantity, sample(s) of the drying rack shall be assembled, completely finished, and tested by the contractor. The sample(s) shall be submitted, together with the contractor's inspection and test reports, to the procuring contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the procuring contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Pending approval of the first article(s), acquisition of materials, components, or commencement of production is at the sole risk of the contractor. Accepted sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

3.2 Materials.

3.2.1 Steel. The steel shall be corrosion resisting, Class 304 conforming to the requirements of QQ-S-766.

3.2.2 Welding Rod. Welding rod shall be American Welding Society Type E308. All welding to be done by qualified welders approved for this class of work.

3.3 Design and construction. The drying rack shall be of the design and size illustrated in figure 1 and 2. The rack shall be welded throughout, of durable and sound construction in all details.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

3.3.1 Frame. The frame shall be panel design, constructed of not less than 0.0478-inch-thick sheet, No. 18, United States Standard Gage (No. 18, U.S.S. Gage). The sides shall be flanged 1 inch; top edge shall be flanged outward 1 inch and upward 1 inch, forming a hanger. The bottom edge shall be flanged outward and downward. Holes shall be provided in top and bottom flanges for wall attachment. All corners shall be continuously and fully welded.

3.3.2 Hangers. The top and bottom vertical flanges of the panel shall be provided with holes for fastening the rack to the wall. The horizontal flange at the bottom of the panel shall be pitched upward $10^{\circ} + 1^{\circ}$ to prevent drops of water from reaching the wall.

3.3.3 Urinal holder. Each urinal holder shall be constructed from a continuous piece of strip material, 1 inch wide, 0.1196 inch thick, (No. 11, U.S.S. Gage). The holder shall be a circular clamp design, 2-7/8 inches in diameter, with a clear opening at the front, 3/4 inch wide. The curve at the back shall be formed in a rectangular shape, measuring 1-3/4 inches long by 1-1/2 inches wide. The urinal holders shall be uniformly mounted on the frame as shown in figure 1 and 2, and shall be suitably welded thereto to properly support the urinal.

3.3.4 Bedpan holder. The bedpan holder shall be oblong in shape and constructed of 0.1196 inch thick, No. 11 U.S.S. Gage, inch wide strip material, and shall measure 12 inches long by 5-1/4 inches wide, outside measurements. The front corners shall be formed to a 1-3/8 inch radius; back corners shall be formed to 90° terminating into back members 3 inches long. Each bedpan holder shall have an integral center member constructed of No. 11, U.S.S. Gage, 1 inch wide strip material to serve as a bottom support for the bedpan. The bedpan holders shall be uniformly mounted on the frame as shown in figure 1and 2, and shall be suitably welded thereto to properly support the bedpans.

3.3.5 Drip-pan support. One triangular bracket with one arm flanged and with integral base support for the drip pan, shall be suitably welded to each of the bottom corners of the frame. The bracket shall be made of 0.1196 inch thick, No. 11 U.S.S. Gage, corrosion-resisting steel. The 1-1/2 inch member of the angle shall be tack welded to the bottom vertical flange of the frame leaving the vertical flange free as a vertical backstop for the drip pan. The 4 inch side upright of the bracket shall be suitably welded to the outside of the side flange of the frame along the part of its surface which comes in contact with that flange. The front to rear dimensions of the bracket shall be 6 inches.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

3.3.6 Drip pans. The drip pans shall be fabricated of No. 11 U.S.S. Gage corrosion-resisting steel, 25-3/4 inches long, 6 inches wide, and 1-1/4 inches high, with welded corners fully hemmed. The pan shall fit freely into the supports described in 3.3.5.

3.4 Finish. All exposed surfaces shall conform to the requirements of QQ-S-766 for No. 4 commercial grind. Unexposed surfaces and welds shall be finished in a proper manner in accordance with the best commercial practice. All exposed welds shall be ground smooth to eliminate traces of pitmarks and seams, and shall be polished to blend with the adjacent surfaces. All edges and corners shall be rounded, ground smooth, or otherwise treated to eliminate burrs and sharp or ragged edges.

3.5 Marking. Each rack shall be permanently marked with the name or registered trademark of the manufacturer.

3.6 Workmanship. The workmanship shall be first class throughout. The racks shall be smoothly and properly finished and free from defects which detract from their appearance or which may impair their serviceability.

3.6.1 Welding. The welding members shall be carefully and properly aligned prior to welding in order to provide a straight and rigid assembly.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total (major and minor defects combined)	II	4.0
For dimensional examination	S-3	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105.

Component (unit of product)	Characteristic	Requirement	Test procedure	Inspection level	AQL
Rack, Drying	Chemical composition	3.1.1	4.2.3 and 4.4.1	*	**

* Sample as specified in 4.2.3.
** Not less than three samples shall be taken, regardless of lot size. Acceptance number shall be zero for all sample sizes.

4.2.3 Raw materials. Four ounces of each lot of metal used in the construction of the racks shall be selected for chemical analysis.

4.3 Examination. The racks shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects *	
Major	
101	Rack not free of cracks, tears, holes, ripples, or identification marking penetration.
102	Edges not free of burrs or sharp edges.
103	Identification marking incomplete, or not legible.
Minor	
201	Finish not free of scratches or mar marks.
202	Rack not free of grease, oil, dirt, chips, or other foreign matter.
203	Rack does not mount evenly on a flat wall surface.

*Examination shall not be restricted to the classified possible defects listed above.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The rack shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Fed. Test Method Std. No. 151.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One rack, as specified, constitutes one unit of issue, one each.

5.1.2 Level A.

5.1.3 Unit package. Each unit shall be completely wrapped in kraft paper; all corners shall be padded with cushioning material or with flexible corrugated fiberboard; which shall be firmly affixed to the unit by means of kraft gummed tape, cotton tape, or twine.

5.1.4 Level C. Units shall be packaged in such a manner, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Each unit as packaged in paragraph 5.1.3 shall be packed in a exterior container, designed for type 2 load, conforming to the requirements of PPP-B-585, style 3, for class 2 use; PPP-B-601, table II, using type III, class 1 plywood; or PPP-B-621, table III.

5.2.1.2 Case liner. Each box shall be lined with a waterproof case liner conforming to MIL-L-10547. Care shall be exercised not to rupture the liner when the unit is block and braced within the container. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Each unit as packaged in paragraph 5.1.3 shall be packed in a exterior container, designed for type 2 load, conforming to the requirements of PPP-B-585, style 3, for class 2 use; PPP-B-601, table I, using type III, class 1 plywood; or PPP-B-621, table I. Each unit shall be secured within the shipping container by means of braces, blocks, or cushioning material in such a manner as to insure against shifting, damage,or marring of surfaces.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The drying rack covered by this specification is intended for use in government hospitals for drying urinals and bedpans following sterilization.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) When First Article is not required (see 3.1).
(c) Where First Article shall be sent (see 3.1).
(d) Selection of applicable levels of packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.


Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

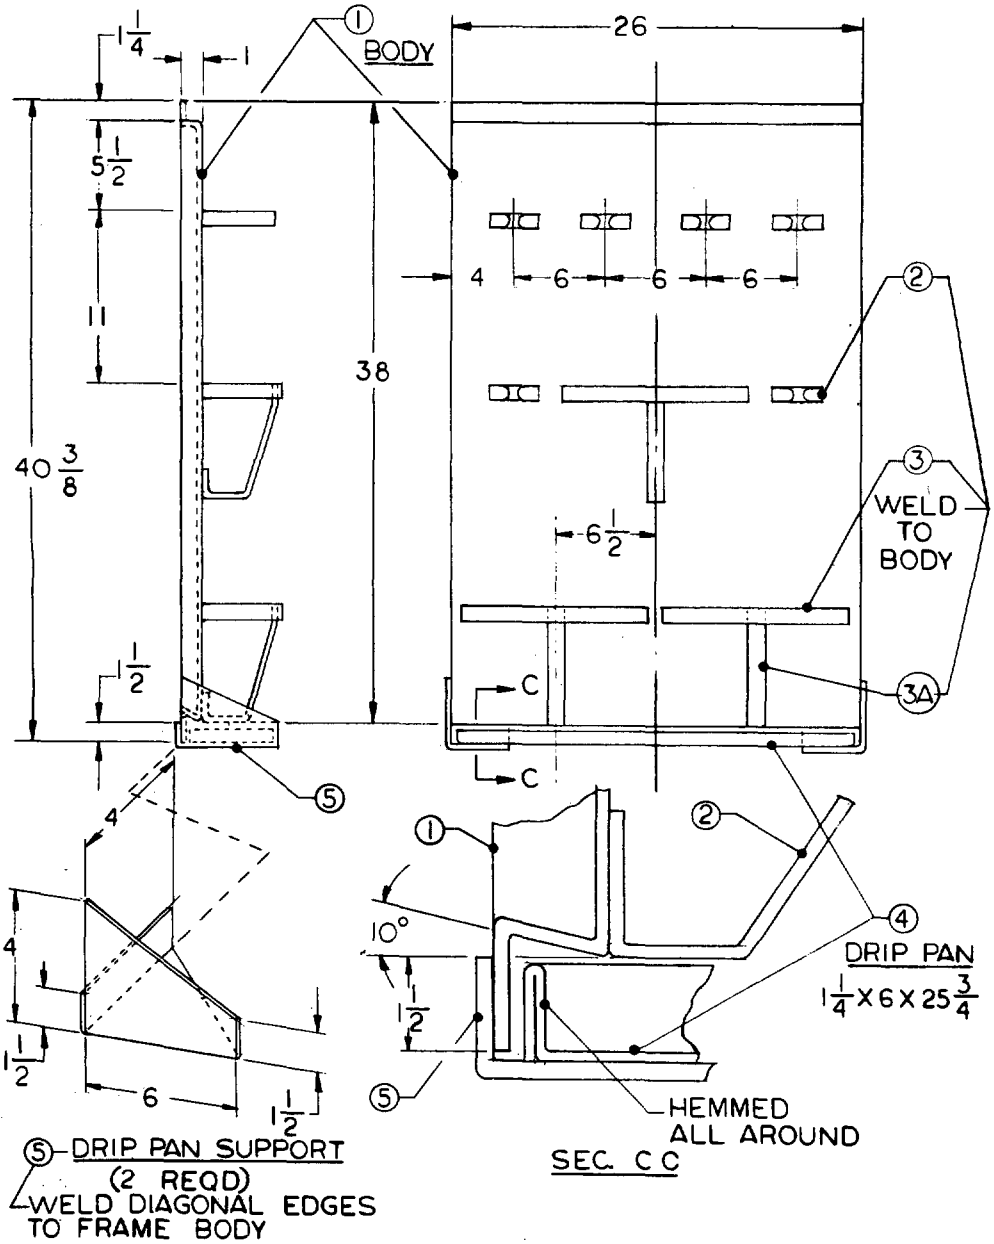

RACK, DRYING, BEDPAN AND URINAL

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

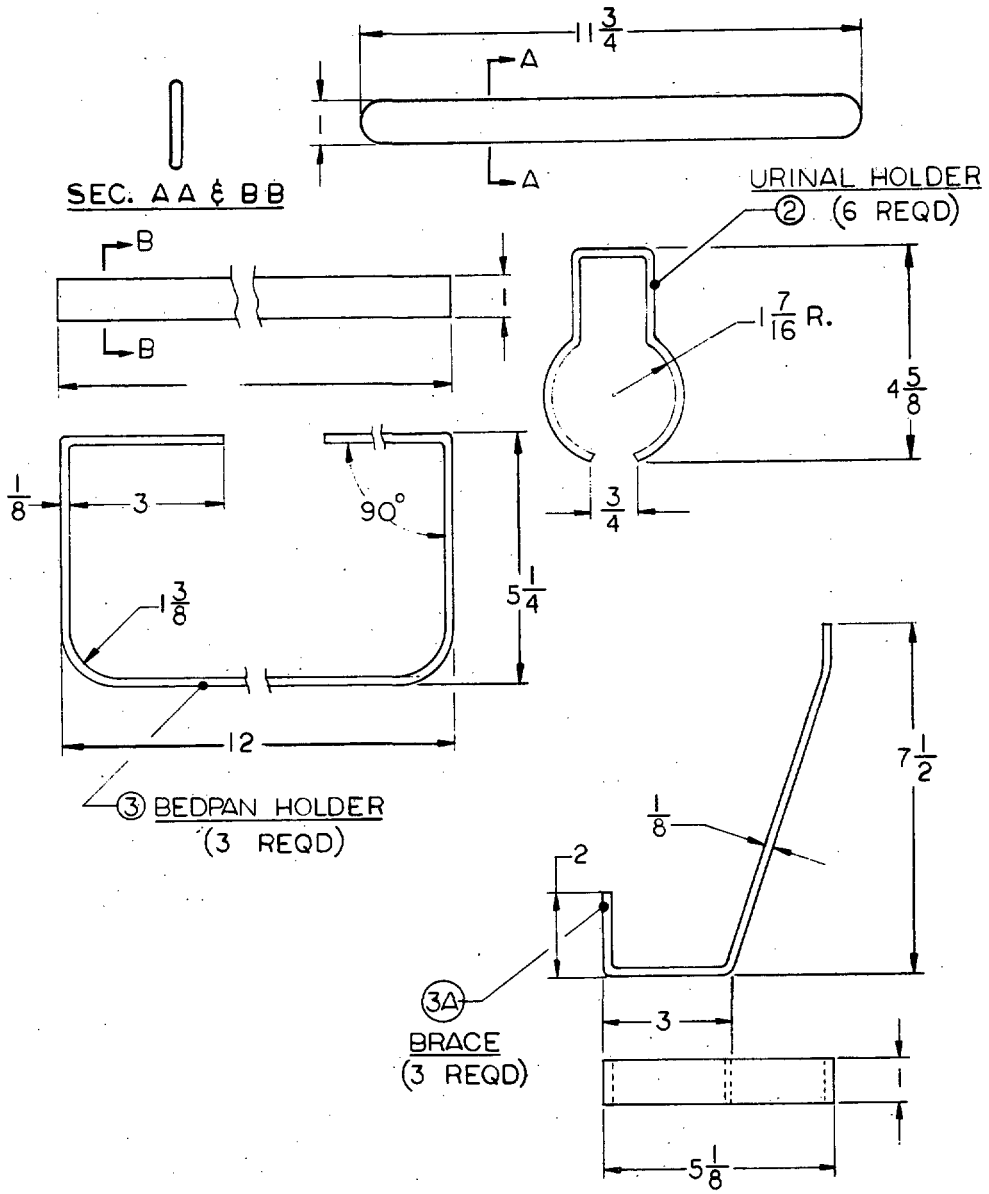


FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

RR-R-0015a (DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 65 1426

REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
AUG 66

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.