RR-R-15
11 JANUARY 1951

FEDERAL SPECIFICATION

RACK, UTENSIL (FOR SIX URINALS AND THREE BEDPANS)

This specification was approved on the above date by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. CLASSIFICATION

1.1 **Type, grade, and size.**—Utensil racks covered by this specification shall be of one type, grade, and size, as hereinafter specified.

2. APPLICABLE SPECIFICATIONS

2.1 The following Federal Specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

QQ-M-151—Metals; General Specification for Inspection of.

QQ-S-766—Steel; Corrosion-Resisting; Plates, Sheets, Strips, and Structural Shapes.

(Copies of Federal specifications and the Federal Specifications Index may be obtained upon application accompanied by postal note, money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C. Prices may be obtained from the Superintendent of Documents.)

2.2 Specifications applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 **Description.**—The utensil rack shall be a wall-type rack of compact design requiring minimum wall space for hanging.

3.2 **Material.**

3.2.1 *Steel.*—The steel shall be corrosion-resisting throughout conforming to the requirements of Federal Specification QQ-S-766, class 1.

3.2.2 *Welding rod.*—The welding rod shall be corrosion-resisting steel similar in composition to the welded members.

3.3 **Design and construction.**—The utensil rack shall be of the design illustrated in figure 1. The rack shall be welded throughout, of durable and sound construction in all details. All exposed welds shall be ground smooth to eliminate traces of pit marks and seams, and shall be polished to blend with the adjacent surfaces. All edges and corners shall be rounded, ground smooth, or otherwise treated to eliminate burrs and sharp or ragged edges.

3.3.1 *Size.*—The over-all dimensions of the rack shall be approximately 40⅜ inches long, 26 inches wide, and 6⅛ inches deep.

3.3.2 *Frame.*—The frame shall be panel design, constructed of not less than 0.050-inch-thick sheet, approximately 38 inches long by 26 inches wide. The sides shall be flanged 1-inch; top edge shall be flanged outward 1-inch and upward 1-inch, forming a hanger. The bottom edge shall be flanged outward and downward. Holes shall be provided in top and bottom flanges for wall attachment. All corners shall be continuously and fully welded.

3.3.3 *Hangers.*—The top and bottom vertical flanges of the panel shall be provided

901697—51—(1)(c)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

with holes for fastening the rack to the wall. The horizontal flange at the bottom of the panel shall be pitched upward approximately 10° to prevent drops of water from reaching the wall.

3.3.4 *Urinal holder.* — Each urinal holder shall be constructed from a continuous piece of strip material, 1 inch wide by 1/8 inch thick. The holder shall be a circular clamp design approximately 2 7/8 inches in diameter, with a clear opening at the front approximately 3/4 inch wide. The curve at the back shall be formed into a rectangular shape, measuring approximately 1 3/4 inches long by 1 1/2 inches wide. The urinal holders shall be uniformly mounted on the frame as shown in figure 1, and shall be suitably welded therto to properly support the urinal.

3.3.5 *Bedpan holder.*—The bedpan holder shall be oblong in shape and constructed of 1/8-inch-thick by 1-inch-wide strip material, and shall measure approximately 12 inches long by 5 1/4 inches wide, outside measurements. The front corners shall be formed to a 1 3/8-inch radius; back corners shall be formed to 90° terminating into back members approximately 3 inches long. Each bedpan holder shall have an integral center member constructed of 1/8-inch-thick by 1-inch-wide strip material to serve as a bottom support for the bedpan. The bedpan holders shall be uniformly mounted on the frame as shown in figure 1 and shall be suitably welded thereto to properly support the bedpans.

3.3.6 *Drip-pan support.* — One triangular bracket with one arm flanged and with integral base support for the drip pan, shall be suitably welded to each of the bottom corners of the frame. The bracket shall be made of 0.050-inch-thick corrosion-resisting steel. The 1 1/2-inch member of the angle shall be tack welded to the bottom vertical flange of the frame leaving the vertical flange free as a vertical backstop for the drip pan. The 4-inch side upright of the bracket shall be suitably welded to the outside of the side flange of the frame along the part of its surface which comes in contact with that flange. The front-to-rear dimensions of the bracket shall be 6 inches.

3.3.7 *Drip pans.*—The drip pans shall be fabricated of 0.050-inch-thick corrosion-resisting steel, 25 3/4 inches long, 6 inches wide, and 1 1/4 inches high, with welded corners fully hemmed. The pan shall fit freely into the supports described in 3.3.6.

3.4 **Finish.** — All exposed surfaces shall conform to the requirements of Federal Specification QQ-S-766 for No. 4 commercial grind. Unexposed surfaces and welds shall be finished in a proper manner in accordance with the best commercial practice. When tested as specified in 4.3.2, a slight surface corrosion which can be easily washed off shall not be considered cause for rejection. Rust or continuous corrosion from pit marks shall be considered as cause for rejection.

3.5 **Marking.**—Each rack shall be permanently marked with the name or registered trade-mark of the manufacturer. Marking may be accomplished by stenciling or other permanent means.

3.6 **Workmanship.**—The workmanship shall be first class throughout. The racks shall be smoothly and properly finished and free from defects which detract from their appearance or which may impair their serviceability.

3.6.1 *Welding.* — The welding members shall be carefully and properly aligned prior to welding in order to provide a straight and rigid assembly.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 **Sampling.**—Unless otherwise specified, at least 1 utensil rack shall be taken at random from each lot of 20 or fraction thereof delivered, for inspection and tests.

4.2 **Inspection.**—The sample shall be in-

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

spected for workmanship, material, dimensions, design, construction, finish, packaging, packing, and marking.

4.3 Tests.

4.3.1 *Chemical composition.*—Millings or drillings shall be taken from racks to determine conformance of the material to the requirements of 3.2.1. The millings or drillings shall weigh not less than 4 ounces and shall be clean, free from dirt, oil, grit, or other foreign matter. Spectrographic analysis may be made in lieu of the above.

4.3.2 *Salt spray.*—The salt-spray test shall be conducted in a closed tank made of neutral material such as wood or soapstone. The test shall consist of exposing the sample utensil rack, to a very fine spray of 10 percent solution of sodium chloride C.P. (by weight) in distilled water at a temperature of 95° ± 5° F. for a period of 48 hours. The tank shall be so designed that there shall be no direct impingement of the spray upon the utensil rack, and the spray shall circulate freely about the specimen to the same degree of contact for uniform action. No liquid which has come in contact with the specimen under test shall return to the aspirator to be resprayed. Before being placed in the salt-spray bath, the utensil rack shall be thoroughly cleaned by washing in petroleum ether and alcohol and then dried.

5. PREPARATION FOR DELIVERY

5.1 **Packaging.** — Unless otherwise specified, each rack shall be packaged in accordance with accepted commercial practice.

5.2 **Packing.**—Unless otherwise specified, the subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 **Marking.**

5.3.1 *Packages.*—Unless otherwise specified, each package shall be marked with the name of the commodity, stock number, quantity contained therein, and the name of the contractor and the manufacturer.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, name of the contractor, number of the contract or order, name and address of the consignee, and the gross weight.

6. NOTES

6.1 **Ordering data.** — Purchasers should exercise any desired options offered herein. (See 4.1, 5.1, 5.2, 5.3, and 7.2.5.)

6.2 This specification covers the following item listed in the Armed Services Catalog of Medical Materiel:

7–071–975—Rack, Utensil, 6 Urinals and 3 Bedpans.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications.*

Federal Specifications:

NN-B-601 —Boxes; Wood-Cleated-Plywood, for Domestic Shipment.

NN-B-621 —Boxes; Wood, Nailed and Lock-Corner.

NN-B-631 —Boxes; Wood, Wirebound, for Domestic Shipment.

Military Specifications:

JAN-P-105 —Packaging and Packing for Overseas Shipment—Boxes, Wood, Cleated Plywood.

JAN-P-106 —Packaging and Packing for Overseas Shipment—Boxes; Wood, Nailed.

JAN-B-107 —Boxes, Wood, Wirebound (Overseas Type).

JAN-P-125 —Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.

JAN-P-140 —Packaging and Packing for Overseas Shipment — Adhesives, Water-Resistant, Case-Liner.

MIL-M-3157—Marking of Domestic Shipments by Contractors for Supplies and Equipment Consigned to the Medical Departments of the Armed Services.

Navy Department Specification:

General Specifications for Inspection of Material.

(Copies of specifications required for Army purchases may be obtained upon application to the procuring agency. Both the title and identifying symbol or number should be stipulated when requesting copies.

(Copies of Federal and Military specifications required for Navy purchases, and Navy Department Specifications may be obtained without cost upon application to the Bureau of Supplies and Accounts, Department of the Navy, Washington 25, D. C.; except that Naval activities should make application to the Commanding Officer, Naval Supply Center, Norfolk 11, Virginia. Both the title and identifying symbol or number should be stipulated when requesting copies of specifications.

(Copies of specifications required for Air Force purchases may be obtained from the Commanding General, Air Matériel Command, Wright-Patterson Air Force Base, Dayton 1, Ohio. Both the title and identifying symbol or number should be stipulated when requesting copies.)

7.2.2 *Packaging, domestic and overseas.*— One utensil rack constitutes one unit. Each unit shall be completely wrapped in kraft paper; all corners and edges shall be padded with excelsior pads or with flexible corrugated fiberboard, or any combination of the two; all of which shall be firmly affixed to the unit by means of kraft gummed tape, cotton tape, or twine.

7.2.3 *Packing.*

7.2.3.1 *Domestic.* — Each unit shall be packed in a shipping container conforming to the requirements of Federal Specification NN-B-601, NN-B-621, or NN-B-631. Each unit shall be secured within the shipping container by means of braces, blocks, or cushioning material in such a manner as to insure against shifting, damage, or marring of surfaces.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

7.2.3.2 *Overseas.* — Each unit shall be packed in a shipping container designed for type 2 load, conforming to the requirements of Military Specification JAN-P-105, JAN-P-106, or JAN-B-107. Closure and strapping shall conform to the requirements of the applicable box specification. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN-P-125, for case liners; seams and closures shall be completely sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Military Specification JAN-P-140.

7.2.3.3 *Packing variation permitted.* — If the number of units in any shipment is not the exact multiple of the number of units specified to be contained in each shipping container, the units not constituting the nearest such multiple shall be packed in a shipping container of suitable size and design, so constructed as to insure safe delivery to the specified destination.

7.2.4 *Marking.*

7.2.4.1 *Packages.*—Each package shall be marked with the stock number, nomenclature, unit, quantity, and the name of the contractor. When the contractor is not the manufacturer, the name of the manufacturer shall also appear as the manufacturer.

7.2.4.2 *Shipping containers.* — Each shipping container shall be marked in accordance with Military Specification MIL-M-3157.

7.2.4.2.1 *Precautionary markings.*—In addition to the marking specified above, each shipping container shall have a precautionary label permanently affixed to three of its surfaces with waterproof adhesive. The labels shall be RED with white print or WHITE with red print and shall bear a suitable legend indicating that the container contents are fragile.

7.2.5 *Ordering data.* — Requests, requisitions, schedules, and contracts or orders should specify domestic or overseas packing and marking of shipping containers. (See 7.2.3 and 7.2.4.2.)

NAVY INTEREST: M

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog.

For sale by the Superintendent of Documents, Washington 25, D. C. Price 5 cents.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:08Z
Check the source to verify that this is the current version before use.

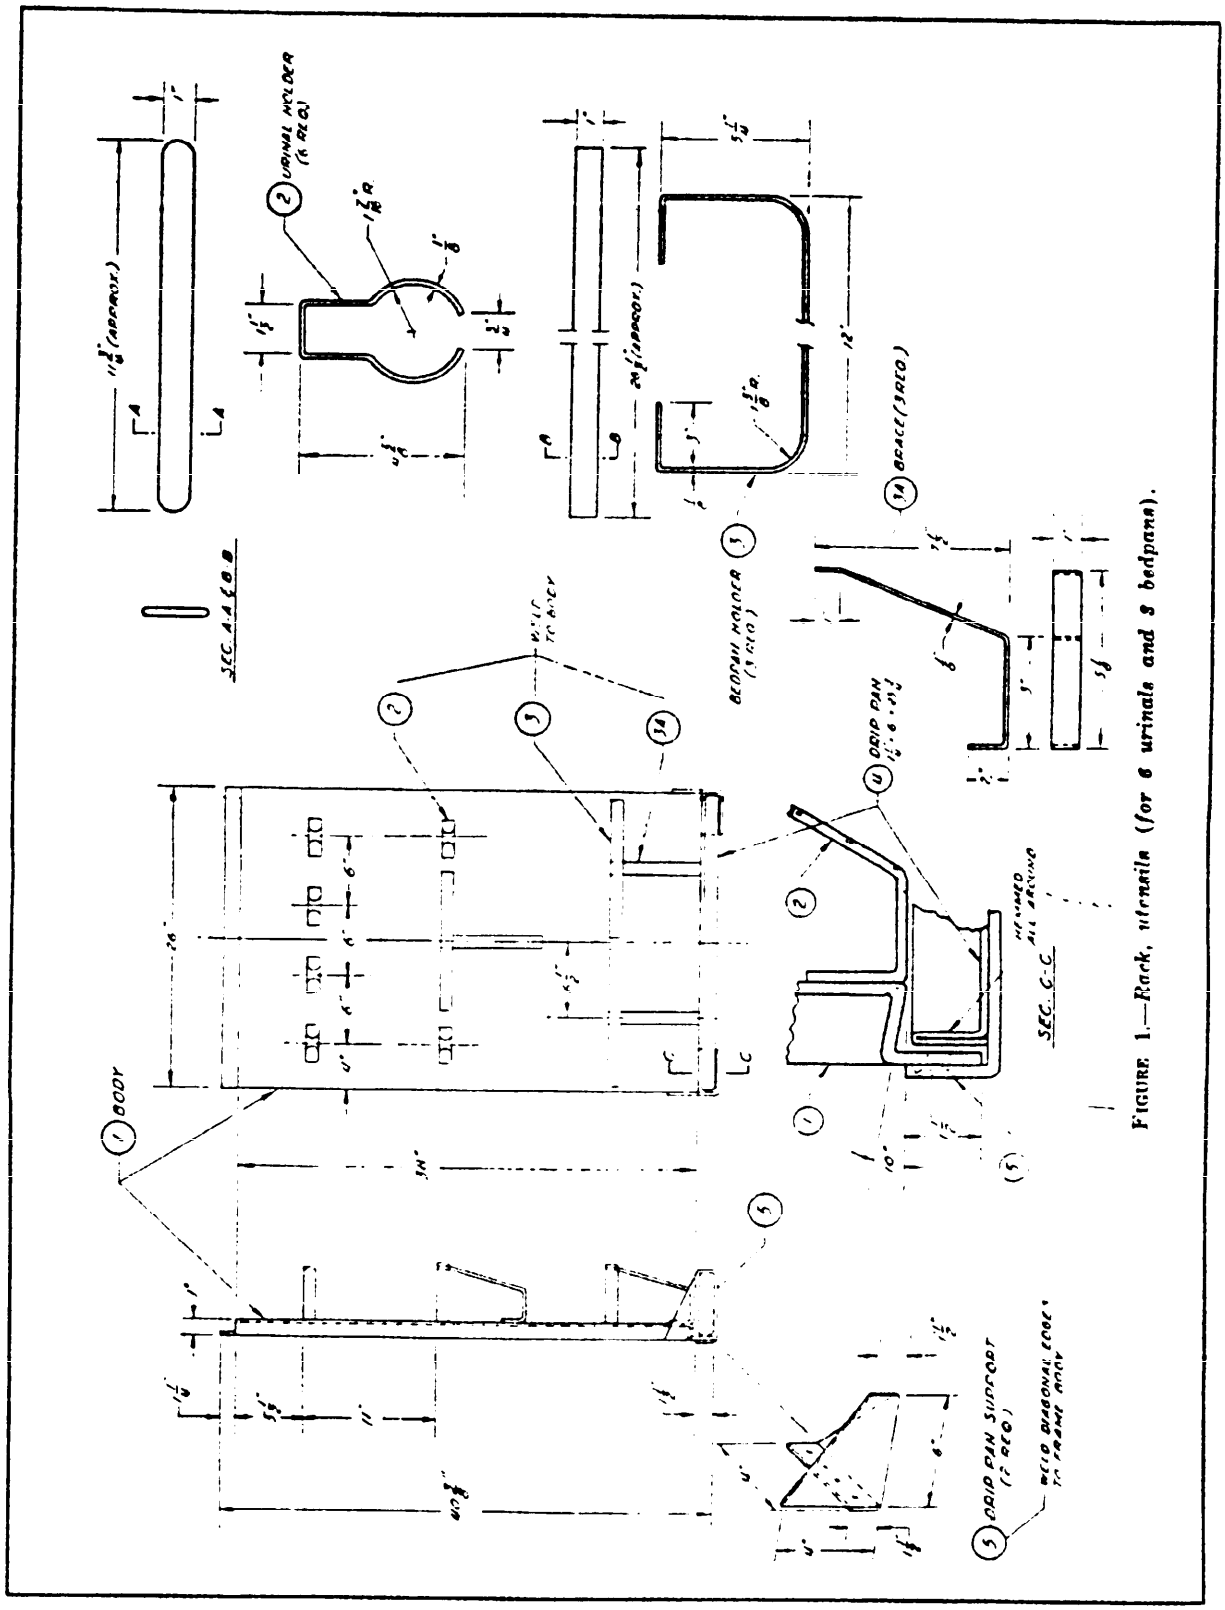


FIGURE 1.—*Rack, urinals (for 6 urinals and 3 bedpans).*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.