A-A-53270
16 November 1987

# COMMERCIAL ITEM DESCRIPTION

## TIP, DENTAL SUCTION APPARATUS

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a dental suction tip suitable for use in the high velocity evacuation of liquid and solid substances during dental procedures.

Salient Characteristics:

The tip shall be in accordance with the applicable requirements of GG-I-526.

Material. The tip shall be fabricated from bright annealed type 304 austenitic stainless steel.

Style, design and dimensions. The tip shall be of one-piece construction. It shall be round in cross section, bent in mid-length, and beveled on both ends such that the bevels are near parallel. The design and dimensions of the tip shall conform to Figure I.

Corrosion resistance. The tips shall show no sign of corrosion when tested in accordance with GG-I-526.

Finish. The outside surface of tip tubing shall have a smooth satin finish. The peripheral edge of tubing shall be chamfered to provide a smooth finish to avoid cutting of tissue. The inside surface of tubing shall be smoothly brushed to preclude attachment of foreign matter.


Workmanship. The tip shall be free from defects which detract from its appearance or impair its serviceability, proper functioning and intended use.

Unit. Each (EA). One tip, as specified, constitutes one unit.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

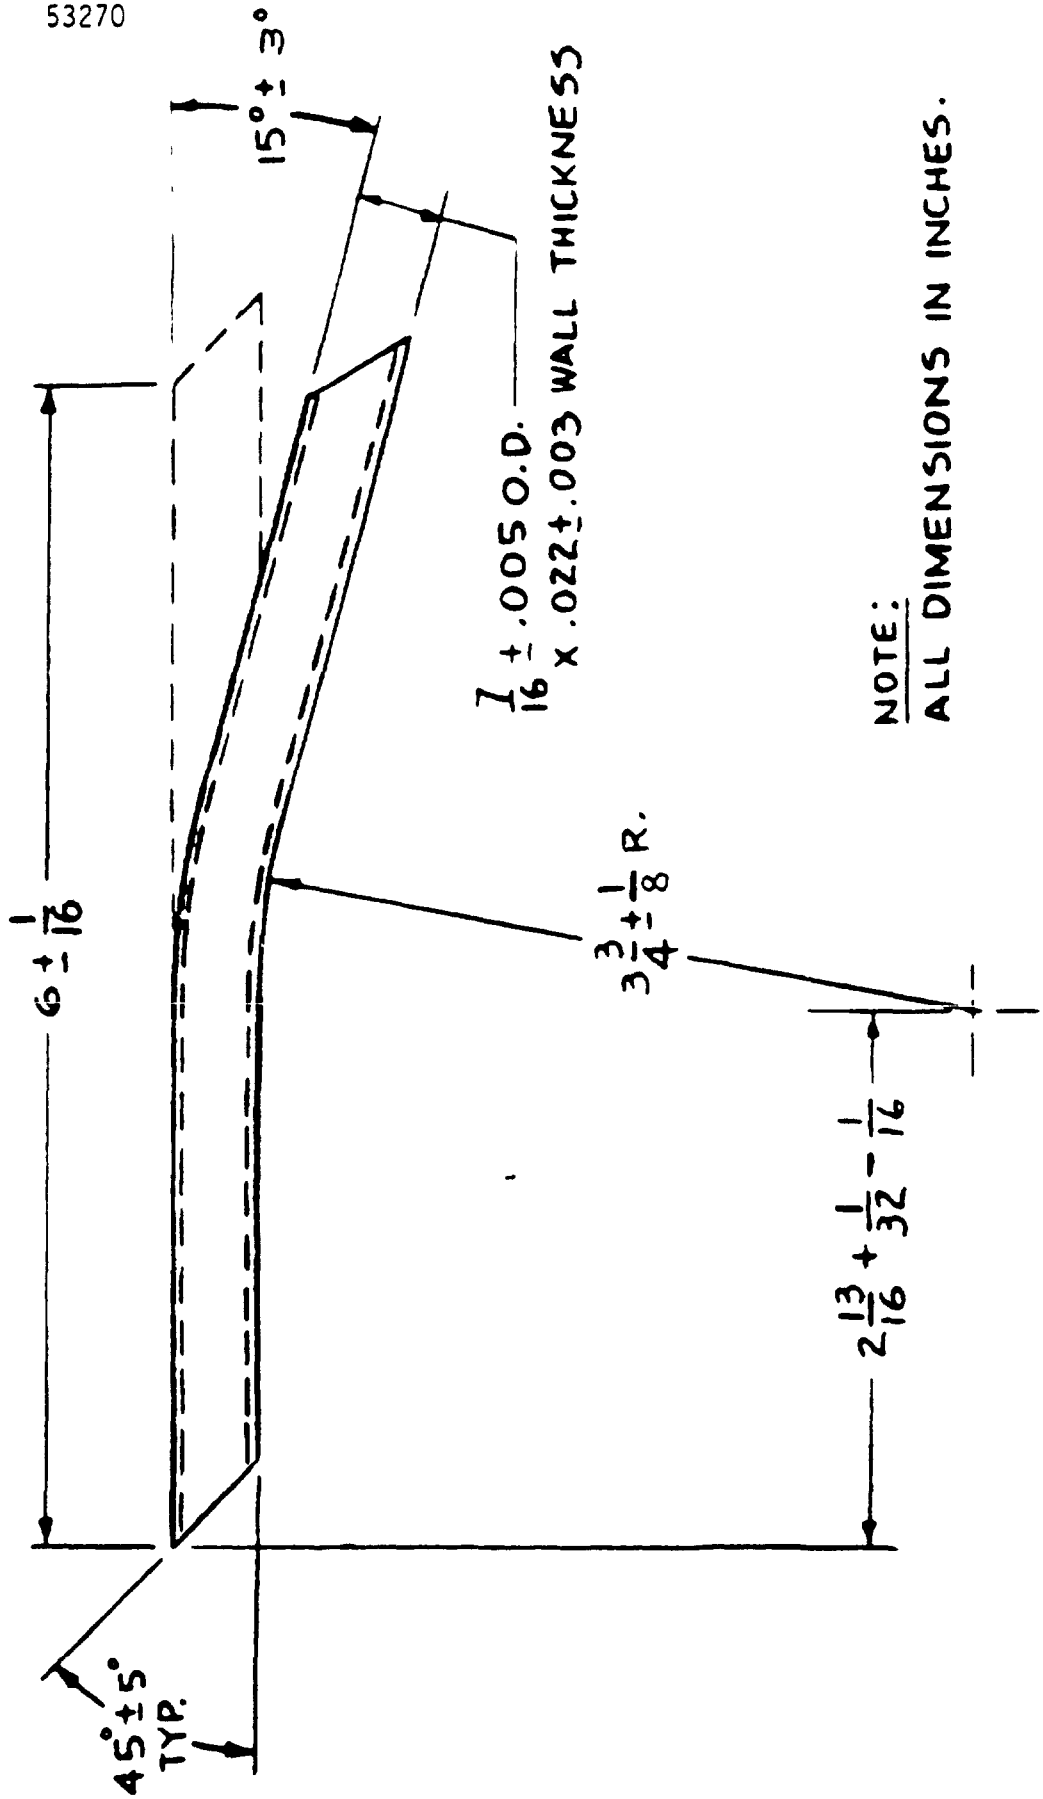


TIP, DENTAL SUCTION APPARATUS (LONG)

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one tip. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

Metric Products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

| National Stock Number | Item Identification |
|---|---|
| 6520-01-185-2532 | TIP, DENTAL SUCTION APPARATUS, High Velocity Evacuation, Round, 7/16 inch (1.1 cm) Diameter, 6 inch (15.2 cm) Long, Corrosion-Resisting Steel. |



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

The tip shall be suitable for use with NSN 6520-01-130-3796, Operatory, Dental, Field, Portable, and NSN 6520-00-140-7663, Dental Operating and Treatment Unit, Field, Portable.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

PGC 58311

Project No. 6520-2024



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

**INSTRUCTIONS** In a continuing effort to make our standardization documents better the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5 be as specific as possible about particular problem areas such as wording which required interpretation was too rigid, restrictive loose ambiguous or was incompatible and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

*NOTE* This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

*(Fold along this line)*

*Fold along this line)*

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1. DOCUMENT NUMBER | 2. DOCUMENT TITLE |
|---|---|
| A-A-53270 | TIP, DENTAL APPARATUS |

| 3a. NAME OF SUBMITTING ORGANIZATION | 4. TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR |
| | ☐ USER |
| b. ADDRESS *(Street, City, State, ZIP Code)* | ☐ MANUFACTURER |
| | ☐ OTHER *(Specify)* |

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

| 7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional | b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional | 8. DATE OF SUBMISSION *(YYMMDD)* |

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:17Z
Check the source to verify that this is the current version before use.