NNN-C-00545(DSA-DM)
11 December 1964
Interim Revision of
Fed. Spec. GG-T-741a
18 April 1952

INTERIM FEDERAL SPECIFICATION

CONNECTOR, ELASTIC TUBING, BRANCHED, METAL

This interim Federal specification was developed by the Defense Medical Supply Center, Third Avenue and 29th Street, Brooklyn, New York 11232, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-T-741a, dated 18 April 1952.

1. SCOPE

1.1 This specification covers one type of metal, Y-shaped, connecting tube.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up, Paperboard.

FSC 6640

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C., 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specification:

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Military Standards:

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Material shall be copper-plated brass of the highest quality throughout and suitable in all respects for the purpose intended.

3.2 Design and construction. Connector shall be a Y-shaped tube in accordance with figure 1. Each of the three arms shall have three turned grooves at the distal end to provide grip for rubber tubing. The arms shall be set in a heavy hexagonal hub of sturdy construction to resist fracture. The arms, when attached to the hexagonal hub, shall form an airtight connection. Arms shall be of equal length.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

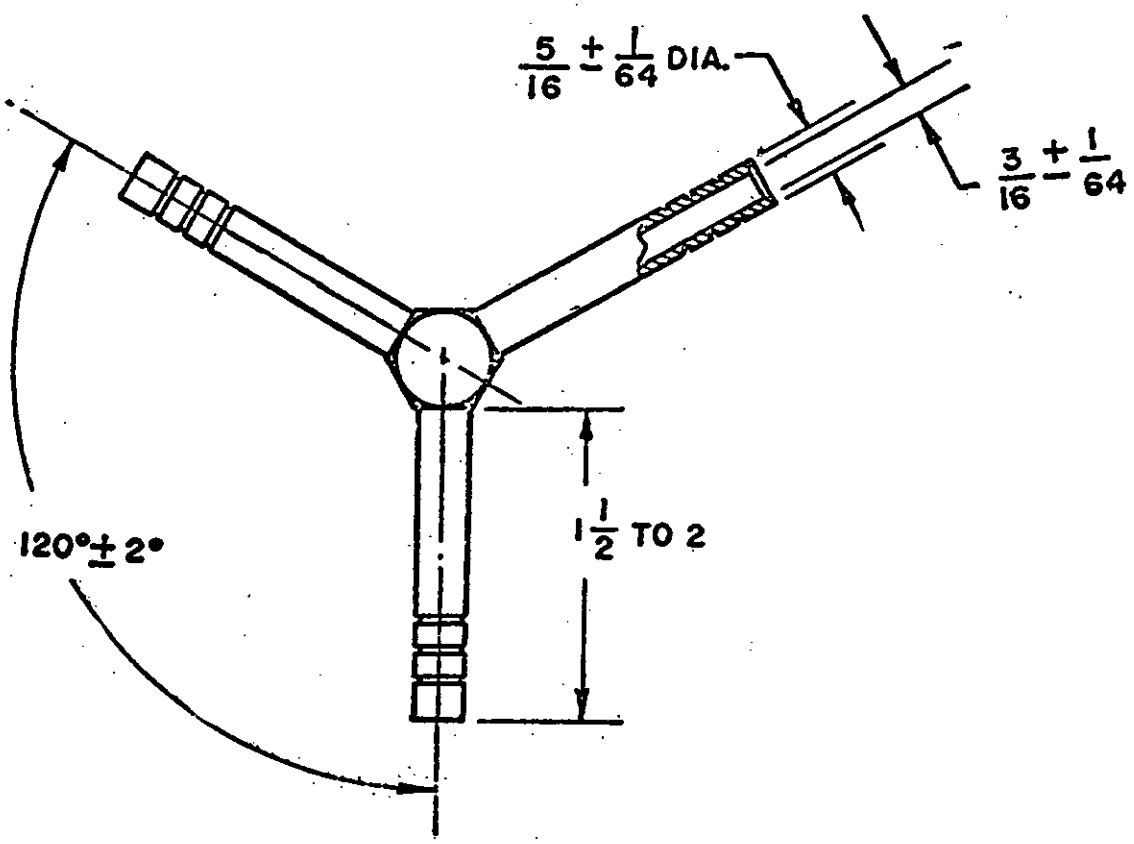


FIGURE 1.—Y-shaped metal connecting tube.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

3.3 Dimensions. Each arm shall be 1-1/2 to 2 inches long and shall have an outside diameter of 5/16 inch ± 1/64 inch and an inside diameter of 3/16 inch ± 1/64 inch.

3.4 Pressure. Connector shall be able to withstand a minimum air pressure of 20 pounds per square inch gage (p.s.i.g.) without air leakage, or any other physical damage, when tested as specified in 4.4.1.

3.5 Identification marking. Each Y-shaped metal connector shall be permanently and legibly marked with the name or registered trademark of the manufacturer.

3.6 Workmanship. Workmanship shall be first class throughout. Y-shaped metal connectors shall be free from defects which detract from their appearance or which may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

	Inspection level	AQL (percent defective)
For visual examination		
Major defects	II	2.5
Minor defects	II	4.0
For dimensional examination	S-2	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105.

Component (unit of product)	Characteristic	Requirement	Test procedure	Inspection level	AQL
Connecting tube	Pressure	3.4	4.4.1	S-1	*

*Acceptance number shall be zero. A minimum of three samples shall be taken regardless of lot size.

4.3 Examination. The connectors shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects*

Major	
101	Connector not free of sharp edges.
102	Connector not free of protrusions.
103	Surface not smooth.
104	Plating does not adhere.
Minor	
201	Plating not free of scratches and bare spots.
202	Identification marking not present, complete, correct, legible, or permanent.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The connectors shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Pressure test. Two of the three arm openings of the "Y" connector shall be capped to withstand an air pressure of 20 p.s.i.g. The open end of the remaining arm shall be securely connected to a 20 p.s.i.g. air source. The connector shall indicated no air leakage when subjected to the air source and submerged in a suitable solution for detecting air leakage or show any other physical damage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One (1) tube, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table I. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be packaged in a kraft paper envelope of suitable size and design. Envelope shall be secured to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors shall be acceptable, or PPP-B-636. Closure shall be adequate to prevent spillage of contents under normal handling.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix and waterproofing shall conform to 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic (method I closure shall be utilized).

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable level of packing (see 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc. of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

NNN-C-00545(DSA-DM)

Military custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force -03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Category: C

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

FOLD UNDER

DEFENSE SUPPLY AGENCY
DEFENSE MEDICAL SUPPLY CENTER
3RD AVENUE AND 29TH STREET
BROOKLYN, N.Y., 11232

POSTAGE FEES PAID
DEFENSE SUPPLY AGENCY

OFFICIAL BUSINESS

DEFENSE SUPPLY AGENCY

DEFENSE MEDICAL SUPPLY CENTER

ATTN: DIRECTORATE OF TECHNICAL OPERATIONS (CODE TM5)

3RD AVENUE AND 29TH STREET

BROOKLYN, N.Y., 11232

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION CONNECTOR, ELASTIC TUBING, BRANCHED, METAL, MIL-C-00545(DSA-DM), DATED 18 APRIL 1952.

ORGANIZATION *(Of submitter)*

CITY AND STATE

CONTRACT NO.

QUANTITY OF ITEMS PROCURED

DOLLAR AMOUNT
$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)*

DATE

DD FORM 1426 1 APR 53

NAVSHIPS 11502

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:48Z
Check the source to verify that this is the current version before use.