INCH-POUND

A-A-53973B
16 December 1993
SUPERSEDING
A-A-53973A
16 July 1993

COMMERCIAL ITEM DESCRIPTION

BAG, BLOOD COLLECTING-DISPENSING-SYSTEM

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers sterile, pyrogen-free disposable, plastic, blood collecting component processing, and dispensing systems. Types I and II shall also provide blood freezing capability.

Salient characteristics:

The system shall consist of the following types:

Type I - Shall consist of the components interconnected as shown in Figure 1.

Type II - Shall consist of the components interconnected as indicated in Figure 2 except that commonality labels shall be attached inverted as indicated herein.

Type III - Shall consist of the components interconnected as shown in Figure 2 except primary bag capacity shall be 600 ml and standard outlet port and tubing shall not be provided. Commonality labels shall also be attached inverted as indicated herein.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Shall be a sterile, pyrogen-free, disposable, plastic, blood collecting component processing and dispensing system. The system and anticoagulant shall be in conformance with all requirements of the U. S. Food and Drug Administration (FDA).

Primary bag. The primary bag shall have an 800 ml capacity for Types I and II systems and a 600 ml capacity for Type III system, and shall contain 63 ml of CPDA-1 anticoagulant for collecting 450 ml of blood. The bag shall be fabricated of polyvinylchloride (PVC). The bag shall possess two blood outlet ports consisting of externally protruding tubes sealed and closed by an internal transverse puncturable plastic diaphragm within the tube. This diaphragm shall be readily puncturable for connecting to a standard blood recipient set, and bowl, washing and waste bag set (See Note 2).

Sterility shall be maintained by a tamperproof protective sheath. Design shall be such that the piercing end of the recipient set will make a leakproof connection prior to puncture of diaphragm and provide protection to the bag walls against piercing. The bag shall have a horizontal slot as a means of suspending for infusion approximately 1-1/4 inch (3.2 cm) long (with two circular end holes) located at the top to permit suspension in the upright position. Type I donor tube and needle shall be not less than 51 inches (129.54 cm) long and shall bear at least 10 indelibly imprinted identification numbers not more than 3-1/4 inches (8.1 cm) apart. Type II and III donor tube, sampling system and needle configuration shall not be less than 71 inches (180 cm) long and shall bear at least 15 indelibly imprinted identification numbers not more than 3-1/4 inches (8.1 cm) apart.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

The donor tubing for Type II and Type III shall contain an undiluted blood sample system 51 inches (129 cm) from the primary bag. The sample system shall be fabricated from PVC and be not less than 5-1/2 inches (14 cm) long, tubular in construction and shall hold between 32 to 34 ml of unanticoagulated blood when full.

Donor needle shall be 16 gauge, thin wall, 1.5 - 1.6 inch (3.81 - 4 cm) long. Needle shall have a sharp, smoothly expanding ground bevel between 0.203 and 0.318 inch (0.516 - 0.808 cm long).

Interior lumen connection to donor tube shall present a smoothly expanding surface to prevent platelet aggregation and clotting. Needle shall be protected by a tamperproof sheath. During removal only sterile surfaces and edges shall contact the needle cannula. Needle cannula shall be Class 3, austenitic corrosion-resisting steel in accordance with ASTM Designation F899.

Transfer packs. The transfer packs shall each have a 400 ml capacity. The first transfer pack shall be suitable for use in collecting excess glycerol.

The second and third transfer packs are to be used for fresh frozen plasma and 5-7 day platelet concentration, one of which must be PVC or polyolefin (including connecting tubing).

All transfer packs must possess two standard outlet ports consisting of externally protruding tubes sealed and closed by an internal transverse puncturable plastic diaphragm within the tube. The diaphragm shall be maintained by a tamperproof sheath. Design shall be such that the piercing end of the recipient set will make a leakproof connection prior to puncture of diaphragm and provide protection to the bag walls against piercing. Packs shall have a horizontal slot, located at the top, as a means of suspending for infusion, approximately 1-1/4 inch (3.2 cm) long with two

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

circular end holes to permit suspension in the upright position.

Outlet port. The standard outlet port shall be provided in Types I and II only and shall be suitable for adding 40% glycerol, rejuvenating solutions and other additions. Shall be of the same type port described under primary bag. Sterility shall be maintained by a tamperproof sheath or cap. Shall allow complete acceptance of the stylet end of a transfer set.

Tubing. Tubing from "Y" connector to transfer pack and donor tubing shall bear indelibly imprinted identification numbers with center-to-center distance being at least 2-7/8 inches (7.2 cm) and not more than 3-1/4 inches (8.1 cm) long. At least 6 numbers shall be provided on the first transfer pack connecting tubing. At least 4 numbers shall be provided on each leg of the second and third transfer pack tubing. Tubing shall have an outer diameter of 0.158 ± 0.003 inch with wall thickness of 0.020 ± 0.002 inch.

Centrifugation. The primary bag and transfer packs shall be shaped to permit centrifugation in the 1000 ml standard trunnion cup of the centrifuge indicated in Note 3. Internal dimensions of the primary bag for Types I and II shall be not less than 8 inches (20 cm) long and 4-3/4 inches (11.8 cm) wide nor more than 9 inches (22.5 cm) long and 5-1/4 inches (13.1 cm) wide. Internal dimensions for the Type III 600 ml primary bag shall not be less than 6-1/2 inches (16.5 cm) long and 4-3/4 inches (12 cm) wide nor more than 7-1/2 inches (19 cm) long and 5-1/4 inches (13.1 cm) wide.

Commonality label. The primary bag and transfer packs shall bear a single label that is printed according to the latest FDA Guidelines for Uniform Labeling. This is referred to as the "Commonality Label" and shall be in conformance with the Food and Drug Administration requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

This label shall be permanently sealed to the bag. For the Type II and III bags the commonality label top shall be adjacent the hanging slot of the bag 3/4 to 1-1/4 inches from the bag fluid seal for the primary bag and in the center of the transfer pack with the label top adjacent the hanging slot.

Additional markings to this label shall include manufacturer's name and lot number. The bag shall be made of such material so that applied labels and writing shall remain adhered throughout the usage time (up to 20 years).

The system internal surfaces shall be pyrogen-free, non-toxic and sterile when tested in accordance with the United States Pharmacopeia (USP) of AAMI guidelines. Material of tubing and bags shall be compatible with the blood or blood component stored herein. The sterility assurance level for the system shall be $1x10^{-6}$ in accordance with AAMI guidelines. The system shall meet Class IV biological tests when tested in accordance with the USP.

Workmanship. The system shall be free from defects which detract from its appearance or impair its serviceability. The system components shall be free from cuts, tears, weak points, discoloration or flash.

Unit. Package (PG). One package (sealed foil pouch) containing 4 blood collecting-dispensing-freezing systems, as specified, constitutes one unit. As an alternate, two sealed foil pouches, each containing 2 blood collecting-dispensing-freezing systems, as specified, shall be overwrapped to constitute one unit. The internal surfaces of the package and the external surfaces of the blood bag system shall be clean and free from fungus or other foreign material. The sealed foil pouch shall be free from fungus or other foreign material. The sealed foil pouch shall be free from tears, holes, and cuts, shall completely seal the contents providing protection from foreign material, and shall be capable of maintaining sterility of contents unless package is damaged or opened.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one blood collecting system. Sampling shall be inspection level S-2 with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one blood collecting system. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations.

Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers (NSN) and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6515-01-234-6831	BAG, BLOOD COLLECTING-DISPENSING-FREEZING, 800 ml with 63 ml CPDA-1 Anticoagulant, Quadruple Pack, Disposable, 4's	I
6515-01-372-3416	BAG, BLOOD COLLECTING-DISPENSING-FREEZING, 800 ml with 63 ml CPDA-1 Anticoagulant, Quadruple Pack, with 5-7 day Platelet Pack, Disposable, 4's, with inverted labels	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

6515-01-372-3417	BAG, BLOOD COLLECTING-DISPENSING Inverted Label, 600 ml with 63 ml CPDA-1 Anticoagulant, Quadruple Pack, with 5-7 day Platelet Pack, Disposable, 4's, with inverted labels	III

NOTE 2: The Blood Collecting-Dispensing-Systems covered by this specification shall be used with an Indirect Transfusion Blood Recipient Set (NSN: 6515-01-128-1407), and a Washing and Waste Bag Set Bowl (NSN: 6640-01-234-9582)(Type I and II only).

NOTE 3: The Blood Collecting-Dispensing-Systems covered by this specification shall be used with a Laboratory Centrifuge (NSN: 6640-01-139-7457), which is equal to Dupont Model RC-3B.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5681
Location: Intergraph/bag

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

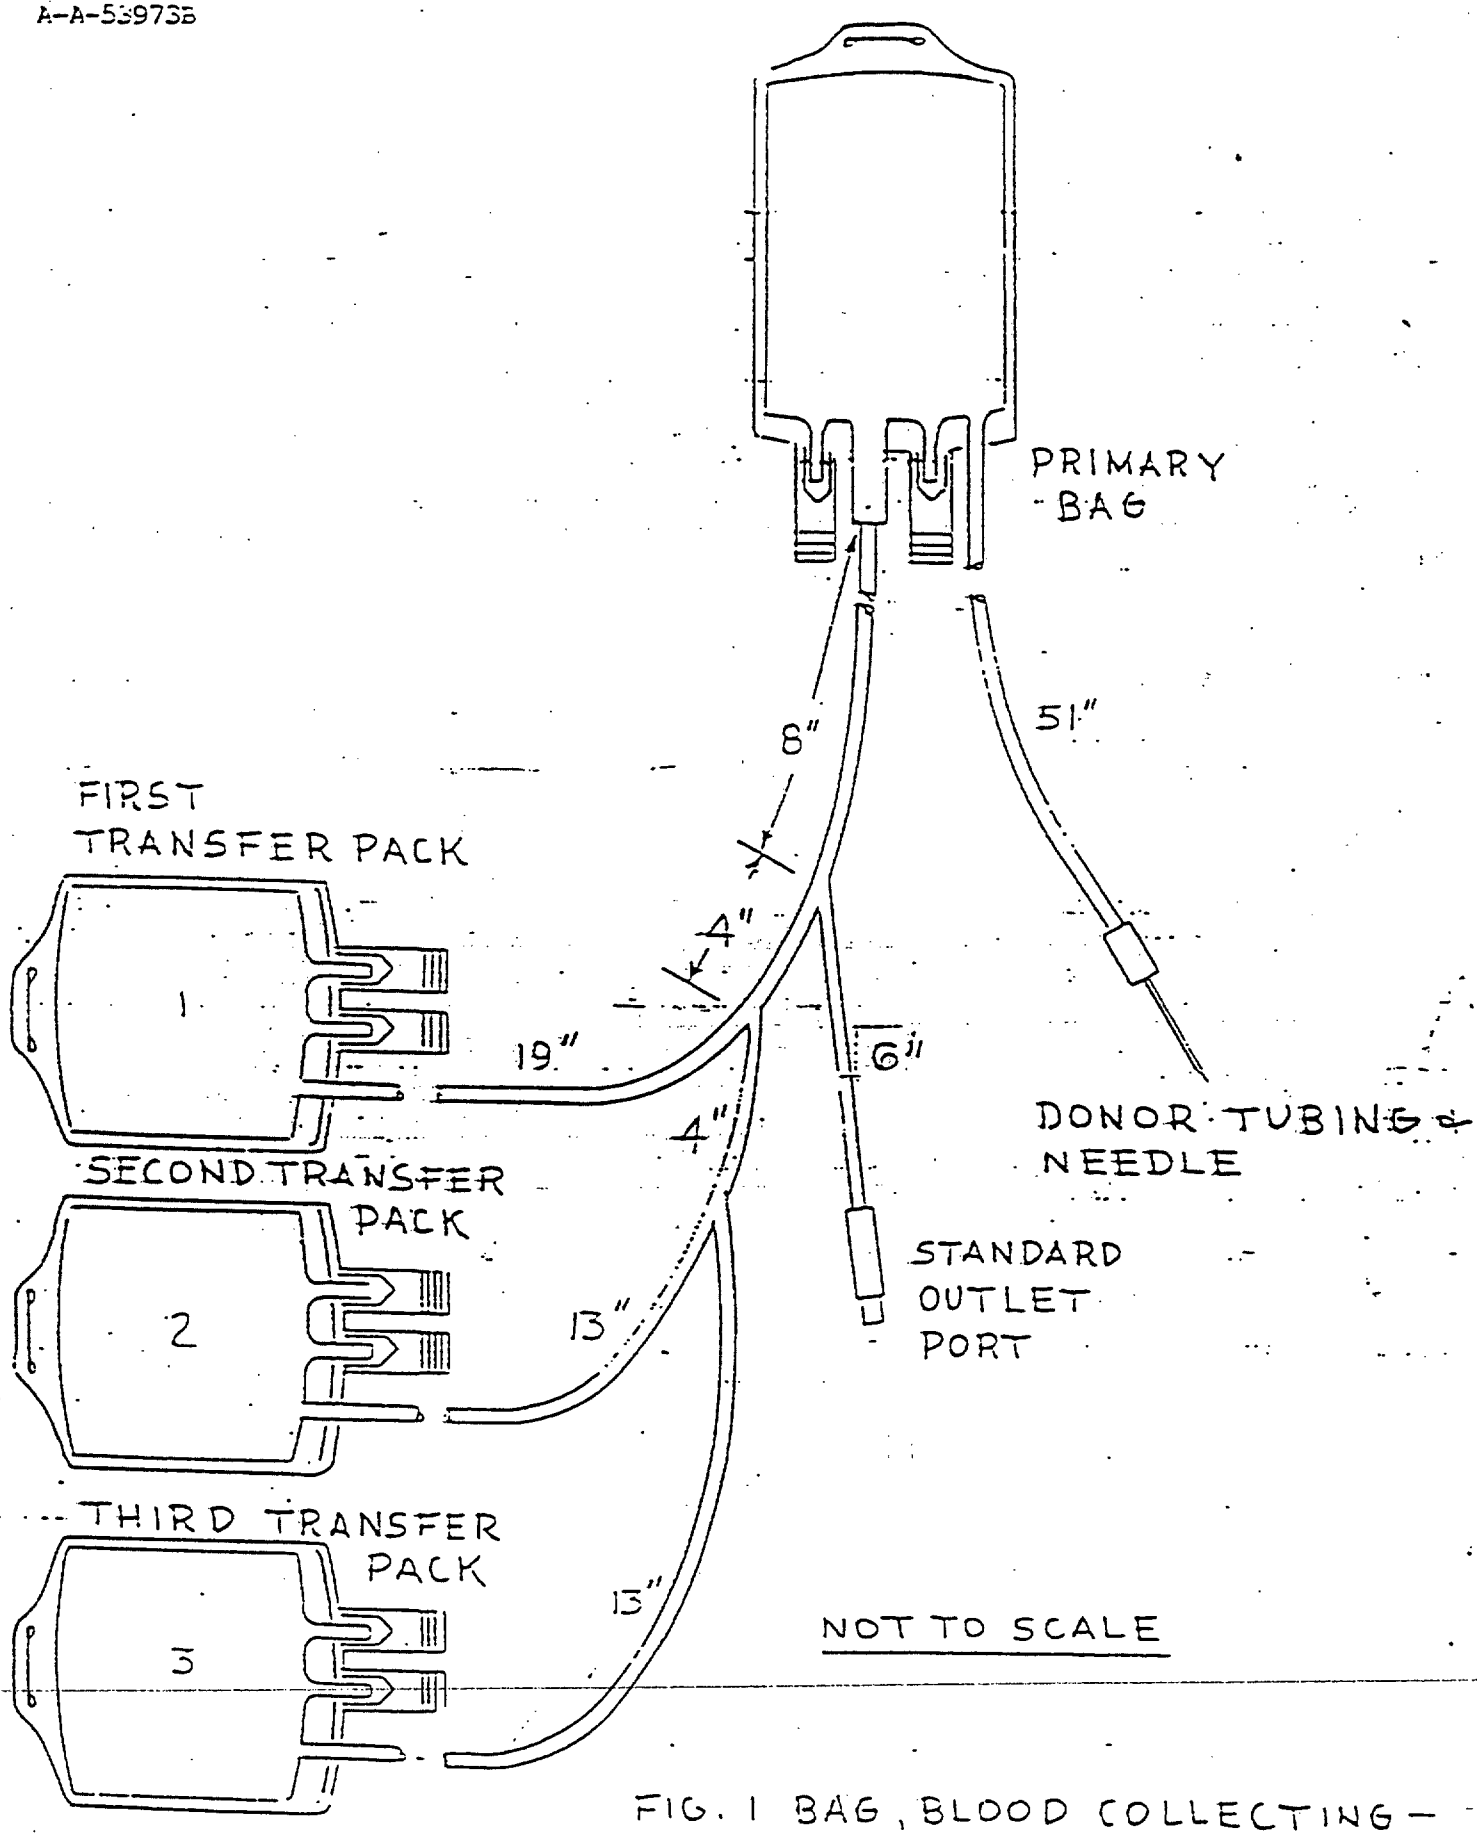


FIG. 1 BAG, BLOOD COLLECTING - DISPENSING, FREEZING

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

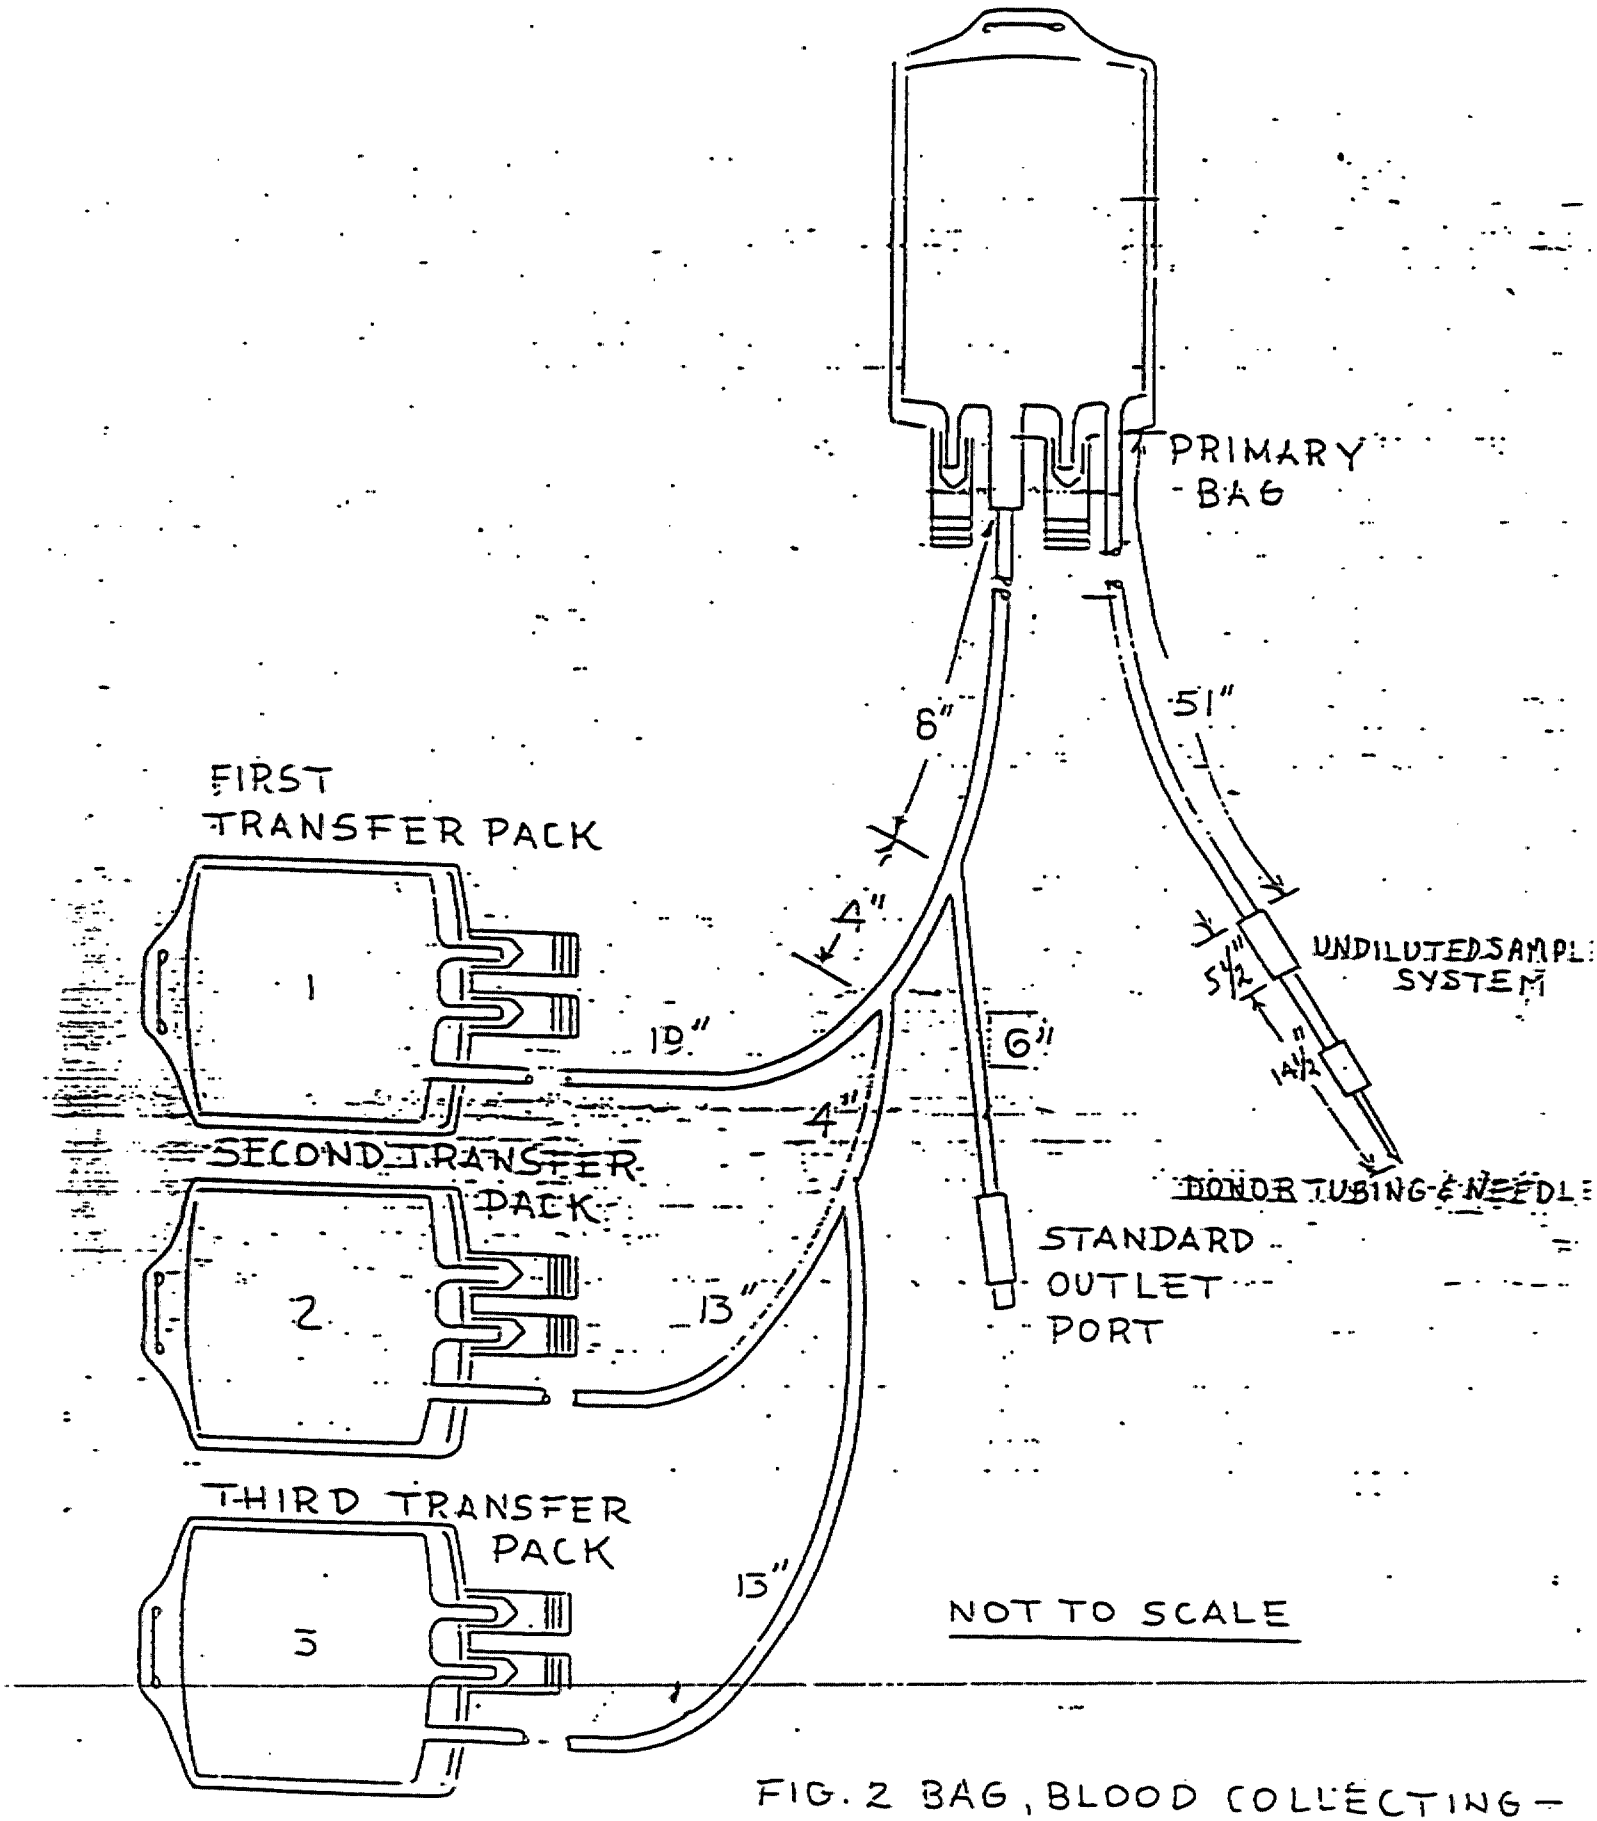


FIG. 2 BAG, BLOOD COLLECTING-DISPENSING (FREEZING, TYPE II ONLY)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:27Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-53973B	931216

3. DOCUMENT TITLE
BAG, BLOOD COLLECTING-DISPENSING-SYSTEM

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial (215) 7372870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil - Downloaded: 2025-11-26T21:27Z
Check the source to verify that this is the current version before use.