SS-P-446D
May 27, 1975
SUPERSEDING
Int. Fed. Spec.
SS-P-00446C (DSA-DM)
August 21, 1973 and
Fed. Spec. SS-P-446a
August 27, 1957

FEDERAL SPECIFICATION

PLASTER, DENTAL, IMPRESSION AND MODELING

This specification was approved by the Commissioner, Federal Supply Services, General Services Administration, for use of all Federal Agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers plaster of paris suitable for taking dental impressions and making dental models.

1.2 Classification.

1.2.1 Types and Sizes. Plaster of paris shall be of the following types and sizes, as specified (see 6.1):

Type I	Dental impression
	Size 1. 2-1/2 pounds
Type II	Dental modeling
	Size 1. 35 pounds
	Size 2. 4 pounds

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

FEDERAL SPECIFICATIONS:

RR-S-366	Sieve, Test.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Shipping Fiberboard.
PPP-C-96	Can, Metal, 28 Gage and Lighter.
PPP-P-704	Pail, Metal (Shipping, Steel 1 through 12 gallon).

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

FEDERAL STANDARD:

Fed. Std. No. 123 Marking for Domestic Shipment (Civil Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal specifications required by activites outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

MILITARY SPECIFICATION:

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

MILITARY STANDARDS:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Society for Testing and Materials (ASTM) Standard:

C 472-73 Physical Testing of Gypsum Plasters and Gypsum Concrete.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103).

3. REQUIREMENTS

3.1 Material. The plaster shall be composed essentially of finely powdered, high quality, hemihydrate of calcium sulfate and necessary modifiers which, when mixed in accordance with instructions, shall form a smooth, homogeneous mixture and set hard. The plaster shall be uniform in texture and free of foreign material and lumps.

3.2 Description.

3.2.1 Type I. Type I shall be an impression plaster suitable for recording in accurate detail the teeth and adjacent tissue of the oral cavity. The plaster shall set while in contact with the oral tissue. Plaster shall fracture cleanly and separate easily, so that impressions can be accurately reassembled. Plaster shall be furnished clean and shall be free of any impurities that would be irritating to the oral tissue. Plaster shall be plain and unflavored.

3.2.2 Type II. Type II shall be a modeling plaster suitable for accurately reproducing the recorded dental details of a negative impression.

3.3 Physical properties. The plaster shall conform to the physical properties shown in Table I for the applicable type specified.

TABLE I. Physical Properties

Property	Type I	Type II
Consistency, millimeters	90 ± 3 1/	30 ± 2 2/
Setting time, minutes	4 ± 1.5	10 ± 3
Setting expansion, percent	0.00 to 0.15	0.00 to 0.30
Compressive strength, minimum at 1 hour Meganewtons/square meter-MN/m^2 (pounds per square inch - psi)	2.4 (350)	8.6 (1250)
Fineness		
Passes No. 100 sieve, minimum, percent	98	98
Passes No. 200 sieve, minimum, percent	90	90

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:13Z
Check the source to verify that this is the currentversion before use.

1/ Slump method

2/ Cone penetration method

3.4 Color. The color of the plaster shall be white.

3.5 Net weight. The plaster shall be furnished in the weights specified in Table II, when tested as specified in 4.4.9.

TABLE II. Net Weight of Plaster

Pounds (Minimum)	
Type I Size 1. 2-1/2 pounds	Type II Size 1. 35 pounds Size 2. 4 pounds

3.6 Reproduction of detail. The plaster shall reproduce a groove 0.050 millimeters (mm) in width, when tested as specified in 4.4.8.

3.7 Stability. The plaster shall comply with all the requirements of this specification for not less than two years from date of manufacture, when stored at controlled room temperature of 59° to 86° Fahrenheit (F.).

3.8 Delivery schedule. Not more than 3 months shall have elapsed from the date of manufacture of the plaster to the date of delivery to the Government.

3.9 Instructions. Adequate and accurate instructions for proportioning and manipulating the plaster shall accompany each unit. Information shall include the powder to water ratio (in terms of cubic centimeters (cc) water/100 grams (g) of powder), setting expansion and setting time. A statement that heavy ingredients settle to the bottom, and that for consistently accurate casts, plaster should be mixed thoroughly before dispensing. In addition, two copies of the instructions shall be forwarded to the contracting officer for information purposes.

3.10 Workmanship. Workmanship shall be first class throughout. The plaster shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:13Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided that lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in Tables III and V (see 4.2.1 and 4.3) and Table IV (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in Table III. Unit of product for examination purposes shall be the unit of issue.

TABLE III. Sampling for Examination

Type Defect	Inspection Level	AQL (Percent Defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:13Z
Check the source to verify that this is the current version before use.

4.2.2 Sampling for tests. Sampling for tests shall be conducted on each lot or control number in accordance with Table IV. If any test determination for a lot does not comply with the requirements specified, the lot shall be rejected.

TABLE IV. Tests

Characterisitc	Requirement	Test procedure	Number of determinations per lot or batch number
Consistency	3.3	4.4.3	3 1/
Setting time	3.3	4.4.4	5 1/
Setting expansion	3.3	4.4.5	2 1/
Compressive strength	3.3	4.4.6	5 2/
Fineness	3.3	4.4.7	2 1/
Net weight	3.5	4.4.9	3 3/
Reproduction of detail	3.6	4.4.8	2

1/ Each determination shall be the average of two specimens.
2/ Each determination shall be the average of five specimens.
3/ In process testing may be used for this characteristic.

4.2.3 Sample unit usage. Where feasible, the same unit of product shall be used for the determination of two or more test characteristics.

4.3 Examination. The plaster shall be examined to determine compliance with the requirements of this specification. Examination shall be conducted in accordance with the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in Table V.

TABLE V. Classification of defects

Categories	Defects
Major:	
101 1/	Plaster not free from foreign matter, dirt, or impurities.
102 1/	Plaster not free from caked or set lumps.
103 1/	Instructions for use inadequate, incomplete, inaccurate, or missing altogether.
Minor:	
201 1/	Plaster not uniformly white in color throughout.
202	Packaging not as specified.
203	Packing not as specified.
204	Marking incorrect, incomplete, illegible, or omitted.

1/ In process examination may be used in examination for these defects.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

4.4 Tests.

4.4.1 Test conditions. The preparation of test specimens and test procedures shall be conducted at a room temperature of 23.0° ± 2.0° Centigrade (C.) and a relative humidity of 50% ± 10%. Equipment and material shall be conditioned at this temperature and humidity at least ten hours prior to testing.

4.4.2 Mixing procedure. Before the plaster sample is weighed, the dry material shall be thoroughly remixed by completely stirring or by rolling the container end over end, if there is sufficient air space in the container to permit the material to move freely. The plaster used in making all test specimens shall be mixed with sufficient distilled water at 23.0° ± 2.0°C. to produce a mix of testing consistency. The testing consistency is defined as the water to powder ratio that gives a slump pat diameter or cone penetration depth meeting the requirements of 3.3. The standard mix for testing consistency shall be made by adding the dry powder to the correct amount of water in a 10 to 13 centimeters (cm) diameter rubber or plastic mixing bowl. The mixture shall be allowed to soak for 30 seconds and then stirred for one minute to a smooth consistency with a round-ended, stiff-bladed spatula at the rate of 120 revolutions per minute (rpm). The spatula shall have a blade approximately 1.9 to 2.5 cm wide and 9 to 13 cm long.

4.4.3 Testing consistency.

4.4.3.1 Testing consistency for type I plaster by slump method. The dry plaster (100 g) shall be added to the test quantity of gauging liquid (4% sodium citrate in distilled water, used only for consistency determinations) and shall be mixed as described in 4.4.2. The time of initial contact of powder with the gauging liquid shall be considered the start of the mix. A cylindrical mold, 50.0 mm long with an internal diameter of 35.0 mm , shall be placed on a clean dry glass plate and shall be filled immediately after spatulation of the mix and struck level. Two minutes from the time of starting the mix, the mold shall be lifted slowly and the mixture allowed to slump or spread over the glass plate on a vibration-free bench. One minute after the mold is lifted, the major and minor diameters of the slumped mixture shall be determined to the nearest millimeter. The average of three tests (six diameters) shall be taken as a measure of consistency. The water powder ratio which gives the consistency required in Table I shall be used for specification testing. Distilled water shall be used in the preparation of all specimens for the determination of setting time, setting expansion and compressive strength. Care shall be exercised to avoid contamination of testing equipment with the sodium citrate solution.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

4.4.3.2 Testing consistency for type II plaster by cone penetration method.

4.4.3.2.1 Modified Vicat apparatus. The modified Vicat apparatus (ASTM-C472-73) shall consist of a bracket bearing a movable metal rod 6.3 mm in diameter and of suitable length to fit the Vicat bracket. On the lower end of the rod, there shall be attached a metal conical plunger having an apex angle of $53^{\circ}08'$, a height of 45 mm and a base diameter of 45 mm. The rod shall bear a mark or be equipped with a pointer to indicate movement of the rod in relation to the scale graduated in millimeters and attached to the bracket. The total weight of the rod-cone assembly shall be 0.34 newton (N) (35 g) for testing type II plaster. The rod shall be held in a vertical position by a screw. The conical ring mold shall be made of a noncorroding, nonabsorbent material, and shall have an inside diameter of 6 cm at the base and 7 cm at the top and a height of 4 cm. The baseplate for supporting the ring mold shall be plate glass and about 10 cm square.

4.4.3.2.2 Procedure. The following test procedure shall be used: Clean the plunger, mold and baseplate of the modified Vicat apparatus. Apply a thin coat of petroleum jelly or other suitable lubricant to the upper surface of the baseplate in order to prevent leaks during the test. The dry plaster (300 g) shall be added to the test quantity of gauging liquid (4% sodium citrate in distilled water, used only for consistency determinations) and shall be mixed as described in 4.4.2. Pour this mixture into the ring mold (large end up), work slightly to remove air bubbles, and then strike off flush with the top of the mold. Wipe the conical plunger clean with a moist cloth before each determination (leave moist), and lower it to the surface of the sample. The cone shall not strike the ring mold when released. Read the scale and release the plunger quickly. After the plunger has settled, read the scale again. The difference in scale readings is millimeters of penetration. Determinations are to be made at seven, eight, and nine minutes after the start of the mix. Two penetrations are to be averaged for each determination. The average of three determinations (six penetrations) shall be taken as a measure of consistency. The water to powder ratio that gives the consistency specified in 3.3 shall be used for all specification testing for type II plaster. The release screw shall be tightened only sufficiently to hold the plunger assembly in position. Excessive force will damage the plunger support rod. The screw shall be released abruptly and completely to prevent drag on the plunger support rod and consequently low penetration readings. The mold shall be struck level with a spatula after each determination. Excess shaking, which promotes water separation, shall be avoided. Distilled water shall be used in the preparation of all specimens for the determination of setting time, setting expansion and compressive strength. Care shall be exercised to avoid contamination of testing equipment with the sodium citrate solution.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

4.4.4 Setting time. The setting time shall be determined by a standard Vicat apparatus (ASTM C472-73). This shall consist of a frame bearing a 2.94N (300 g) movable rod. One end of the rod shall be 1 cm in diameter for a distance of 5 cm ; the other end shall have a removable needle 1 mm in diameter and 5 cm in length. The rod shall be reversible and it shall be held in any desired position by a screw, and shall have an adjustable indicator that moves over a scale (graduated in millimeters) attached to the frame. The sample to be tested is held in a rigid cylindrical mold that rests on a glass plate. The mold shall be made of non-corroding, nonabsorbent material and shall have an inside diameter of 2.5 cm and shall be 2.5 cm high. In addition, the Vicat apparatus shall conform to the following requirements: weight of plunger shall be 300 ± 0.5 g ; diameter of needle shall be 1 ± 0.05 mm. A standard mix shall be made with use of 200 g of powder and the required amount of water. On completion, the mixed mass shall be transferred immediately to the cylindrical mold. The mold shall be completely filled and shall be struck level. The setting time shall be determined by bringing the tip of the 1 mm needle into contact with the surface of the test material and locking it in position with the thumb screw. The needle shall be released and allowed to penetrate the sample at 15-second intervals, beginning one to two minutes prior to the anticipated setting time (usually at the loss of gloss or excess water). After each penetration, the needle shall be wiped clean and the mold shall be moved to permit the next penetration to be in a new area. The total elapsed time from the start of the mix to when the needle first fails to penetrate the sample completely, shall be taken as the Vicat setting time. The average value for two tests shall be reported to the nearest 0.25 minute.

4.4.5 Setting expansion. The change in length on setting shall be determined by observation of the movement of ruled markers placed approximately 30 cm. apart on a specimen in a 90° V-shaped trough. These observations shall be made with a micrometer microscope comparator or by the use of equipment of equal accuracy. The V-shaped trough, into which the specimen is poured, shall be lined with rubber dam. The initial reading shall be made one minute before the time of setting as determined in 4.4.4. The final reading shall be made two hours after the start of mix. A standard mix composed of 300 g of the powder and the proper amount of water shall be made and shall be placed in the prepared trough. The entire mix shall be used and the overall length of the poured mass shall not exceed 36 cm The average of two tests shall be reported to the nearest 0.01%.

4.4.6 Compressive strength. Compressive strength shall be determined on five cylindrical specimens, 20 mm in diameter and 40 mm high. Split molds shall be used to form the specimens. The prepared mix shall be poured or spatulated down the side of the inclined mold that is retained on a glass plate. The molds shall be vibrated gently while being filled. The overfilled molds shall be covered with a second glass plate that shall be rocked into place and that shall be pressed firmly into contact with the top surface of the mold. The specimens shall be removed from the split molds at one-half hour from the start of the mix and shall be stored in air at 23.0 ± 2.0° C. and 100% relative humidity until they are crushed at one hour after the start of the mix. The specimens shall be crushed at a loading rate of 980 ± 200 N /minute (100 ± 20 kilograms per minute (kg /min)). Values for the five specimens shall be averaged. Values that depart from the average by more than 15% shall be discarded and the remaining values shall be averaged. If less than three values remain to be averaged, the test shall be repeated.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:13Z
Check the source to verify that this is the current version before use.

4.4.7 Fineness. Fineness shall be determined by an alcohol wash method of sieving. The sieves shall conform to RR-S-366. A 10.00 g sample shall be placed on each 100 and 200 mesh sieve (Figure 1) and shall be washed with denatured alcohol at a pressure of 0.021 MN/m^2 (3 psi). The sieves of 2 inches in diameter are recommended. The assembly is connected to a container, such as a pressure cooker, that will hold at least 6 quarts of denatured alcohol. Air pressure is provided from any source and is reduced with a regulator to 0.103 $\pm$ 0.014 MN $/m^2$ (15 $\pm$ 2 p s i) and then to 0.021 $\pm$ 0.002 MN $/m^2$ (3 $\pm$ 0.3 p s i) by the assembly control. The sieve is held by hand and is rotated under the multiple stream from the nozzle. The sieve is also raised and lowered slightly while it is being rotated to insure that liquid hits the sides and all parts of the screen. A 2- to 3-liter beaker is used to catch the alcohol. If the nature of the sample causes clogging of the sieve, the powder shall be partially washed through with a stream of alcohol from a wash bottle. This removes some of the fines and wets the rest so pressure sieving may be carried out as usual. After sieving has been carried out under pressure for 60 seconds, the sieve and the bottom of the sieve are wiped with a clean cloth or cleansing tissue. The sieve shall be transferred to a dryer at 90° $\pm$ 5°C. and dried for 20 minutes. When dry and cool, the sieve and the residue shall be weighed and the amount of residue shall be determined by subtracting the weight of the sieve. The average values for two tests shall be reported to the nearest 0.1%.

4.4.8 Reproduction of detail. A ring 15 mm high and with a 30 mm inside diameter shall be placed on the test block shown in Figure 2 so that the intersection of a crossline and a groove 0.050 mm wide is in the center of the ring. As an alternate, a ring of the type specified above shall be positioned on a stainless steel test block similar to that shown in Figure 3 so that the three lines of the test block are centered on the ring. The prepared mix shall be poured or spatulated into the ring while the block and ring are being vibrated. The ring and the plaster shall be separated from the test block at one-half hour and shall be examined under low-angle illumination. The reproduction of the 0.050 mm line shall be considered satisfactory if it is continuous for the full width of the ring when viewed under ten power (10X) magnification.


4.4.9 Net weight. The net weight of the plaster shall be determined using a balance or scale suitable for the purpose intended.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified. (see 6.1).

5.1.1 Unit of issue. One can containing 35 pounds of type II, size 1 or 4 pounds of type II, size 2 or 2-1/2 pounds of type I, size 1 material, as specified, constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:13Z
Check the source to verify that this is the currentversion before use.

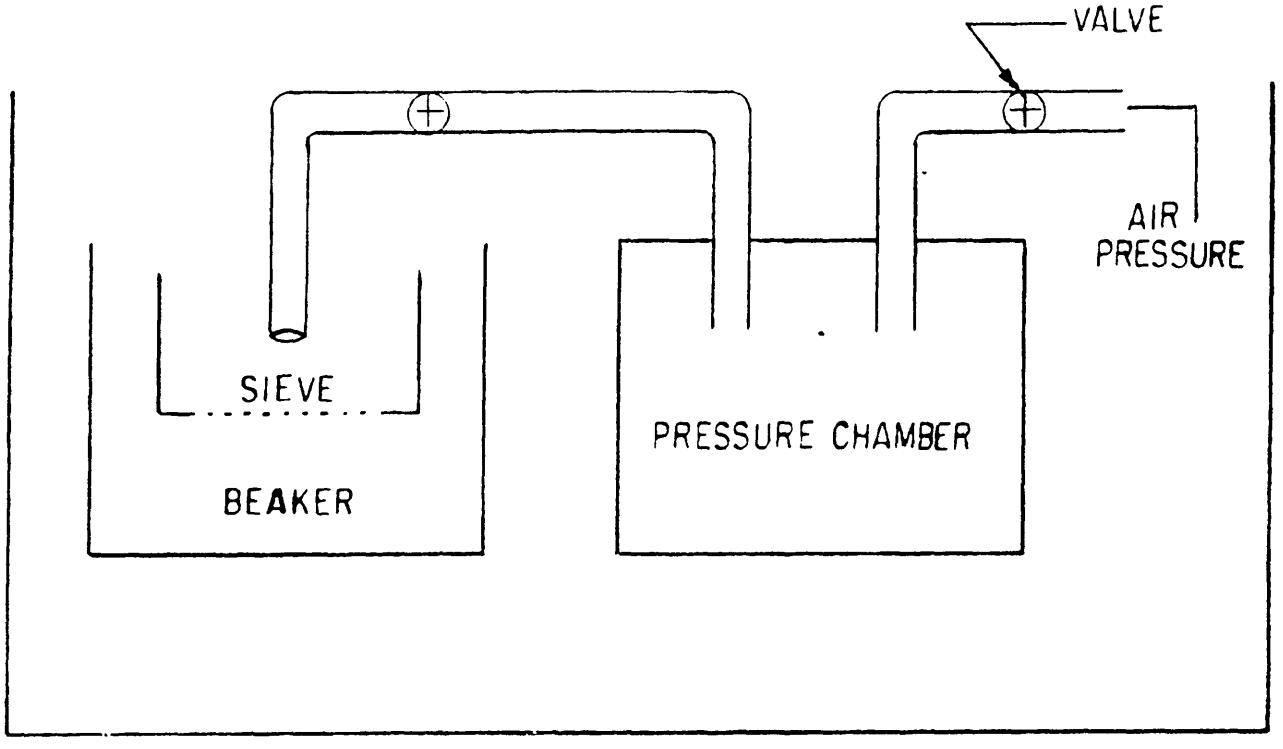

WET SIEVING APPARATUS

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.



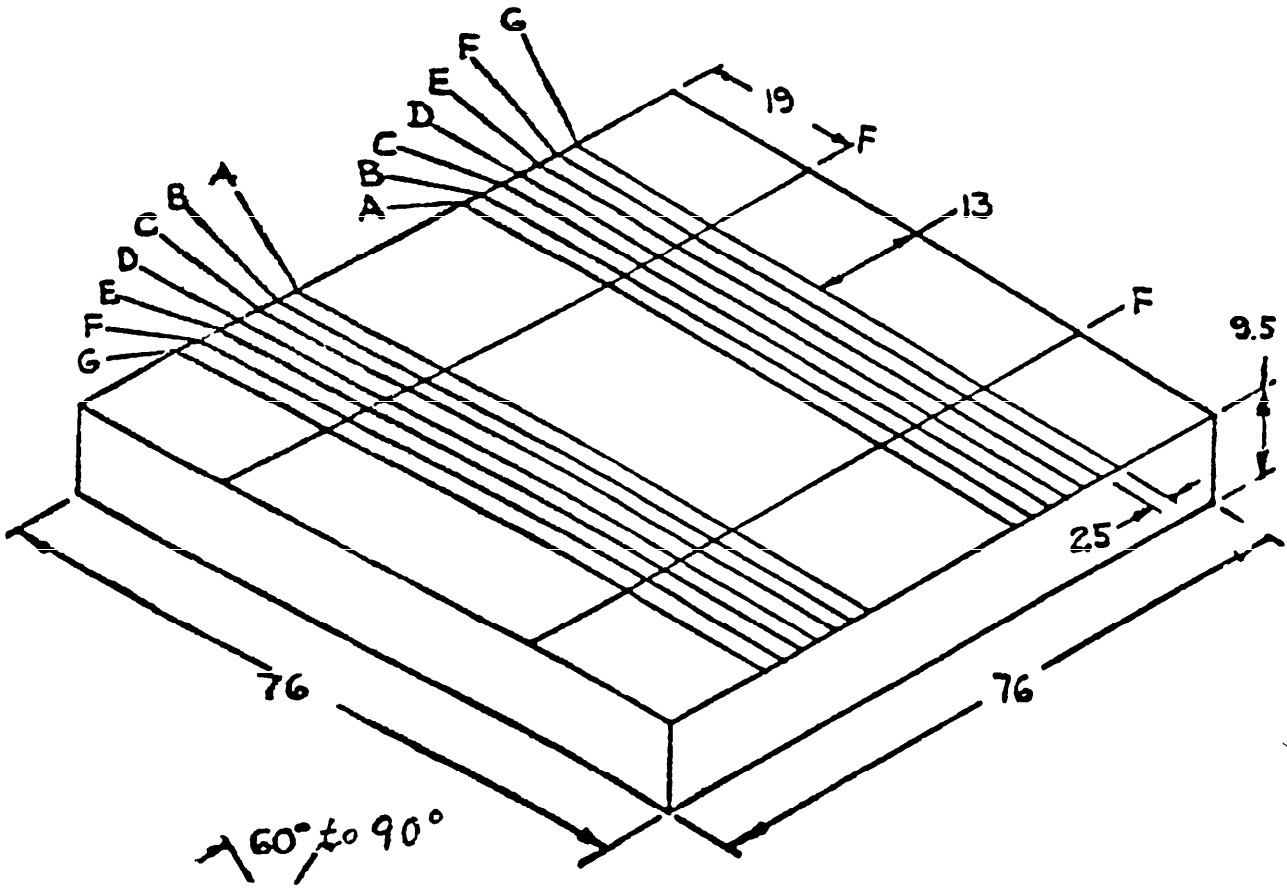


Figure 2 Test Block for Detail Reproduction

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

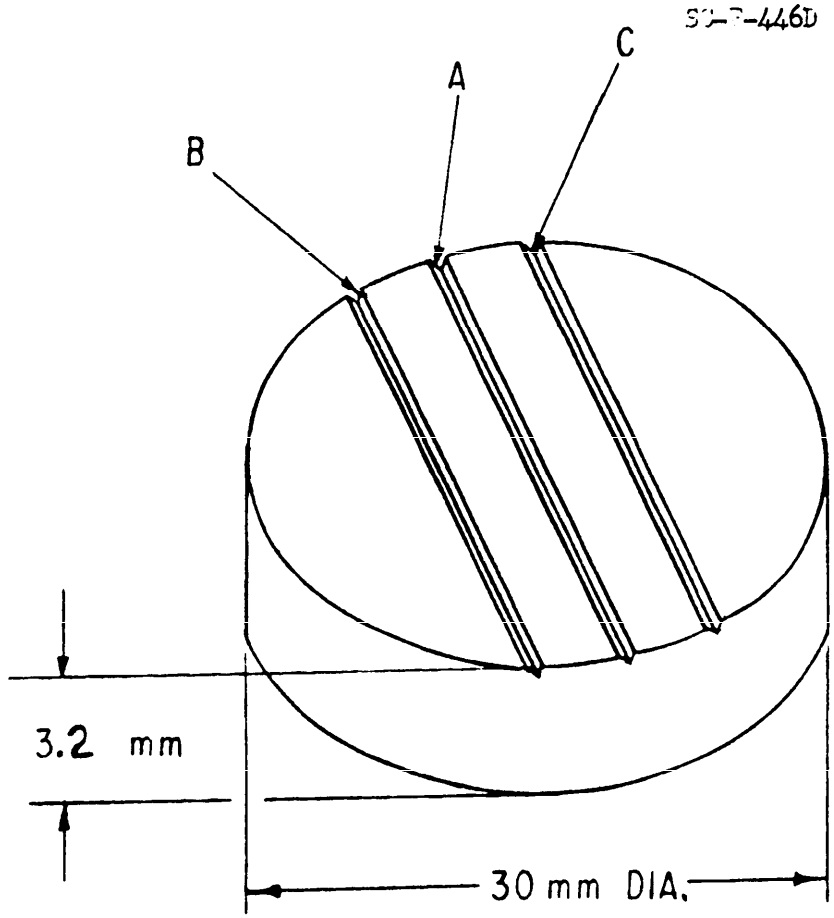

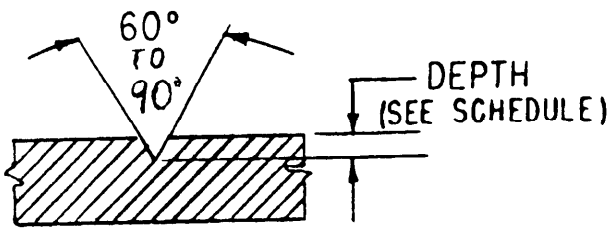

CROSS SECTION OF RULED LINES

DEPTH OF RULED LINES:
LINE "A" – 0.025 mm
LINE "B" – 0.050 mm
LINE "C" – 0.075 mm

FIGURE 3

ALTERNATE TEST BLOCK FOR DETAIL REPRODUCTION

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

5.1.2 Level A.

5.1.2.1 Type II, size 1. Each unit shall be packaged in a container constructed in accordance with PPP-P-704, type II, class 1. The size shall be appropriate to contain 35 pounds of plaster of paris. Each container shall be lined with a bag fabricated of polyethylene not less than 0.002 inch in thickness. Bag shall be secured by means of a cord, metal tie, or other suitable means.

5.1.2.2 Type II, size 2 and type I, size 1. Each unit shall be packaged in a hermetically sealed metal container conforming to type III of PPP-C-96. Size of can for type I, size 1 plaster shall not exceed 5-1/8 inches in diameter and 6-3/4 inches in height. Cans shall be tested for leakage as specified in PPP-C-96.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B, or C, as specified. (see 6.1).

5.2.1 Level A.

5.2.1.1 Type II, size 1. Units packaged as specified in 5.1.2.1 shall require no further overpacking.

5.2.1.2 Type II, size 2 and type I, size 1. Twelve units of one type and size shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.3 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with 30.4 of PPP-B-636.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Type II, size 1. Units packaged as specified in 5.1.2.1 shall require no further overpacking.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

5.2.2.2 Type II, size 2 and type I, size 1. Twelve units of one type and size shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2.4 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.3 Marking.

5.3.1 Civil agencies. In addition to any special marking required by the contract or order, interior packages and shipping containers shall be marked in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Contract or purchase order number, name of contractor and lot (control) number shall be shown. The date of manufacture shall be shown in lieu of the date packed. Unit containers for type 1, size 1 and type 1, size 2 shall be marked with the following statement:

"Heavy ingredients settle to bottom. For consistently accurate casts, mix thoroughly before dispensing."

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) number shall be shown. The date of manufacture shall be shown in lieu of the date packed.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type and size required (see 1.2.1).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

6.2 Specification changes. The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

6.3 National Stock Number (NSN) coverage. This specification covers the following items appearing in the Federal Supply Catalog:

Stock Number	Item Identification
6520-00-116-1440	PLASTER, DENTAL, Impression, 2-1/2 lb.
6520-00-203-7235	PLASTER, DENTAL, Modeling, 35 lb.
6520-00-687-7892	PLASTER, DENTAL, Modeling, 4 lb.

6.4 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - I

Project No. 6520-1373

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See Section 2 of this specification to obtain extra copies and other documents referenced herein. Price 40 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

SS-D-446D

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:13Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:13Z
Check the source to verify that this is the current version before use.