FEDERAL SPECIFICATION

COVER, BEDPAN, PAPER

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 **Scope.** This specification covers disposable, flushable, paper, bedpan covers.

1.2 **Classification.**

1.2.1 *Types.* Bedpan covers shall be of the following types, as specified (see 6.1):

Type I.—Bag.

Type II.—Drape.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 **Specifications and standards.** The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

UU-P-31 — Paper; General Specifications and Methods of Testing.

PPP-B-566 — Boxes, Folding, Paperboard.

PPP-B-585—Boxes; Wood, Wirebound.

PPP-B-601—Boxes, Wood, Cleated-Plywood.

PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.

PPP-B-636—Box, Fiberboard.

PPP-B-676 — Boxes, Set-Up, Paperboard.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123—Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specification:

MIL-L-10547 — Liners, Case, Waterproof.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:21Z
Check the source to verify that this is the current version before use.

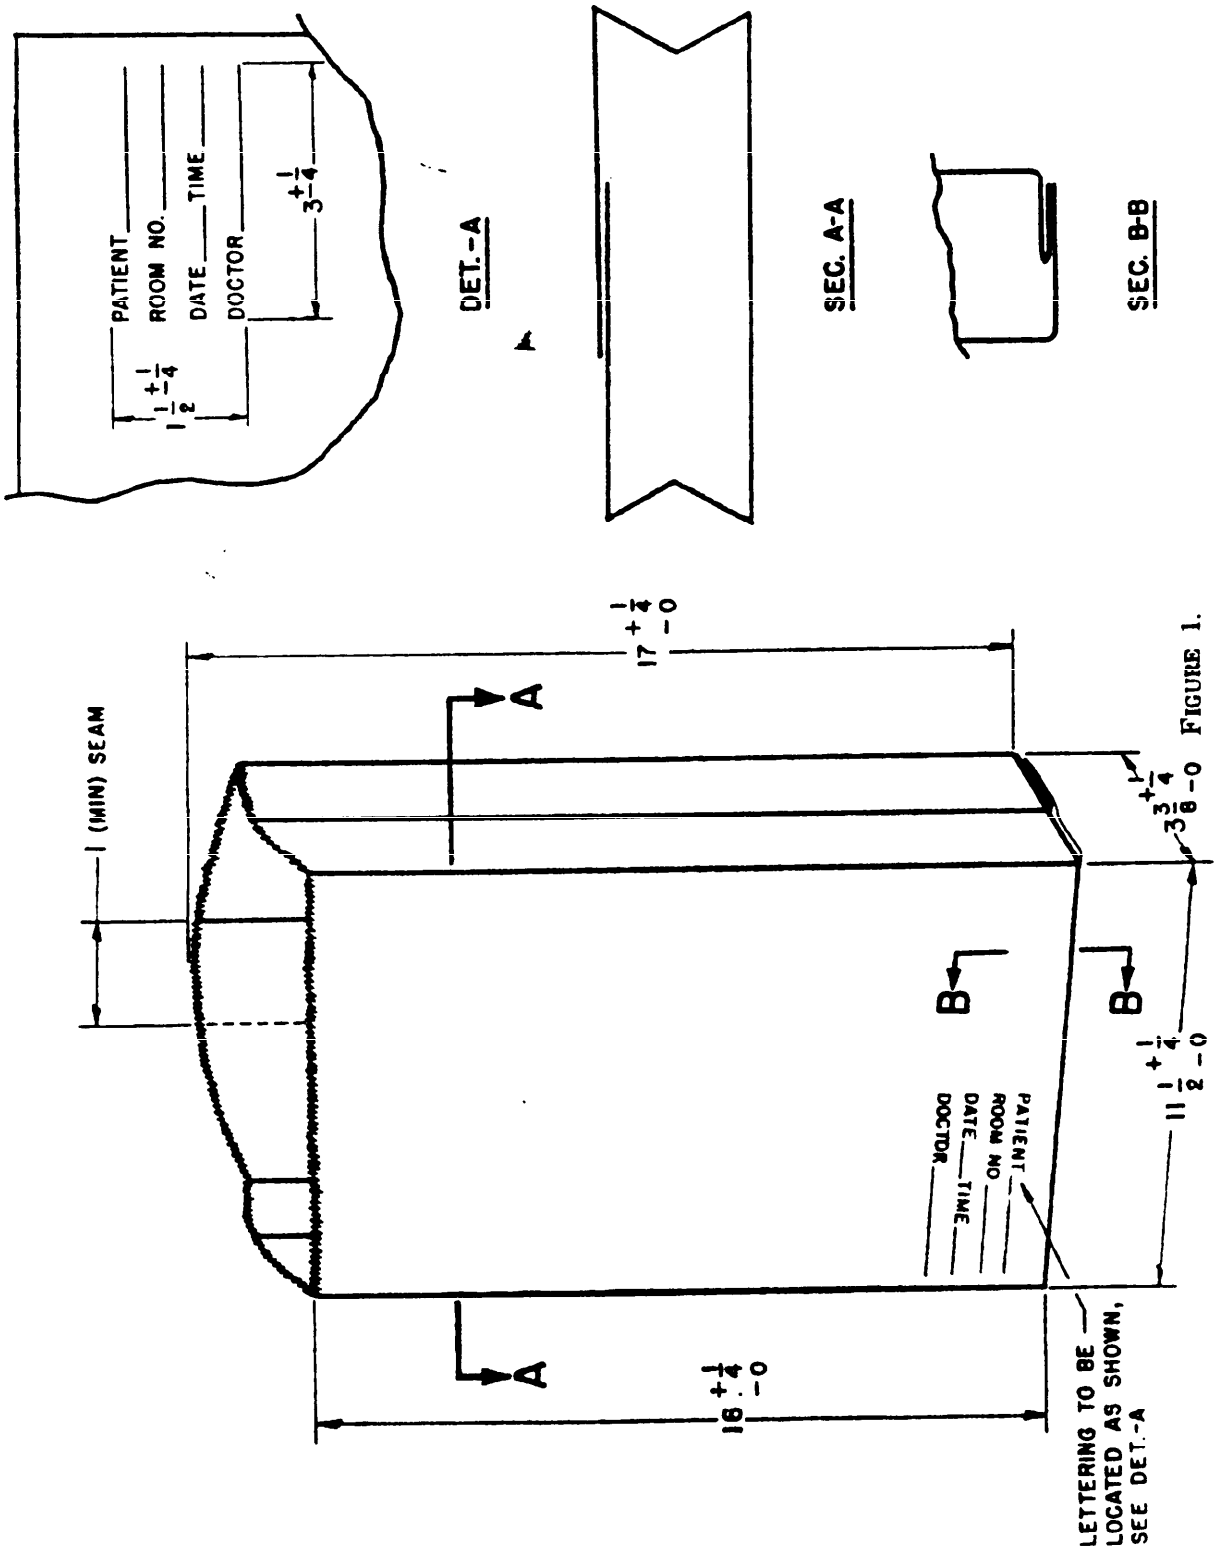


FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:21Z
Check the source to verify that this is the currentversion before use.

MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material.

3.1.1 *Type I.*

3.1.1.1 *Paper.* The paper used for fabricating the type I bedpan cover shall be unsized, soft, flexible, machine-glazed, white tissue, free of defects which may impair the serviceability of the finished item. The paper shall be free from wet-strength chemicals.

3.1.1.1.1 *Physical properties.* The paper shall conform to the following physical properties, when tested as specified in 4.4.1:

Basis weight, pounds per 480, 24 by 36 sheets	12 ± 1
Thickness, inch	0.002 ± 10 percent
Bursting strength, minimum, points	2.5
Tearing resistance, machine direction, minimum, grams	9
Tearing resistance, cross direction, minimum grams	10
Water absorptiveness, 0.01 milliliter of water, maximum, minutes	5
Brightness, minimum, percent	60

3.1.1.1.2 *Composition.* The paper shall have the following composition, when tested as specified in 4.4.1.

Bleached chemical wood fibers	50 percent minimum
Mechanical wood fibers	15 percent maximum
Unbleached chemical wood fibers	remainder

3.1.1.2 *Adhesive.* The adhesive for bonding seams of covers shall be a suitable water-soluble-type glue, and shall pass the test specified in 4.4.2.

3.1.2 *Type II.*

3.1.2.1 *Paper.* Type II cover shall be fabricated of a creped, pliable, soft, 2-ply, embossed and unembossed (surface finish) facial-type tissue, made from bleached sulphite pulp and a maximum of 30 percent ± 5 percent unbleached groundwood pulp. The paper shall have a 15 percent crepe plus 5 percent or minus 2 percent, and shall have an average rate of absorbency not to exceed 10 seconds when tested as specified in 4.4.1.1, and there shall be a minimum absorbency of 10 times its own weight. There shall be no sizing in the paper or any wet-strength treatment which may impair its instant absorbency or disintegration.

3.1.2.1.1 *Physical properties.* The paper shall conform to the following physical properties, when tested as specified in 4.4.1:

Basis weight (embossed and unembossed), pounds per 480, 24 by 36 inches	not less than 9 not more than 11
Elongation, percentage, average minimum	20

3.2 Construction.

3.2.1 *Type I.* Type I bedpan cover shall be constructed in accordance with figure 1 and this specification. Bedpan cover shall be fabricated of a single sheet of paper. The cover shall be seamed along its longitudinal center, with the edges overlapping not less than 1 inch and joined with a continuous glued line. The front face shall be folded at the bottom not less than 1 inch over the back face, and shall be glued down at three spots to form the closed end of the cover. The tuck width of the cover shall be 3⅜ inches. Bedpan cover shall be capable of being readily flushed down a conventional bedpan washer-sterilizer.

3.2.1.1 *Name panel.* Each type I cover shall have a name panel printed on the front located as indicated on figure 1. The panel shall consist of the following information:

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:21Z
Check the source to verify that this is the current version before use.

Patient _____
Room No. _____
Date _____ Time _____
Doctor _____

3.2.2 *Type II.* Type II cover shall be of a 2-ply facial-type tissue (see 3.1.2.1), rectangular in shape, and embossed to prevent separation of the paper. The embossing pattern shall be of a design so spaced that not less than two impressions nor more than four impressions shall cover a square inch. The finished cover shall be even on all sides with no overlapping edges. When placed over the bedpan, the cover shall immediately drape to follow the contours of the sides with the four edges of the cover hanging perpendicular to the floor. The cover shall measure 24 by 24 inches, ± ¼ inch. Each finished cover shall be folded prior to packaging so that it shall be 24 inches long, ± ¼ inch, and 12½ inches wide, ± ¼ inch. Bedpan cover shall be capable of being flushed down the drain.

3.2.2.1 *Dispensing carton.* Dispensing carton shall be a double-faced disposable fiberboard carton of approximate size to contain 250 covers packaged flat. When opened, the carton shall serve as a dispenser permitting the removal of one cover at a time.

3.3 Identification marking. Each type I cover shall be marked with the name or registered trademark of the manufacturer.

3.4 Workmanship. Workmanship shall be first class throughout. Finished bedpan covers shall be free from holes, dirt, tears, or other defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 *Certificates of quality.* When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performances of such testing by the contractor.

4.2 Sampling.

4.2.1 *For examination.* Sampling for examination shall be conducted in accordance with Military Standard MIL–STD–105.

	Inspection level	AQL (percent defective)
For visual examination:		
Major A defects	II	1.0
Major B defects	L3	1.0
Total A (Major A and Minor A combined) defects	II	4.0
For dimensional examination	L3	2.5

4.2.2 *For tests.* Sample size for glue test (4.4.2) shall be in accordance with inspection level L4 of Military Standard MIL–STD–105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:21Z
Check the source to verify that this is the current version before use.

The acceptance number shall be zero and not less than ten covers shall be taken for test regardless of lot size.

4.2.3 *Materials.* Sufficient samples of the paper shall be selected from each lot used in the manufacture of the covers to perform tests as required by the applicable subsidiary specifications or by tests specified in 4.4.1 and 4.4.1.1. One sample unit shall be selected from each lot. The sample unit for testing shall be the quantity necessary to perform all required tests one time each. No test result shall fall below the minimum or exceed the maximum values specified.

4.2.4 Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 **Examination.** The covers shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 *Classification of defects for type I.* Examination shall be conducted in accordance with the following classification of defects:

*Categories and defects**

Major A:

101. Cover not free of cuts, tears, and holes.
102. Longitudinal seam not continuously glued.
103. Bottom seam not glued as specified.
104. Cover not clean and not free of stains and foreign matter.

Major B:

151. Unit package and exterior container not marked as specified.
152. Packaging not as specified.

Minor A:

201. Cover not white in color.
202. Cover not permanently and legibly marked with a name panel as shown on figure 1.
203. Cover not permanently and legibly marked with name or registered trademark of the manufacturer.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 *Dimensional examination.* The covers shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 **Tests.** Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 *Paper.* Tests shall be conducted in accordance with the applicable methods of Federal Specification UU–P–31, as listed below:

Property	*Method No.*
Basis weight	110
Thickness	173
Bursting strength	112
Tearing resistance	170
Water absorptiveness	180
Brightness	111
Composition	300

4.4.1.1 *Absorbency.* The average absorbency capacity of type II covers shall be determined by taking five random samples, each approximately 2½ inches square and weighing 5 grams. Each 5-gram specimen shall be laid on a flat 4-inch square of brass screen, which has been previously weighed. The screen shall be held horizontally and about ½ inch above the surface of distilled water at 25° centigrade (C.) ± 1° C. The screen and specimen shall be lowered into the water, keeping the screen horizontal and low enough to prevent retardation and absorption but high enough to prevent disintegration of the tissue as it expands due to absorption. The time elapsed after the specimen touches the water until it is completely submerged shall be taken using a stopwatch or pendulum. The screen and specimen shall be removed from the water and shall be allowed to drain for 10 seconds while in a horizontal position. The specimen and screen shall be lowered into a suitable tared receptacle and weighed to the nearest 0.1 gram. The average weight of water retained based on the results of the five tests shall be calculated.

4.4.2 *Glue.* A 2-inch strip of the glued seam section of type I covers shall be soaked

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:21Z
Check the source to verify that this is the current version before use.

in water at room temperature for 15 minutes. The plies of paper shall separate without tearing.

5. PREPARATION FOR DELIVERY

For civil agencies only, Federal Standard No. 102 shall be referred to for definitions and applications of the various levels of packaging protection for supplies and equipment.

5.1 Packaging.

5.1.1 *Unit of issue.* Two hundred fifty covers, as specified, constitute one unit of issue.

5.1.2 *Packaging quantities.* The number of units of issue indicated in table I shall be packaged in each unit and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE I.—*Packaging quantities*

Type	*Unit package*	*Intermediate package*	*Exterior container*
I -------	1 unit	Not required	12 units
II ------	1 unit	Not required	4 units

5.1.2.1 *Packing variation permitted.* If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*

5.1.3.1.1 *Type I.* Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP–B–566 or PPP–B–676. Each carton shall be adequately secured to prevent accidental opening.

5.1.3.1.2 *Type II.* Unit package shall be as specified in 3.2.2.1

5.1.4 *Level C.* Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.* Exterior container shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; or PPP–B–621, table III.

5.2.1.2 *Case liner.* Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.* Exterior container shall be a box constructed in accordance with Federal Specification PPP–B–636, type I, class 1, and fabricated from not less than 275-pound test fiberboard.

5.2.3 *Level C.* The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:21Z
Check the source to verify that this is the current version before use.

to point of delivery called for in the contract or order.

5.3 Marking.

5.3.1 *Civil agencies.* Marking for civil agencies shall be in accordance with Federal Standard No. 123.

5.3.2 *Military agencies.*

5.3.2.1 *Unit packages.* Each unit package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2.2 *Exterior container.* Exterior container shall be marked in accordance with Military Standard MIL–STD–129.

6. NOTES

6.1 **Ordering data.** Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Type required (see 1.2).

(*c*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.3 **Transportation description.** Transportation descriptions and minimum weights applicable to this commodity are:

Rail:

Toilet seat covers, paper.
Carload minimum weight 24,000 pounds, subject to Rule 34, Uniform Freight Classification.

Motor:

Toilet seat covers, paper.
Motor volume minimum weight 24,000 pounds.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded, by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

CUSTODIANS:
Army—Army Medical Service
Navy—Bureau of Medicine and Surgery
Air Force.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:21Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:21Z
Check the source to verify that this is the current version before use.