RR–B–616a
January 31, 1955
SUPERSEDING
Int. Fed. Spec. RR–B–00616a (GSA–FSS)
July 30, 1954 and
Fed. Spec. RR–B–616 May 4, 1940

FEDERAL SPECIFICATION

# BOWLS, SPONGE; CORROSION-RESISTING STEEL

*This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.*

## 1. SCOPE AND CLASSIFICATION

**1.1 Scope.**—This specification covers sponge bowls of corrosion-resisting steel for use in medical and surgical operation.

**1.2 Classification.**

**1.2.1** *Grade, type, and sizes.*—The bowls covered by this specification shall consist of 1 grade, 1 type and 4 sizes as shown in table I.

## 2. APPLICABLE SPECIFICATIONS AND STANDARDS

**2.1** The following Specification and Standard of the issues in effect on date of invitation for bids, form a part of this specification:

*Federal Specification:*

QQ–S–766—Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.

*Military Standard:*

MIL–STD–105—Sampling Procedures and Tables For Inspection by Attributes.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.

(Copies of Military Standard required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

**2.2** Specifications and standard applicable only to individual departments are listed in section 7.

## 3. REQUIREMENTS

**3.1 Material.**

**3.1.1** *Sheet and strips.*—Sheet and strips shall be corrosion-resisting steel conforming to class 1 or class 2 of Federal Specification QQ–S–766. Commercial tolerances shall apply.

**3.2 Construction.**

**3.2.1** *Bowl construction.*—The bowl shall be of conventional shape, formed seamlessly from one single piece of corrosion-resisting steel, 20 U. S. Standard gage (0.037 inch thick), which shall not be reduced below 0.033 inch thick at any point in the finished bowl. The bowls shall have a tight, flat, double-rolled beaded edge and, unless otherwise specified, the bottom shall be rounded. (See fig. 1).

**3.2.1.1** *Design and dimensions.*—The design shall be as shown in figure 1 and dimensions shall be as shown in table I.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.

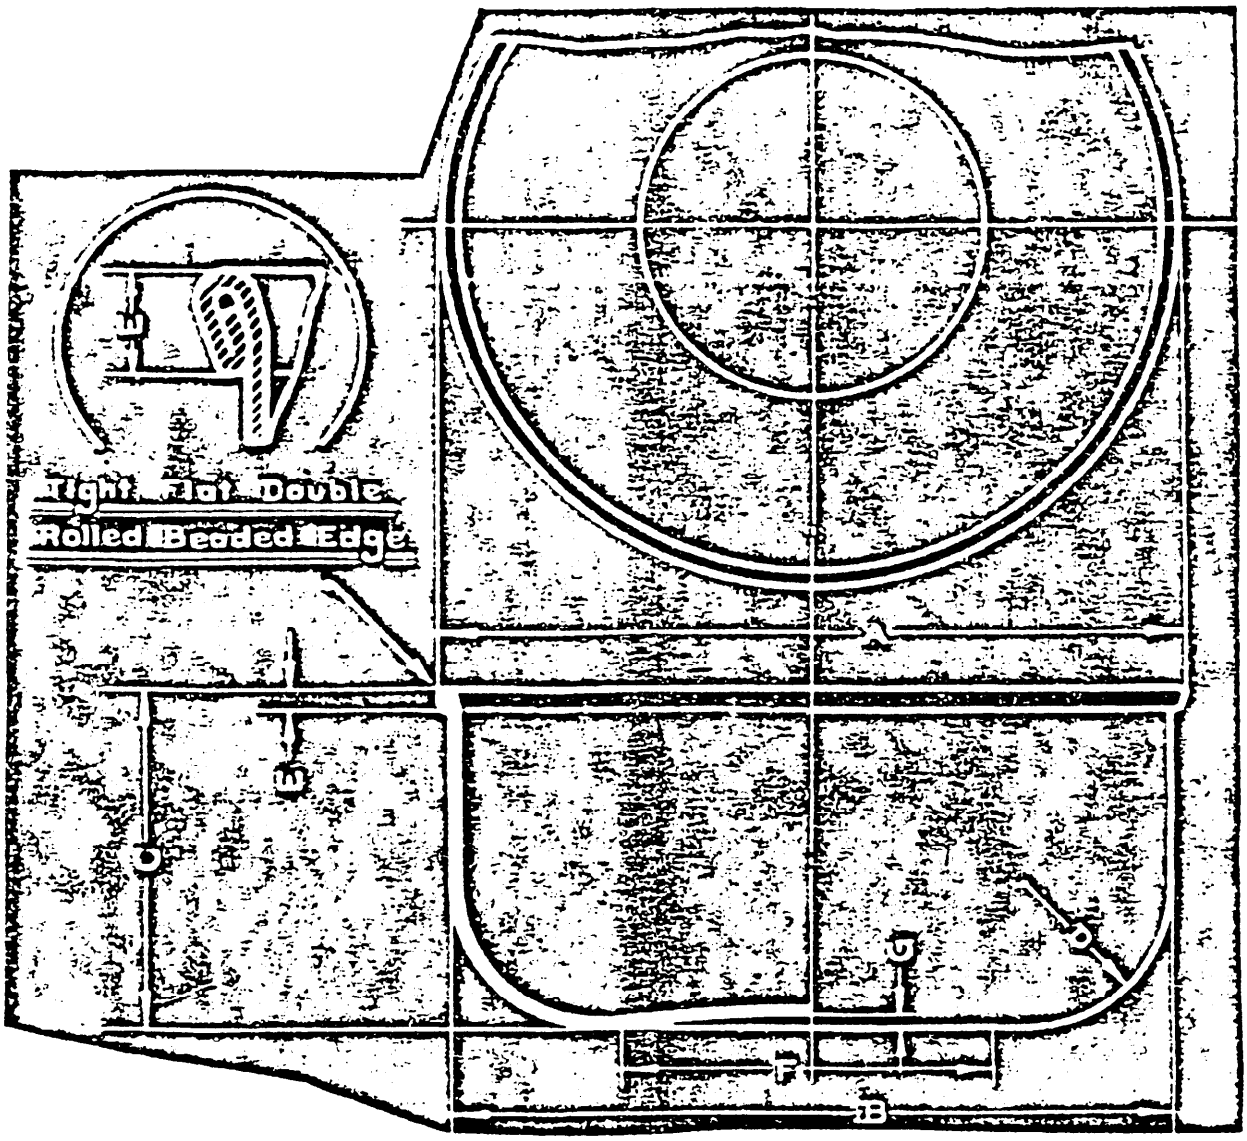



FIGURE 1.

TABLE I.—*Bowls, sponge*

| Size No. | All dimensions in inches | | | | | | | |
|---|---|---|---|---|---|---|---|---|
| | A | B | C | D | E | F | G | U. S. standard gage |
| 1 | 4½ | 4¼ | 2¼ | ⅛ | ⅛ | 2⅛ | ⅛ | 20 |
| 2 | 6¼ | 6 | 3⅛ | 1⅛ | 5/16 | 3¼ | ⅛ | 20 |
| 3 | 7¾ | 7⅛ | 3 | 1⅛ | 5/16 | 3¼ | ⅛ | 20 |
| 4 | 12 | 11¾ | 4⅛ | 1⅛ | 5/16 | 3¼ | ⅛ | 20 |

**3.3 Finish.**

**3.3.1** *Grinding.*—The entire inside and outside surfaces shall be finished with a No. 200 emery after all surface imperfections have been removed by previous grinding. This last grinding shall produce a uniform, finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet forming the bowls shall not be reduced below the thickness specified in 3.2.1 by grinding to remove surface imperfections.

**3.3.1.1** *Electropolishing.*—When specified



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.

the interior of the bowl may be finished by electropolishing. The electropolishing shall result in a uniform, bright, and shiny surface which may be easily cleaned.

3.3.2 *Cleaning.*—As a final operation, the bowls shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

**3.4 Identification marking.**—Each bowl shall be impressed with the manufacturer's name or trade-mark, and also, when specified in the invitation for bids, with such identifying letters or numbers as may be required. The identifying letters or numbers shall be placed, and conform to size, as specified in the invitation for bids. All impressions shall be made at even pressure so as not to penetrate the inside surface of the bowls.

**3.5 Tolerances.**—Unless otherwise specified, a plus or minus tolerance of 6 percent will be allowed in capacity, and a plus or minus tolerance of $\frac{1}{8}$ inch will be allowed in all measurements of 1 inch and over, and a plus or minus tolerance of $\frac{1}{16}$ inch will be allowed in all measurements of less than 1 inch, except those applying to thickness of the material. The tolerances shall be applied in such a way as not to interfere with the proper stacking of the bowls of like size and design.

**3.6 Workmanship.**—The workmanship shall be free from defects which will affect the appearance or may affect the serviceability. It shall be free from rough grindmarks, trimming marks, pits, scales, or other defects or imperfections. All surfaces shall have a smooth finish and shall be free from sharp edges.

## 4. SAMPLING, INSPECTION AND TEST PROCEDURES

**4.1 Sampling for lot acceptance.**

4.1.1 *Inspection lot.*—All bowls of the same size presented at one time shall be considered a lot for the purpose of acceptance, inspection and tests.

4.1.2 *Sampling for inspection.*—Samples of bowls shall be taken in accordance with quantities listed in table II from each inspection lot of bowls offered for Government inspection of visual, dimensional, and weight characteristics with lot acceptance based on the sampling inspection requirements in accordance with Military Standard MIL-STD-105.

TABLE II.—*Sampling for visual, dimensional and weight inspection AQL (approximate) 2.5 percent defective*

| Number of bowls of each size in inspection lot | Number of bowls of each size in sample | Acceptance number (defectives) | Rejection number (defectives) |
|---|---|---|---|
| 15 or under | 3 | 0 | 1 |
| 16 to 40 | 7 | 0 | 1 |
| 41 to 110 | 15 | 1 | 2 |
| 111 to 300 | 35 | 2 | 3 |
| 301 to 500 | 50 | 3 | 4 |
| 501 to 800 | 75 | 4 | 5 |
| 801 and over | 110 | 6 | 7 |

4.1.3 *Sampling for lot acceptance tests.*—One bowl shall be selected by Government inspector from each 300 bowls or fraction thereof in a shipment for lot acceptance tests.

**4.2 Tests.**—One bowl shall be selected for test from among the sample bowls selected in accordance with paragraph 4.1.3, submitted for inspection. Any or all tests as outlined below shall be conducted on the representative specimen bowls. These tests shall be made by the inspector, or through his instruction at any Government laboratory or other designated place.

4.2.1 *Retests.*—If any sample of bowls tested should fail two additional samples shall be tested, both of which shall comply with the requirements of this specification. Failure of these samples to pass acceptance tests will be cause for rejection of the entire lot.

4.2.2 *Chemical composition.*—From the bowl or bowls selected for test, millings or drillings for chemical analysis shall be taken to determine the conformity of the material with the requirements of 3.1.1. The millings or drillings shall weigh not less than 4 ounces and shall be clean, free from oil, dirt, grit, or other foreign matter. Spectrographic analysis may be used in lieu of above method.

4.2.3 *Salt-spray test.*—From the bowl or bowls selected for test the following salt-spray test shall be conducted. The salt-spray test shall consist of exposure, in a closed tank made of neutral material (such as wood or soapstone),



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.

to a finely divided spray at 95° plus or minus 5° F., 10-percent solution of sodium chloride c. p. (by weight) in distilled water for a period of 48 hours. The tank shall be so designed that there shall be no direct impingement of the spray upon the specimen bowl and the spray shall circulate freely about the specimen to the same degree. No liquid which has come in contact with the specimen under test shall return to the aspirator to be resprayed. Before being placed in salt-spray bath the specimen bowl tested shall be thoroughly cleaned by washing in petroleum ether and alcohol and then dried. Slight surface corrosion of the specimen which can easily be washed off shall not be considered as cause for rejection, but if the specimen should rust or show continuous bleeding from pits it shall be considered as having failed to pass the test.

## 5. PREPARATION FOR DELIVERY

**5.1 Packaging.**—Unless otherwise specified, bowls shall be wrapped in kraft paper and packed individually in substantial cartons.

**5.2 Packing.**—Unless otherwise specified, cartons containing bowls shall be packed for shipment in standard commercial containers, so constructed as to permit acceptance by carrier for safe transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

**5.3 Marking.**

5.3.1 *Issue packages.*—Each package shall be marked with the name of the material and the name of the manufacturer.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name of the material and the quantity contained therein as defined by the contract or order under which the shipment is made, the name of the contractor, and the number of the contract or order.

## 6. NOTES

**6.1 Intended use.**—Bowls covered by this specification are intended for use in hospitals, physicians' offices and first-aid offices, in applications suitable for each type.

**6.2** Purchasers should exercise any desired options offered herein. (See 1.2.1, 3.3.1.1, 3.5, 4.2.2, 5.1, 5.2, 5.3.2, and 7.2.5.)

**6.3** It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

**6.4** Federal specifications do not include all types, classes, grades, sizes, etc., of the commodities indicated by the titles of the specifications, or which are commercially available, but are intended to cover the types, etc., which are suitable for Federal Government requirements.

**6.5** This specification covers the following item appearing in the Armed Services Medical Stock List:

6530–772–0326—Bowl, gauze pad, corrosion resisting steel.

**6.6 Transportation description.**—Transportation description applicable to this item is:

Sheet steel ware, not otherwise indexed by name, with or without copper bottoms. (Indicate nested, not nested or nested solid, flat or folded flat.)
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Sheet steel articles, not otherwise indexed.
Truckload minimum weight 20,000 pounds.

**Patent notice.**—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

## 7. DEPARTMENTAL REQUIREMENTS

**7.1** The following specifications and standards, of the issues in effect on date of invitation for bids, and special requirements, form a part of this specification for purchases made under this specification by the respective departments.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.

**7.2 Army, Navy, and Air Force.**

**7.2.1** *Applicable specifications and standard:*

*Federal Specifications:*

NN-B-621—Boxes, Wood, Nailed and Lock-Corner.

NN-B-631—Boxes, Wood, Wirebound (for Domestic Shipment).

LLL-B-631—Boxes, Fiber Corrugated (for Domestic Shipment).

PPP-B-601—Boxes, Wood, Cleated, Plywood.

PPP-B-676—Boxes, Setup, Paperboard.

*Military Specifications:*

JAN-P-106—Packaging and Packing for Overseas Shipment Boxes; Wood, Nailed.

MIL-B-107—Boxes, Wood, Wirebound (Overseas Type).

MIL-B-10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

MIL-L-10547—Liners, Case, Waterproof.

*Military Standard:*

MIL-STD-129—Marking for Shipment and Storage.

**(Copies of specifications, standard, and drawings, required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).**

**7.2.2** *Packaging.*

**7.2.2.1** *Unit of issue.*—One (1) bowl, as specified, constitutes one unit.

**7.2.2.2** *Unit packaging.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with the requirements of Federal Specification LLL-B-631 or PPP-B-676. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Each carton shall be adequately secured to prevent accidental opening.

**7.2.3** *Packing.*

**7.2.3.1** *For domestic shipment.*—Twenty-four unit cartons (24 units) shall be overpacked in an exterior container. Construction, closure, and strapping (when required) shall be in accordance with the requirements of Federal Specification NN-B-621, NN-B-631, or Military Specification MIL-B-10377 (table I), for type 2 load; or Federal Specification PPP-B-601 (table I; type III, class 1 plywood).

**7.2.3.2** *For overseas shipment.*—Twenty-four unit cartons (24 units) shall be overpacked in an exterior container designed for type 2 load and constructed in accordance with the requirements of Military Specification JAN-P-106, MIL-B-107, or MIL-B-10377 (table II); or Federal Specification PPP-B-601 (table II; type III, class 1 plywood).

**7.2.3.2.1** *Case liner.*—Each box shall be lined with waterproof case liner conforming to the requirements of Military Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

**7.2.3.2.2** *Strapping.*—Strapping, when required, shall be in accordance with applicable box specification.

**NOTE.—Strapping will not be permitted for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.**

**7.2.3.3** *Packing variation permitted.*—If the number of units in any shipment is less than the specified number of units to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design which will insure safe delivery to destination.

**7.2.4** *Marking.*—Each unit carton and each shipping container shall be marked in accordance with Military Standard MIL-STD-129.

**7.2.5** *Ordering data.*—Requests, requisitions, schedules, and contracts or orders should specify whether the subject commodity is to be packed for domestic or overseas shipment. (See 7.2.3.1 and 7.2.3.2.)

**Military Interest:**
**Army: M**
**Navy: Md**
**Air Force: USAF**



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:10Z
Check the source to verify that this is the current version before use.