RR-C-901/3
January 15, 1981
SUPERSEDING
MS39226
December 1, 1969

FEDERAL SPECIFICATION SHEET

CYLINDER, COMPRESSED GAS:

DOT SPECIFICATION 3AA

AND ALUMINUM APPLICATIONS,

FOR MEDICAL SERVICES

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal Agencies.

The complete requirements for procuring compressed gas cylinders, Specification DOT 3AA described herein, shall consist of this document and the issue in effect of Specification RR-C-901.

TABLE I

Part Number	Size Code	Gas Service	Capacity lbs	Dia Hgt inches	Valve MIL-V-2	Max Wt lbs	H_2O Cap cu in
C901/3-1	D	Nitrous Oxide N_2O	250 Gal	4-1/4 x 17	V38-911	10	170
C901/3-2	M	Nitrous Oxide	2000 Gal	7 x 43	V37-1321	64	1320
C901/3-3	D	Oxygen O_2	95 Gal	4-1/4 x 17	V42-871	10	170
C901/3-4	E	Oxygen O_2	165 Gal	4-1/4 x 26	V42-871	14	283
C901/3-5	M	Oxygen O_2	800 Gal	7 x 43	V41-541	64	1320
C901/3-6	H	Oxygen O_2	1650 Gal	9 x 51	V41-541	120	2640

DESIGN REQUIREMENTS:

1. The cylinder shall be as specified in table I. All dimensions are in inches with tolerances for diameter, plus or minus 1/4 inch and for height, plus or minus 1 inch.
2. All cylinders fabricated for medical services shall be supplied with a medical valve as specified. Each medical cylinder shall be equipped with a flange and a valve protection cap in accordance with figure 1, unless otherwise specified.

FSC 8120

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

3. When aluminum cylinders are specified they shall conform to the issue of RR-C-901 in effect.
4. MIL-STD-101 is mandatory for all Government medical cylinders for both Government-owned and vender-owned containers and all materials provided in the cylinder package shall pass tests specified in MSFC-SPEC-101A (NASA).
5. Military Medical Services Tag. A tag shall be used on filled medical cylinders when medical cylinders are purchased as part of a medical gas commodity contract. The tag shall be in accordance with UU-T-81, type B, class 2, size 5, grade 15 SU, and shall be attached to each cylinder. Marking shall include the National Stock Number, the name of the specified gas, cylinder size, cylinder capacity in gallons, lot number contract number, cylinder serial number, contractor's name or registered trademark, and necessary precautionary markings. The statement "CAUTION: Federal Law Prohibits Dispensing Without Prescription." shall appear on the tag, if it does not appear on the cylinder. In addition, tags for nitrous oxide cylinders shall bear the markings for total gross weight of the cylinder, tare weight and net weight (weight of nitrous oxide liquid). These markings shall allow weights to be indicated in pounds and ounces.

   The tags shall be furnished with a metal eyelet and stringing wire. The wire shall be tinned, annealed, or galvanized, and be not less than 23 gage.

   Tag colors shall be as follows:

   Background - Same color as cylinders
   Print - Black

   OR

   Background - White
   Print - Same color as cylinders

   The bottom of the tag shall be designed with a three-part legend marked on both sides with perforated lines between the legends for easy removal as follows:

   "EMPTY"
   "IN USE"
   "FULL"

6. Marking for medical cylinders. Medical cylinders shall be permanently marked not less than 3/16 inch high for cylinders less than 6 inches in outside diameter and not less than 3/8 inch high for cylinders more than 6 inches in outside diameter as follows:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

(a) The capacity in gallons shall be marked on the shoulder of each cylinder. (Capacities shall be at 15° C and 760 mm Hg.)
(b) To the right of the manufacturer's symbol, the letters "MED" shall be added either horizontally or vertically.
(c) Name of gas abbreviated as follows:

	STAMPED	STENCILED
1. OXYGEN	"O_2"	OXYGEN - U.S.P.
2. NITROUS OXIDE	"N_2O"	NITROUS OXIDE - U.S.P.

7. Valves. Medical valves shall be in accordance with MIL-V-2 as specified in table I.

INTENDED USE:

The cylinders covered in this specification sheet are intended for use in medical gas services for storage and transportation.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

X-3179A

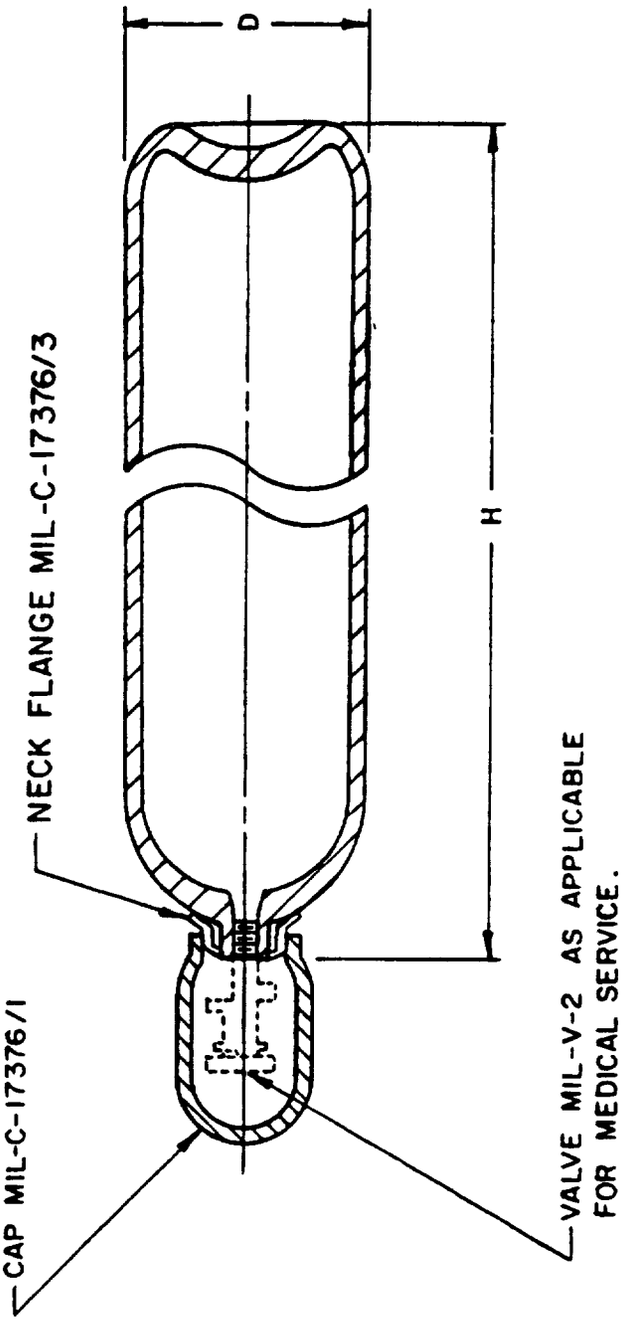


FIGURE 1. Cylinder configuration.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - ME
Navy - SH
Air Force - 68

Review activities:

Army - MI, EA
Navy - MS, AS, OS

User activities:

Navy - YD, MC
DLA - GS, PS

Civil Agency Coordinating Activities:

GSA-FSS
DOT-OHM
HEW-NIH
JUS-FPI
VA-DMS

Preparing activity:

Army - ME

Project No. 8120-0370

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No 22-R255

INSTRUCTIONS The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document DoD contractors, government activities or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government Fold on lines on reverse side, staple in corner, and send to preparing activity Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements Attach any pertinent data which may be of use in improving this document If there are additional papers, attach to form and place both in an envelope addressed to preparing activity

DOCUMENT IDENTIFIER AND TITLE RR-C-901/3 Cylinder, Compressed Gas: DOT Specification 3AA and Aluminum Applications, for Medical Services

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1 HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A GIVE PARAGRAPH NUMBER AND WORDING

B RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2 COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3 IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO (If "Yes" in what way?)

4 REMARKS

SUBMITTED BY (Printed or typed name and address - Optional)	TELEPHONE NO
	DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

FOLD

POSTAGE AND FEES PAID
DEPARTMENT OF THE ARMY
DOD – 314

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

Commander
US Army Mobility Equipment Research and
Development Command
DRDME-DE/DS
Fort Belvoir, VA 22060

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.