RR-S-705E
September 3, 1976
SUPERSEDING
Int. Fed. Spec. RR-S-00705D(DSA-DM)
September 22, 1970 and
Fed. Spec. RR-S-705
June 20, 1949

FEDERAL SPECIFICATION

STAND, BASIN

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers three types of basin stands, complete with basins, for use in medical facilities.

1.2 Classification.

1.2.1 Types. The stands covered by this specification shall be of the following types (see 6.2).

Type I - Stand, Basin, Single, Corrosion-Resisting Steel for 9 quart basins.

Type II - Stand, Basin, Double, Corrosion-Resisting Steel for 7 quart basins.

Type III - Stand, Basin, Double, Corrosion-Resisting Steel for 9 quart basins.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

FF-C-77 - Casters, Rigid and Swivel (Institutional Duty).
RR-B-120 - Basin; Emesis, Basin Wash; (Corrosion- Resisting Steel).
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

Federal Standards:

Fed. Std. No. 66	- Steel; Chemical Composition and Hardenability.
Fed. Std. No. 123	- Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 151	- Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.

Military Specifications:

MIL-L-10547	- Liners, Case and Sheet, Overwrap, Water-Vaporproof or Waterproof, Flexible.

Military Standards:

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

National Fire Protection Association (NFPA)

No. 56A Standard for the Use of Inhalation Anesthetics (Flammable and Non-flammable)

(Application for copies should be addressed to the National Fire Protection Association, 470 Atlantic Avenue, Boston, MA 02210.)

American Welding Society, Inc.

Welders Handbook, 6th Edition

(Application for copies should be addressed to the American Welding Society, Inc., 345 East 47th Street, New York, NY 10017.)

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Material. Material for the stands and basins shall be corrosion-resisting steel, conforming to chemical composition for AISI 302 or 304 of Fed. Std. No. 66, when tested as specified in 4.4.1. Commercial tolerances shall apply to all thicknesses specified herein.


3.3 Design and construction. Design and construction of the basin stand shall be as shown for the applicable type in figures 1, 2, 3, and 4 and as specified herin.

3.3.1 Type I stands. Type I stands shall have one basin ring which shall accommodate one 9 quart basin. One basin shall be furnished and shall be in accordance with type II, class 1, 9 quart capacity, of RR-B-120 except the overall height of the basin shall be 4-7/8 ± 1/8 inches.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

COMPONENT	TYPE I DIMENSIONS		TYPE II DIMENSION	
LEG	A	34 ± 1	A	34 ± 1
TRANSVERSE BRACE	B	13 13/32 ± 1/8	B	12 1/4 ± 1/32
	C	8 1/4 ± 1/4	C	8 1/4 ± 1/4
LENGTHWISE BRACE	D	13 1/4 ± 1/8	D	30 ± 1/4
BASIN RING	E	I.D. OR DISTANCE BETWEEN, RODS 13 1/16 ± 1/16	E	I.D. 11 15/16 ± 1/16

NOTE: ABOVE DIMENSIONS ARE FOR DESIGN PURPOSES.
MANUFACTURING TOLERANCES ARE AS FOLLOWS:
0-12 INCHES, ± 1/32 INCH
OVER 12 INCHES, ± 1/16 INCH

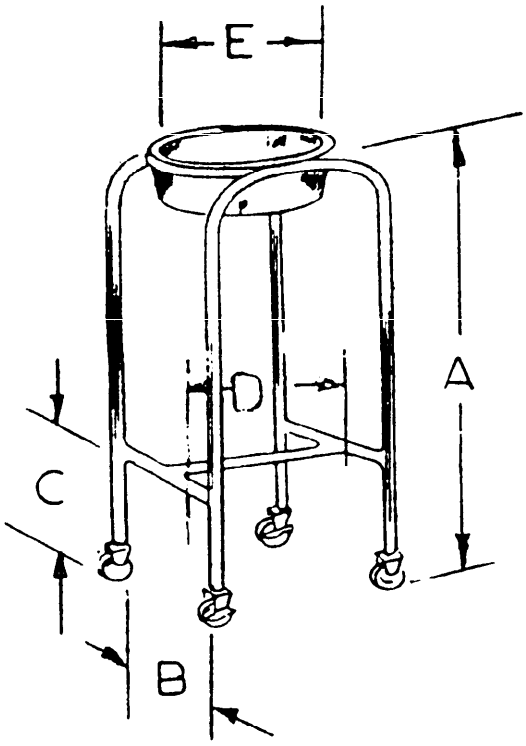


TYPE I ONE BASIN STAND

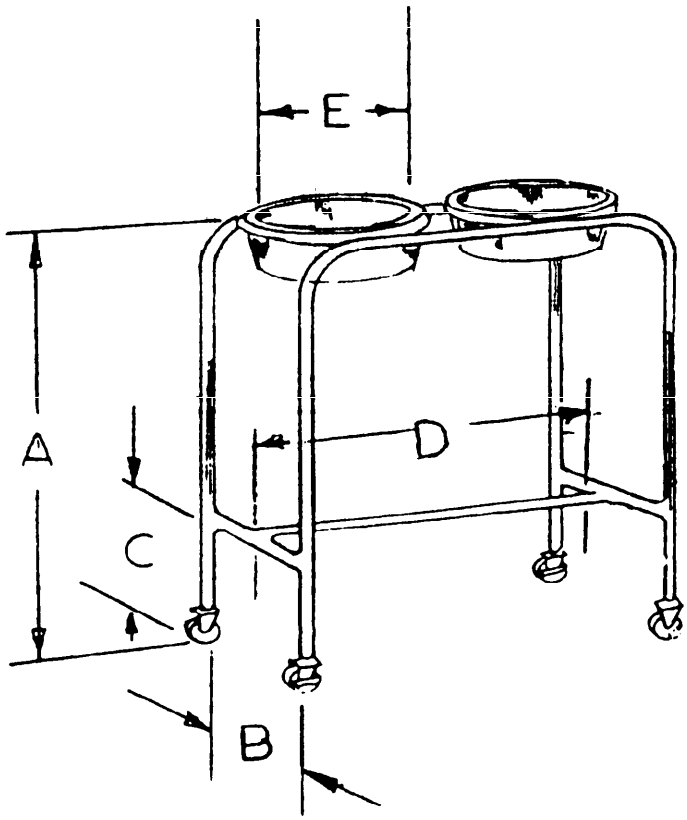

TYPE II TWO BASIN STAND

NOTE: WELD BASIN RING 7± 1/4 INCHES FROM EACH END AS MEASURED FROM INSIDE OF LEGS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

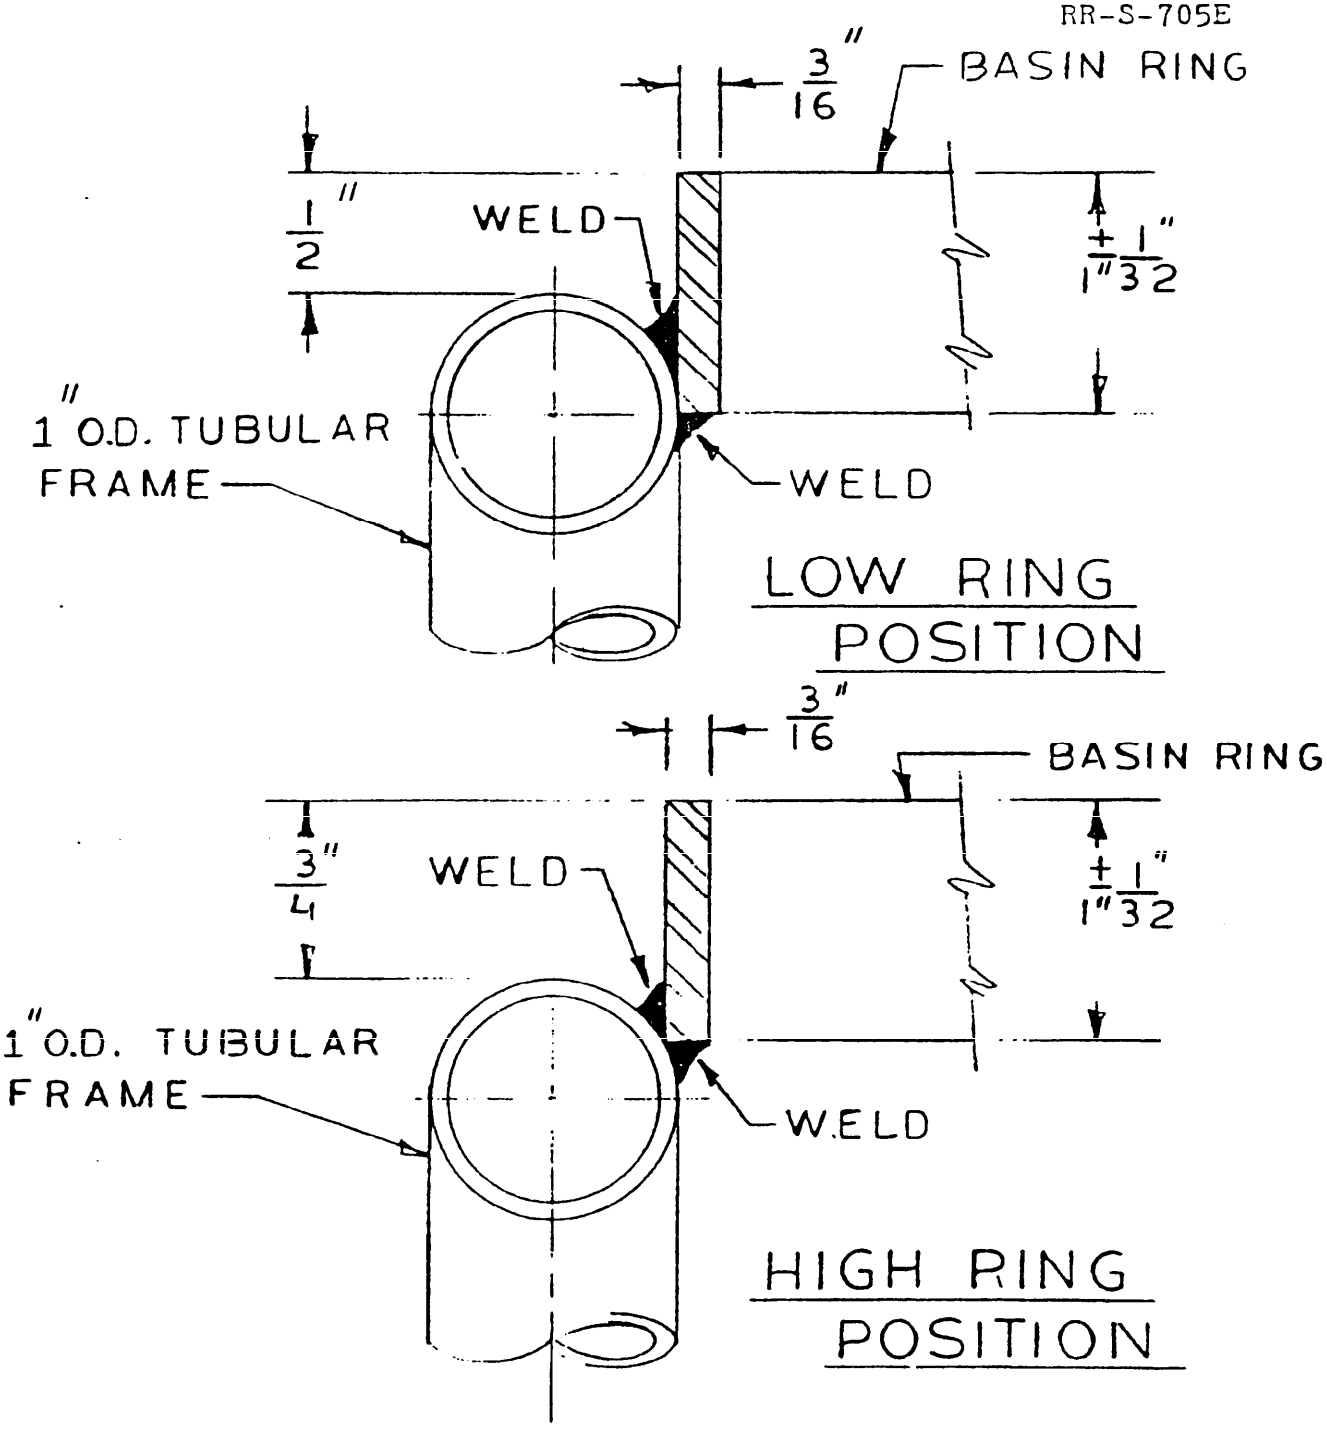

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.


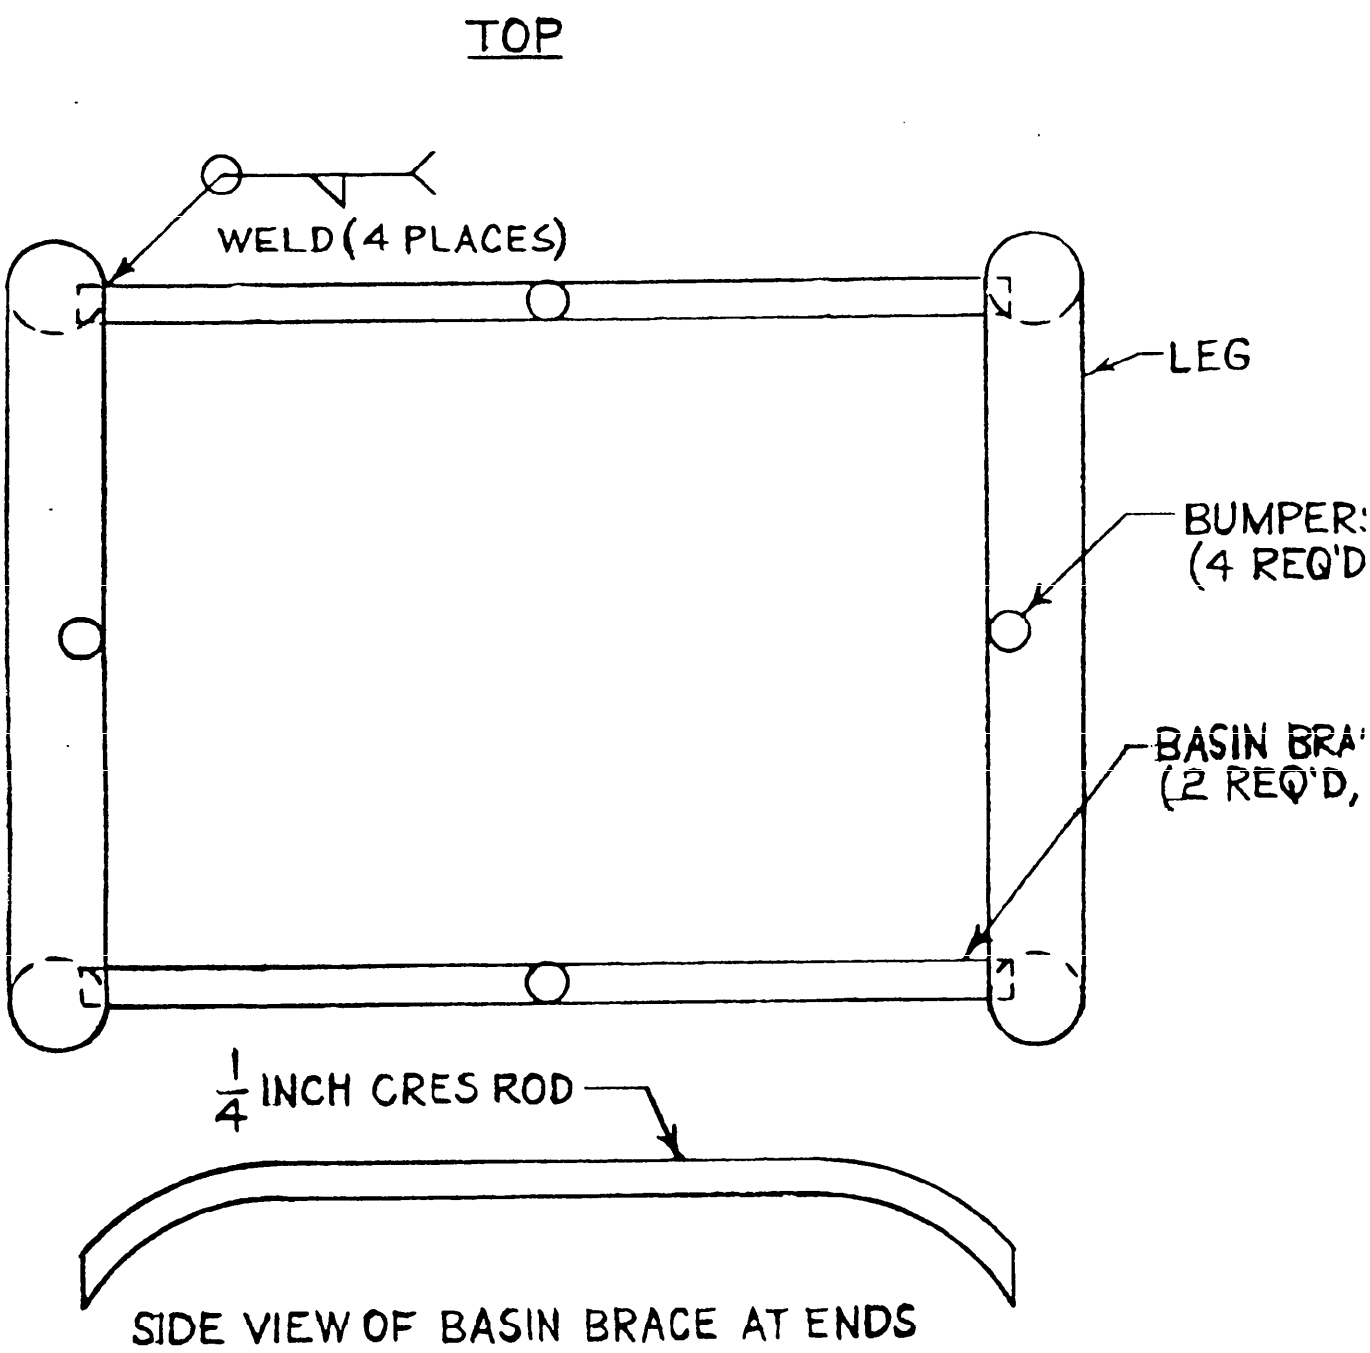


FIGURE 3

ALTERNATE BASIN BRACE CONSTRUCTION FOR ONE BASIN STAND

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

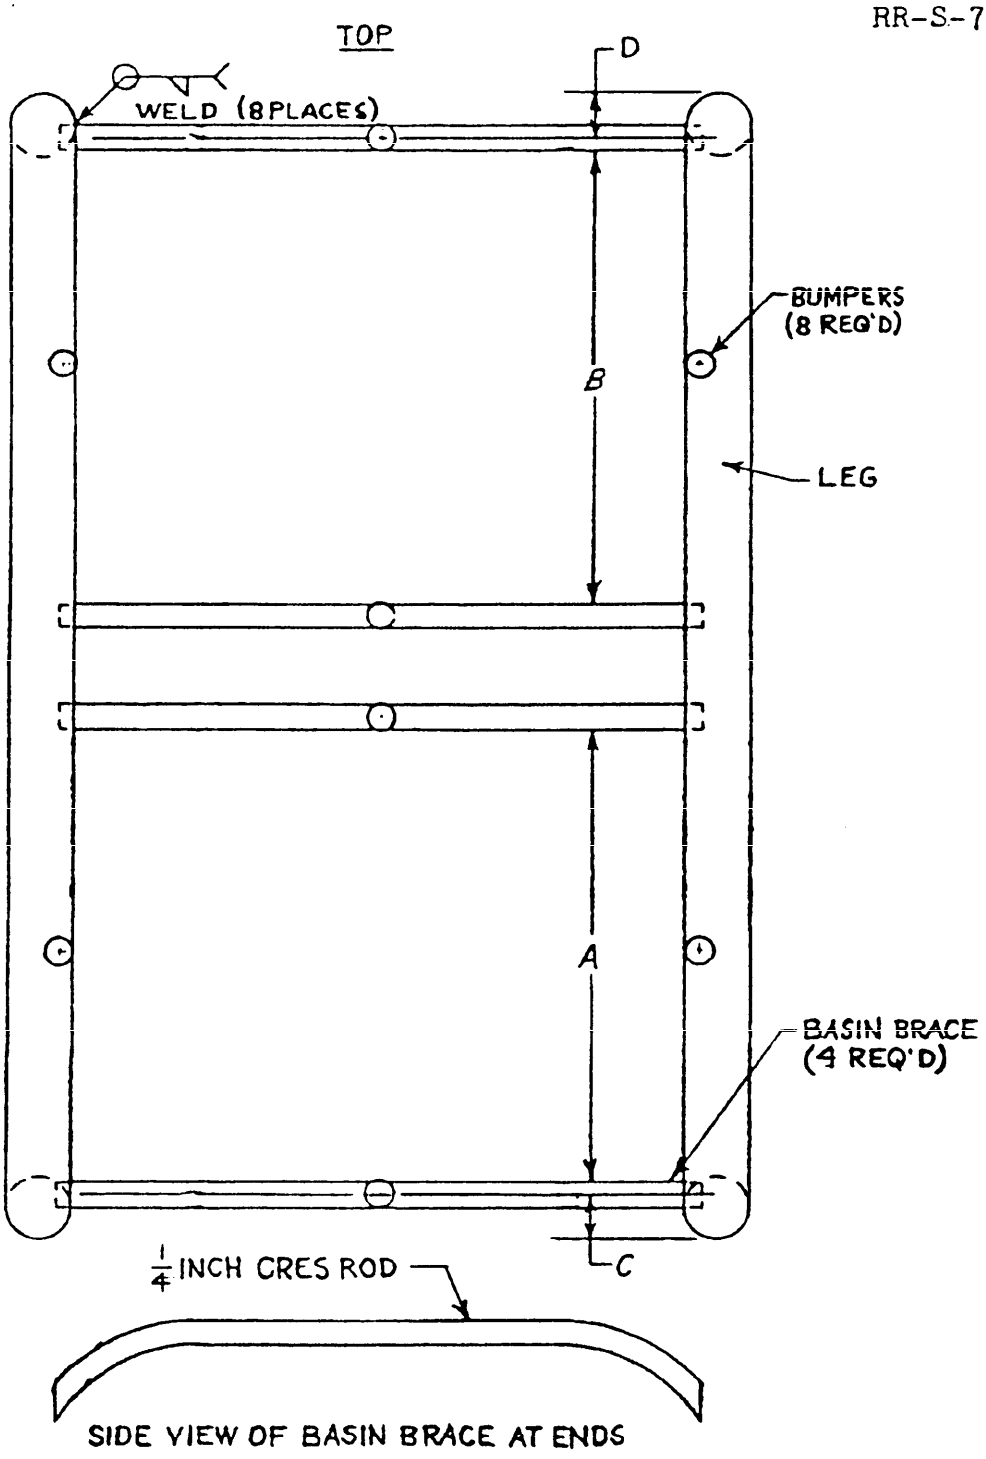

NOTE: BASIN BRACES SHALL BE LOCATED SUCH THAT BASINS WHEN SEATED ON THE RUBBER CONDUCTIVE TIPS REMAIN IN A POSITION NORMAL TO THE UPRIGHTS. FURTHER, THE BASIN BRACES SHALL BE LOCATED SUCH THAT DIMENSIONS "A" AND "B" ARE EQUAL AND "C" AND "D" ARE EQUAL.

FIGURE 4

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

3.3.1.1 Frame. The frame shall be made from seamless or welded tubing not less than .049 inch thick (No. 18 Birmingham Wire (B.W.) gage) nor greater than .065 inch thick (No. 16 B.W. gage) except as indicated below. Round tubing shall be 7/8 + 1/8, -1/64 inches in diameter, while square tubing shall be 7/8 ± 1/64 inches wide. Two lengths of tubing shall be bent and shaped on 3 inch radii to form two well rounded inverted "U"s. Each "U" tubing shall form one longitudinal side of the top and two legs. Dimensions shall be as shown in figure 1. The legs of the frame shall be equipped with casters, see 3.4.

3.3.1.2 Transverse brace. The transverse brace shall be made from seamless or welded tubing not less than .049 inch thick (No. 18 B.W. gage) not greater than .065 inch thick (No. 16 B.W. gage) except as indicated below. Round tubing shall be either 3/4 ± 1/64 inches or 7/8 + 1/8, -1/64 inches in diameter, while square tubing shall be 7/8 ± 1/64 inch wide. As an alternate to round or square tubing for the brace, 3/8 inch corrosion-resisting steel rod shall be allowed. The tubing or rod shall be welded to each end of the frame and shall protrude at least 1/4 inch within the wall of the frame. Dimensions shall be as shown in figure 1.

3.3.1.3 Longitudinal brace. The longitudinal brace shall be made from seamless or welded tubing not less than .049 inch thick (No. 18 B.W. gage) nor greater than .065 inch thick (No. 16 B.W. gage) except as noted below. Round tubing shall be either 1/2 ± 1/64 inches or 7/8 + 1/8, -1/64 inches in diameter, while square tubing shall be 7/8 ± 1/64 inch wide. As an alternate to round or square tubing for the brace, 3/8 inch corrosion-resisting steel rod shall be allowed. The tubing or rod shall be welded to the middle point of the two transverse braces, forming a double "T" brace, see figure 1. Dimensions shall be as shown in figure 1.

3.3.1.4 Basin ring. The basin ring shall be fabricated from corrosion-resisting steel strip having the following dimensions: 1/8 to 3/16 inch thick, 31/32 to 1-1/4 inch wide. The steel strip shall be shaped into a ring and shall be attached to the top of the frame and shall extend 1/2 to 3/4 inches above the top of the frame, see figure 2. The ring shall be welded into a single seamless piece before being welded to the frame. The steel strip basin ring shall be continuously welded to the frame midpoint from the ends by welds not less than 1-1/4 inches in length. Welding shall be as specified in 3.6.

3.3.1.4.1 Alternate basin support. As an alternate, the basin support shall consist of 1/4 inch corrosion-resisting steel rod welded to the legs as shown in figure 3. The steel rod basin braces shall be level with the top of the frame.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

3.3.1.5 Rubber bumper tips. There shall be four well rounded electrically conductive tips, attached to the inner surface of the basin rings by a screw which passes through the ring and into the back of the rubber for basin rings constructed of steel strip. Basin supports fabricated from corrosion-resisting steel rod shall have the rubber tips fastened to the frame and brace rods in the same manner as described above; see figure 3. As an alternative, three electrically conductive bumpers may be fastened to the basin rings as described above, however, the bumpers shall be located 120 degrees apart from each other. The basin shall rest on top of the basin ring and shall be prevented from rattling by the rubber tips.

3.3.2 Type II stands. Type II stands shall have two basin rings and shall accommodate two 7 quart basins. Two 7 quart basins shall be furnished and shall be in accordance with the applicable requirements in RR-B-120 for type II, class 1, 7 quart capacity.

3.3.2.1 Frame, transverse and longitudinal braces. Frame and longitudinal and transverse braces shall be made of the same material and construction as specified for type I stands (3.3.1) except as indicated in figure 1.

3.3.2.2 Basin ring. Shall be as specified in 3.3.1.4 except the ring shall be welded into a single seamless piece having an inside diameter as indicated in figure 1. The steel strip basin rings shall be continuously welded to the frame from the ends, by welds not less than 1-1/4 inches in length. Welding shall be as specified in 3.6.

3.3.2.2.1 Alternate basin support. As an alternate, the basin support shall consist of 1/4 inch corrosion-resisting steel rod welded to the legs as shown in figure 4. The steel rod basin braces shall be level with the top of the frame.

3.3.2.3 Rubber bumper tips. Shall be as specified in 3.3.1.5 except as shown in figure 4. As an alternate, three electrically conductive bumpers may be fastened to the basin rings as described above; however, the bumpers shall be located 120 degrees apart from each other. The basin shall rest on top of the basin ring or support and shall be prevented from rattling by the rubber tips.

3.3.3 Type III stands. Requirements for type III stands shall be the same as for type II stands except that they shall accommodate two 9 quart basins. The 9 quart basins shall be furnished and shall be in accordance with the applicable requirements in RR-B-120 for type II, class 1, 9 quart capacity. The basin ring shall be as specified in 3.3.1.4; The inside diameter of the ring shall be 13-1/16 $\pm$ 1/16 inches.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

3.4 Casters. Each basin stand shall be equipped with 3 inch diameter electrically conductive casters, conforming to Type II, Class A, Style b, Mounting A or N of FF-C-77. Two casters are required to have side brakes. If utilized, rubber adapters in rubber expanding stems shall be of electrically conductive rubber, or have metal clips designed so that positive metal to metal contact is made as the adapter is expanded. The stand with the casters in place shall meet the requirements for Reduction in Electrostatic Hazard Furniture as specified in 4.4.2.

3.5 Finish. Stands shall have a No. 4 commercial finish.

3.6 Welding. Welding shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society in the Welders Handbook, 6th Edition. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal and/or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreing matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks which affect the quality, and have more strength than required for purpose intended. For the purpose of requirements in this specification, welded fully, fully welded continuously welded, and continuous weld shall all have the same meaning such that all the mating surfaces between the parts being welded are closed by welds without any breaks or voids. Grinding wheels used to remove excess weld metal and to prepare weld surfaces for subsequent polishing operations shall be of a suitable grit, free of metal filings or other iron materials such as iron oxides which would tend to cut into the parent metal surfaces and allow for rusting at a later date.

3.7 Workmanship. Workmanship shall be first class throughout. The basin stands, and basins, shall be free from defects which detract from their appearance, or which may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties.)

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the stands when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and tests of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as shown in table I.

TABLE I. Sampling for examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-3	1.0
Total (major and minor combined)	S-3	4.0
For dimensional examination	S-1	2.5

4.2.1 For tests. Sampling for tests shall be conducted in accordance with inspection level S-3 of MIL-STD-105. The acceptance level shall be zero.

4.3 Examination. The basin stands, and the basins, shall be examined to determine compliance with all the reqirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects shown in table II. Examination shall not be restricted to the classified possible defects listed below.

TABLE II. Classification of defects

Categories	
Major:	
101	Any component part missing, broken or otherwise unusable.
102	Exposed parts not free of burs.
103	Exposed parts not free from sharpness.
104	Stands not free from wobble; do not set level when resting on level floor.
105	Casters not free from binding.
106	Casters not freely running.
107	Tubular elements not smoothly bent to the required radius.
108	Casters not of the required size.
109	Casters not the required design.
110	Basins do not fit properly in basin rings.
111	Tubular elements not free of kinks.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

TABLE II. Classification of defects -continued

Categories	Defects
Minor	
201	Finished stands not free from dents, cracks, or crimps.
202	Finished not as specified.
203	Finished stands not free from oil, grease, dirt.

4.3.2 Dimensional examination. The stands be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as defect.

4.3.3 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of section 5. Defects shall be scored but not limited to those as specified in table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of percent defective.

TABLE III. Examination of preparation for delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted; incorrect; illegible; improper size, location, sequence, or method of application.
Materials	Any component missing or damaged.
Workmanship	Bulging or distortion of containers. Cushioning inadequate, improper or missing.

4.3.4 Examination of closure, waterproofing and banding for containers. When shipping containers are required to comply with PPP-B-601, PPP-B-621 or PPP-B-636, examination for defects in closure, waterproofing and banding shall be in accordance with the appendix to the appropriate specification.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of Fed. Test Method Std. No. 151.

4.4.2 Electrical conductivity. The basin stands, complete with casters, rubber ring tips and basin(s) shall be tested using the method described in NFPA No. 56A.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit preparation. Each complete stand shall be protected by wrapping with kraft paper and cushioned with flexible corrugated fiberboard or similar cushioning material. The wrapping and cushioning material shall be secured by tying or taping. The work shall be accomplished in such a manner as to insure against marring, scratching or damage to the stand.

5.1.2 Level C. Each stand shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Each complete stand shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant, grade V3c. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable box specification. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof as specified in the appendix of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. Each complete stand shall be packed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, type CF, class domestic. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

5.3.2 Military activities. Each exterior container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. Intended for use in surgical service and treatment rooms of hospitals.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number, and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1, 6.3).
d. Type required (see 1.2.1).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification	Type
6530-00-708-1000	STAND, BASIN, Double, Corrosion-Resisting Steel	II
6530-00-708-1025	STAND, BASIN, Single, Corrosion-Resisting Steel.	I

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Civil Agency Coordinating Activities:

GSA-FSS
VA-DMS

Project No. 6530-1386

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 45 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the currentversion before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

RR-S-705E STAND, BASIN

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.