RR-S-709B
August 20, 1975
SUPERSEDING
Int. Fed. Spec. RR-S-00709A(DSA-DM)
September 29, 1966 and
Fed. Spec. RR-S-709
September 8, 1954

FEDERAL SPECIFICATION

STAND, IRRIGATOR

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 Scope. This specification covers an irrigator stand for use in suspending solution containers or an irrigator can.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

Federal Specifications:

PPP-B-601 - Box, Wood, Cleated-Plywood.
PPP-B-621 - Box, Wood, Nailed and Lock-Corner.
PPP-B-640 - Box, Fiberboard, Corrugated, Triple-Wall.

Federal Standards:

Fed. Std. No. 66 - Steel: Chemical Composition and Hardenability.
Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 151 - Metal, Test Methods.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal specifications required by activities outside the Federal Government for bidding purposes are available without charge from the Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specification:

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Welding Society

Welders Handbook, 6th Edition

(Applications for copies should be addressed to American Welding Society, Inc., 345 47th Street, New York, NY 10017.)

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material.

3.1.1 Corrosion-resisting steel. Corrosion-resisting steel shall conform to the chemical requirements for AISI 302 or 304 of FED-STD-66, when tested as specified in 4.4.1.

3.2 Construction. The irrigator stand shall consist of a glide mounted base, a fixed vertical tubular post, an inner telescoping extension tube for adjustment from 72 to 104 inches, an automatic locking device, and a straight crossbeam having a notch at each end. Construction shall be in accordance with Figure 1.

3.2.1 Base. The base shall consist of four evenly spaced legs manufactured in accordance with Figure 1. The center of the base shall be so constructed as to receive, and rigidly hold, the fixed tubular post in a vertical postion. The base shall be weighted for stability so that the stand can be tilted a minimum of 25 degrees without overturning when tested as specified in 4.4.2.

3.2.1.1 Glides. Glides shall be corrosion-resisting steel with the following minimum dimensions: 1 inch diameter base, 1-1/2 inch height, and 1/4 inch diameter threaded stem.

3.2.2 Fixed tubular post. The fixed tubular post shall be one continuous piece of corrosion-resisting steel tubing fabricated in accordance with Figure 1 so that it can be securely attached to the base. It shall be possible to disconnect tube from base to facilitate shipping and storage.

3.2.3 Automatic locking device. The stand shall be provided with an automatic locking control mechanism with convenient one-hand control that shall permit unrestrained upward and downward movement of the telescoping extension tube. The lock shall be activated by a suitable means such as a sleeve, trigger or button-type release. The telescoping tube shall automatically and positively lock in place at the point of adjustment desired when tested as specified in 4.4.3. Reference to a suitable locking device is provided in 6.2. All parts of the slide lock mechanism shall be fabricated of corrosion-resisting steel and corrosion-resisting metal; plastic parts are not considered to be suitable. The locking mechanism shall support a ten pound load when tested as specified in 4.4.4. Any slippage in the locking mechanism shall be considered a defect.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:11Z
Check the source to verify that this is the currentversion before use.

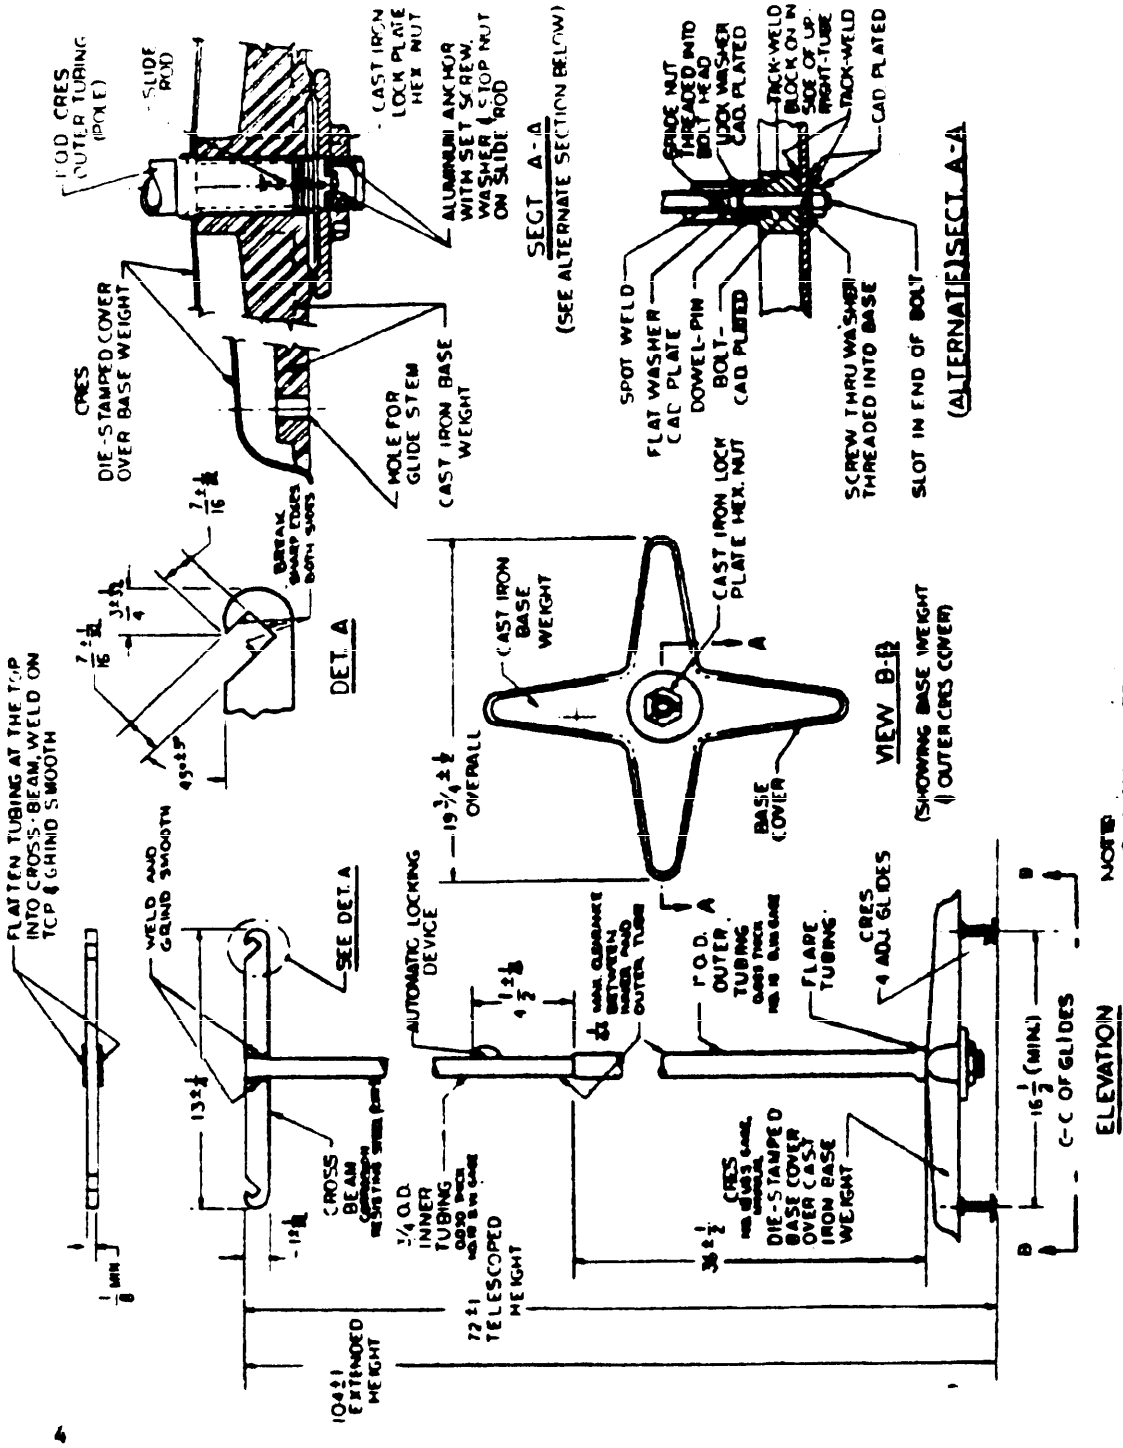


FIGURE 1. STAND, IRRIGATOR

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:11Z
Check the source to verify that this is the current version before use.

3.2.4 Extension Tube. The extension tube shall be one continuous piece of corrosion-resisting steel tubing fabricated in accordance with Figure 1. The outside diameter shall fit freely within the fixed tubular post but without perceptible side play.

3.2.5 Crossbeam. The crossbeam shall be a corrosion-resisting steel bar as detailed in Figure 1, securely welded to the top of the extension tube.

3.3 Welding. Shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal and/or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive spatter. Fusion through the full thickness of the base metal, in areas other than those where 100% penetration is a requirement of joint design, are not acceptable when welding materials over 0.050 inch in thickness. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks and have more strength than required for purpose intended.

3.4 Finish. All visible surfaces of the stand shall be ground and polished to produce a No. 4 commercial finish. The irrigator stand shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, grinding compound, and metal residue. Before assembling to the base, the cast iron weight shall be painted on all surfaces, except caster mounting holes, with aluminum paint.

3.5 Identification marking. Each stand shall be marked with the contract or purchase order number.

3.6 Workmanship. Workmanship shall be first class throughout. The stand shall be free from defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

SUPERSEDING

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

TABLE I. Sampling for Examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total defects (Major and Minor combined)	II	4.0
For dimensional examination	S-3	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 for an Inspection level of S-1 and AQL of zero.

4.3 Examination. The stand shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects, as shown in Table II.

TABLE II. Classification of Defects*

Categories	Defects
Major	
101	Any component part missing, broken, or otherwise unusable.
102	Exposed edges not free of burs or sharpness.
103	Base legs do not rest evenly on a flat surface.
104	Telescoping extension tube not vertical at all desired heights.
105	Crossbeam not perpendicular to the extension tube.
106	Crossbeam height not adjustable within specified range of elevation.
Minor	
201	Identification marking not complete or legible.
202	Finish not free of chipped areas, cracks, scratches, or roughness.

*Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of FED-STD-151.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

4.4.2 Stability test. The telescoping tube of the stand shall be extended so that the top of the crossbeam is 7 feet above the floor line. The unit shall then be tipped on two legs, and the maximum angle from the vertical from which the stand will return to the normal vertical position when released shall be measured.

4.4.3 Automatic locking device. The automatic locking control mechanism shall be operated by one hand, to determine whether there is free movement of the telescoping extension tube, and the automatic and positive locking in place of the tube at the point of adjustment desired. The telescoping tube shall be run through its maximum travel a minimum of five times. A five pound weight shall be suspended from one end of the cross during this test.

4.4.4 Load test. The telescoping tubing shall first be extended to the maximum height. The crossbeam elevated height measurement shall be taken prior to the weights being hung in the notched portions of the crossbeam. Two 5 pound weights shall each be hung simultaneously on the crossbeam and allowed to remain in place for 1 hour. At end of the 1 hour period, the crossbeam elevated height measurement shall be repeated to determine if slippage has occurred.

4.5 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of section 5. Defects shall be scored as specified in Table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery, the lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE III. Examination of Preparation for Delivery

Examination	Defect
Containers	Not as specified.
Contents not as specified	Quantity in interior packages and shipping containers not as specified.
Packaging and packing materials	Any component missing or damaged.
Workmanship	Bulging or distortion of containers. Cushioning or fittings inadequate or improper.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

4.5.1 Examination of closure, waterproofing and banding of containers. When shipping containers are required to comply with PPP-B-601, PPP-B-621 or PPP-B-640, examination for defects in closure, waterproofing and banding shall be in accordance with the appendix of the appropriate specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A, B or C as specified (see 6.1).

5.1.1 Unit package.

5.1.1.1 Level A. Each stand (disassembled as far as practicable) shall be packed in a box of appropriate size designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-640, class 2, style E. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure and strapping shall be in accordance with the appendix of the applicable box specification. A packing list and instructions for assembly shall be provided with the stand.

5.1.1.1.1 Case liner. Each level A box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard boxes shall be waterproof as specified in the appendix of PPP-B-640.

5.1.1.2 Level B. Each stand (disassembled as far as practicable) shall be packed in a box of appropriate size designed for a type 3 load and constructed in accordance with PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-640, class 1, style E. Box shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure shall be in accordance with the appendix of the applicable box specification. A packing list and instructions for assembly shall be provided with the stand.

5.1.1.3 Level C. Each stand shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, to point of delivery called for in the contract or purchase order.

5.2 Packing. No further packing is required.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.3 Unit package. Each unit package shall be marked as required for the exterior container specified in MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 20261O-26T12:11Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging (see 5.1).

6.2 The Deal Slide Lock manufactured by Deal Slide Lock Company, Box 292, Long Boat Key, Florida 33548, is acceptable for the locking device specified in 3.2.3.

6.3 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-791-6030	STAND, IRRIGATOR, Corrosion-Resisting Steel

6.4 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activity:

GSA-FSS

Preparing Activity:

DSA-DM

Project No. 6530-1342

Orders for this publication are to be placed with General Services Administration, acting as agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 35 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
RR-S-709B, STAND, IRRIGATOR

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:11Z
Check the source to verify that this is the current version before use.