GGG-M-125/5A
September 20, 1982
SUPERSEDING
GGG-M-125/5
March 28, 1975

FEDERAL SPECIFICATION

RESPIRATOR ASSEMBLY: HALF MASK, PARTICULATE-FILTER (FOR METAL FUMES, DUSTS AND MISTS)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

The complete requirements for procuring the respirators described herein shall consist of this document and the issue in effect of GGG-M-125/GEN.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers the requirements for a half-mask respirator with air filters for removing dust, metal fumes, or mists from respirable air.

1.2 Classification. Half-mask respirators covered by this specification shall be of the following types as specified (see 6.2):

Type I - Half-mask respirator, with provisions to replace the air-purifying element(s) (reusable).
Type II - Half-mask respirator where the air-purifying element(s) is/are not intended to be replaceable (disposable).

2. APPLICABLE DOCUMENTS

Latest issue of GGG-M-125/GEN and documents referenced therein and the additional documents specified herein.

3. REQUIREMENTS

3.1 Approval and certification. (See GGG-M-125/GEN).

3.2 Design. Respirator masks shall be of a design that covers the mouth and nose, leaving the eyes uncovered. The design shall allow respirable air to pass through the filter with minimum resistance to breathing when worn. Type I mask (see figure 1) shall have provisions for allowing one or two filters to be attached to the facepiece. Type II mask (see figure 2) shall be a completely disposable item, that is discarded after use. Both types shall permit the wearer to have unobstructed and good downward vision even when protective spectacles or eyeglasses are worn. The design shall provide a gas-tight seal with the face, when worn.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:37Z
Check the source to verify that this is the current version before use.

3.3 Principal parts. Respirators shall consist of the following parts where required:

a. Half-mask facepiece.
b. Head harness (see 3.3.1).
c. Exhalation valve or valves (see 3.3.2).
d. Inhalation valve or valves (see 3.3.3).
e. Filter(s) or filter cartridge(s) (see 3.3.4).

3.3.1 Head harness. The head harness shall be of the type supplied on the respirator when certified by the NIOSH/MSHA.

3.3.2 Exhalation valve. The exhalation valve or valves shall be securely mounted on the facepiece, and shall be so designed as to permit passage of the exhaled air and prevent entrance of air to the mask during inhalation.

3.3.3 Inhalation valve. The inhalation valve or valves shall be securely mounted on the facepiece, and shall be so designed to permit the entry of inhaled air into the mask through the filter with no outward leakage during exhalation.

3.3.4 Filters. The filters shall provide protection against concentrations of metal, dusts, fumes, and mist contaminants specified in 30 CFR, part 11.

3.3.4.1 Filters for type I respirator. Unless otherwise specified (see 6.2), 50 filters shall be furnished with each type I respirator having a single receptacle mask, and 100 filters shall be furnished with each type I respirator having a dual mask.

3.4 Interchangeability. Requirements in accordance with GGG-M-125/GEN.

3.5 Instructions. Requirements in accordance with GGG-M-125/GEN.

3.6 Marking. Requirements in accordance with GGG-M-125/GEN.

3.7 Workmanship. Requirements in accordance with GGG-M-125/GEN.

3.8 Sanitization. Type I shall conform to the requirement for masks specified in GGG-M-125/GEN.

4. QUALITY ASSURANCE PROVISIONS

4.1 Quality assurance provisions shall be in accordance with the requirements of GGG-M-125/GEN and the additional requirements specified herein.

4.2 Examination. Respirator samples selected in accordance with GGG-M-125/GEN shall be examined for the defects listed in table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

TABLE I. Classification of defects.

Categories	Defects
Major:	
101	Type not as specified.
102	Respirator not in accordance with NIOSH/MSHA requirements.
103	Principal parts missing.
104	Quantity of extra filters for type I not as specified.
105	Instructions missing.
106	Markings not as specified.
107	Material not new.
108	Poor workmanship.

4.3 Tests. Respirator assemblies sampled in accordance with GGG-M-125/GEN shall be subjected to the following test:

a. Cleaning and sanitization test type I only (see GGG-M-125/GEN).

5. PREPARATION FOR DELIVERY (In accordance with GGG-M-125/GEN).

6. NOTES

6.1 Intended use. Half-mask respirators covered by this specification are intended to give protection to the respiratory organs of the wearer from dusts, mists, and metal fumes that are not immediately dangerous to life or health. Component parts of respirators are not interchangeable between manufacturers nor are they always interchangeable on different models produced by the same manufacturer.

6.2 Ordering data. Purchasers shall select the preferred options offered herein and include the following data in procurement documents:

a. Title, number, and date of this specification.
b. Type required (see 1.2).
c. If different quantity of filters is required (see 3.3.4.1).
d. Level of packaging and level of packing required (see GGG-M-125/GEN).

6.3 Cross reference of classifications. The following respirators were previously classified as indicated:

New	Old
GGG-M-125/5A Type I	GGG-M-125/5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

MILITARY INTEREST:

Custodians

Army - EA
Navy - YD
Air Force - 99

Review Activities

Army - MD, ME
DLA - GS

User Activities

Navy - SH, CG, MC

CIVIL AGENCY COORDINATING ACTIVITY:

GSA - FSS
TVA -
DCG


PREPARING ACTIVITY:

Navy - YD


Project No. 4240-0445

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

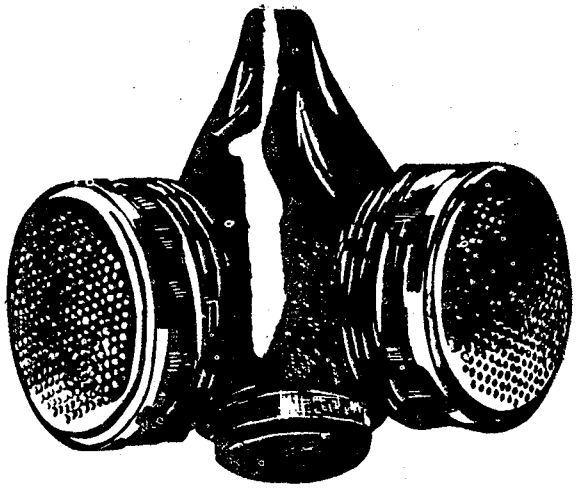

Dual filter half-mask respirator.

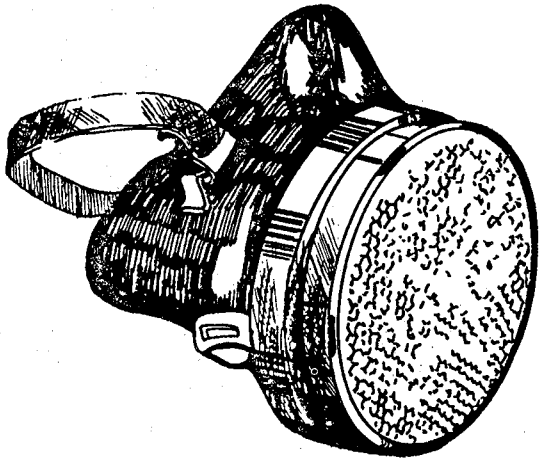

Single filter half-mask respirator.

Figure 1. Type I metal fumes, dusts, and mists half-mask respirator assemblies.
(For illustrative purposes only.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.

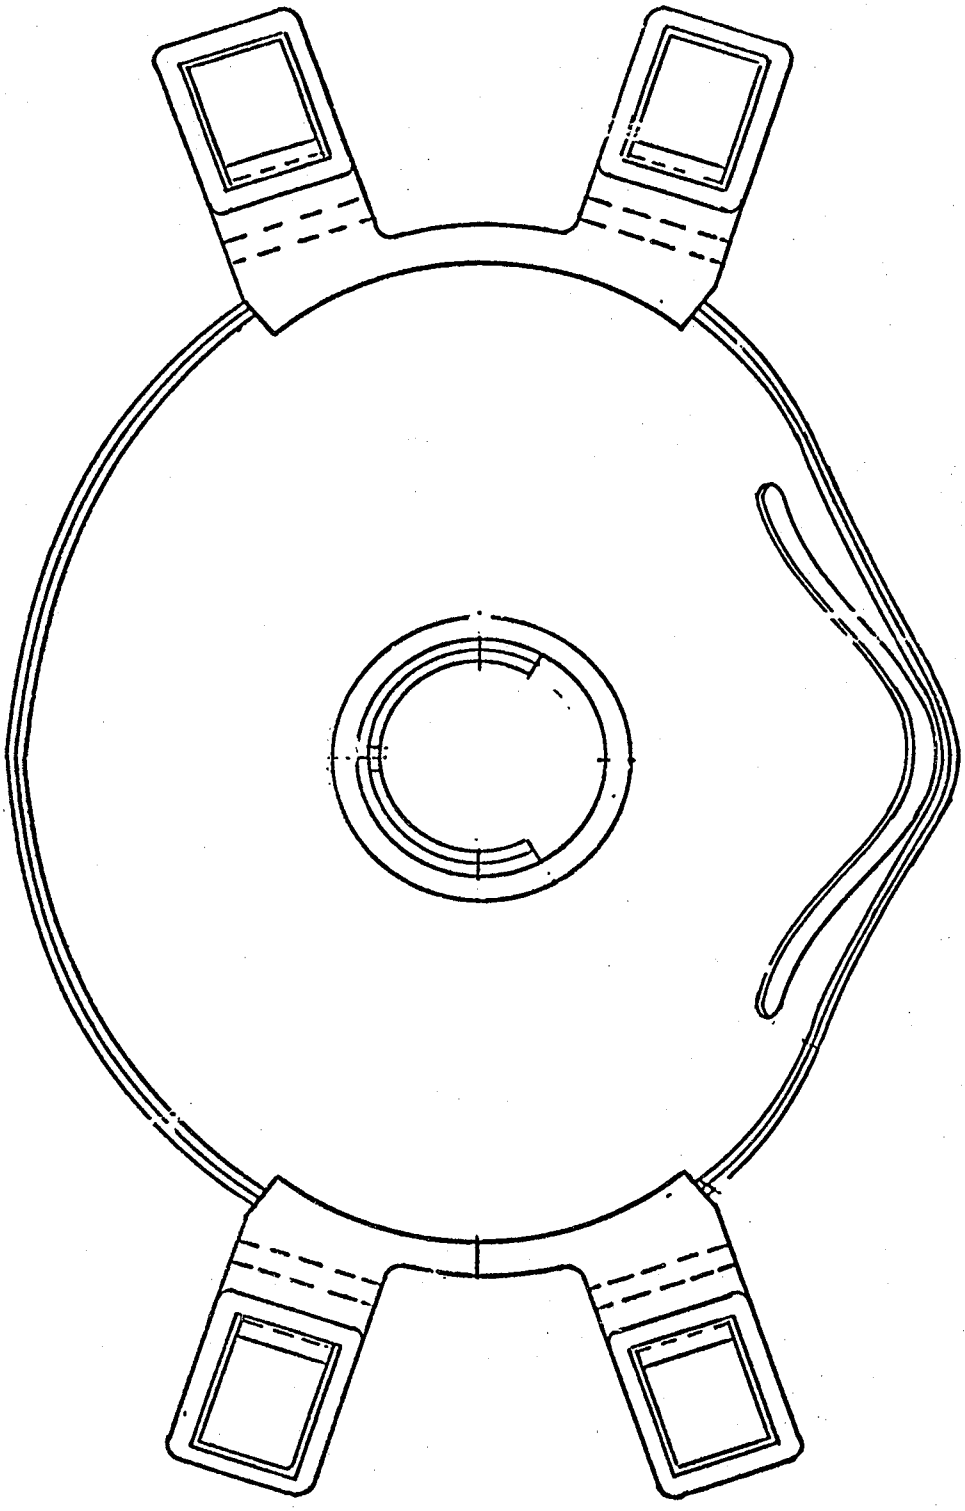


Figure 2. Type II metal fumes, dusts, and mists half-mask respirator assembly.
(For illustrative purposes only.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:37Z
Check the source to verify that this is the current version before use.