GG-C-1969A
November 14, 1977
SUPERSEDING
GG-C-1969
January 15, 1976

PROPOSED FEDERAL SPECIFICATION

CURETTE, MASTOID, SPRATT

This specification was approved by the Commissioner, Federal Supply Services, General Services Administration for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. Mastoid curettes covered by this specification shall be of the Spratt design suitable for the removal of diseased cells of the Mastoid.

1.2 Classification.

1.2.1 Sizes. Mastoid curettes covered by this specification shall be of the following sizes as specified (see 6.2):

Size 00
Size 1
Size 2
Size 3
Size 5
Size 6

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

GG-I-526	- Instruments, Dental and Surgical; General Specification.
PPP-B-566	- Boxes, Folding, Paperboard.
PPP-B-585	- Boxes, Wood, Wirebound.
PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

(10) Any exposed or accessible edge, corner, or surface not free of

Federal Specifications:

PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Set-up.

QQ-B-626 - Brass, Leaded and Non-Leaded: Rod, Shapes, Forgings, and Flat Products with Finished Edges (Bar, Flat Wire, and Strip).

Federal Standards:

Fed. Std. No. 66 - Steel: Chemical Composition and Hardenability.
Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).
Fed. Std. No. 151 - Metals, Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-P-116 - Preservation-Packaging, Methods of.
MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

(Copies of Military Specifications, Standards, and Publications required by suppliers in connection with specific procurement functions should be botained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

Uniform Classification Committee, Agent:

Uniform Freight Classification.

(Application for copies should be addressed to the Uniform Classification Committee, Room 1106, 222 South Riverside Plaza, Chicago, IL 60606.)

National Motor Freight Traffic Classification, Inc., Agent:

National Motor Freight Classification.

(Application for copies should be addressed to the American Trucking Association, Inc., ATTN: Tariff Department, 1616 P Street, N.W., Washington, DC 20036.)

American Society for Testing and Materials (ASTM) Standards:

E-10 - Brinell Hardness of Metallic Materials.
E-18 - Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials.
E-92 - Vickers Hardness of Metallic Materials, Test for.
E-140 - Standard Hardness Conversion Tables for Metals.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

American Iron and Steel Institute (AISI):

Steel Products Manual.

(Application for copies should be addressed to the American Iron and Steel Institute, 1000 16th Street, N.W., Washington, DC 20036.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 General requirements. The individual part requirements shall be as specified herein and in accordance with the applicable requirements of GG-I-526. In the event of any conflict between the requirements of GG-I-526 and those of this specification, the latter shall govern.

3.2 Materials.

3.2.1 Metal parts. All metal parts shall be as specified in table I and in accordance with the requirements of GG-I-526. They shall be of a corrosion resistant material or treated in a manner to render them adequately resistant to corrosion.

TABLE I. Materials.

Component	Material	Type	Class	Applicable Specification	Hardness
Blade and Shank	Steel, Stainless	420 1/	4	GG-I-526	C50-55 5/
	Steel, Stainless	420 1/	4		
Handle	Steel, Stainless	302 2/	3		B75 min
	Steel, Stainless	304 2/	3		
	Steel, Stainless	420	4		
	Brass, Cartridge (70%)	260	8		4/
	Brass, Yellow (65%)	270	8		
	Brass (free cutting)	280	8		
	Brass (composition 21)	-	3/	QQ-B-626	

1/ Carbon content may be 0.30% minimum.
2/ Chromium content may be 17.00 - 20.00%.
3/ Complying with plating and corrosion test requirements for Class 8, type 260, 270 or 280 of GG-I-526.
4/ Natural hardness.
5/ As an alternate German stainless steel WS 3021 (carbon content 0.17% to 0.22%) with hardness of R_C 45 min.


3.3 Design and construction. The instrument shall be a mastoid curette of the Spratt design, having an overall nominal length of 7 inches. It shall be designed with an oval shaped spoon having a sharp edge, a rigid straight shank and hollow handle securely attached to the shank.

3.3.1 Dimensions and configuration. The configuration and dimensions of the instrument shall be in accordance with figure 1.

3.3.2 Hardness.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

Contact resistance:

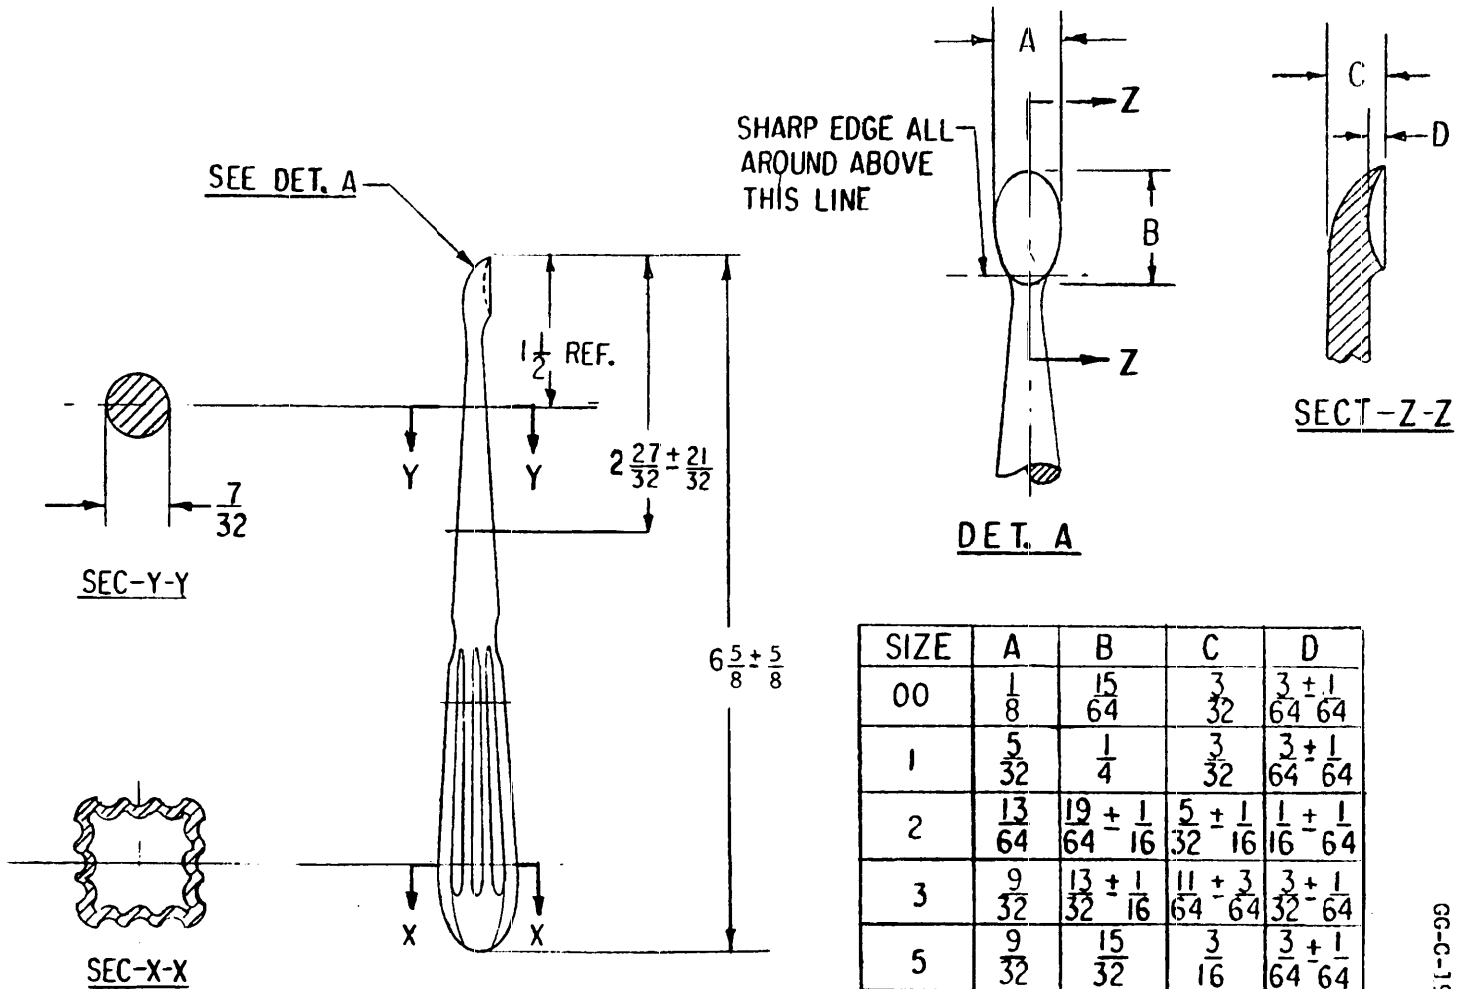

SIZE	A	B	C	D
00	1/8	15/64	3/32	3/64 ± 1/64
1	5/32	1/4	3/32	3/64 ± 1/64
2	13/64	19/64 ± 1/16	5/32 ± 1/16	1/16 ± 1/64
3	9/32	13/32 ± 1/16	11/64 ± 3/64	3/32 ± 1/64
5	9/32	15/32	3/16	3/64 ± 1/64
6	3/8	17/32 ± 1/16	7/32 ± 1/16	7/64 ± 3/64

NOTE:
1. Unless otherwise specified all dimensions are in inches..
2. Unless otherwise specified all dimensions are nominal.

FIGURE 1. Curette; mastoid, Spratt

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T11:54Z
Check the source to verify that this is the current version before use.

3.3.2.1 Blade and shank. After proper stress relieving the hardness of the finished instrument's blade and shank shall be in accordance with the requirement of table I (see 3.2.1) when tested as specified in 4.5.1.

3.3.2.2 Handle. After proper stress relieving the hardness of the finished instrument's handle, fabricated from AISI Type 300 or Type 400 material, shall be in accordance with the requirement of table I (see 3.2.1) when tested as specified in 4.5.1. Handles fabricated of nonferrous materials shall be of adequate hardness for the function intended.

3.3.3 Corrosion resistance. The instrument shall be corrosion resistant conforming with the requirements of GG-I-526 when tested in accordance with the applicable test specified in 4.5.2.

3.4 Finish. The blade and shank of the completed instrument shall have a mirror finish. The handle shall have a mirror or satin finish. The finish shall be in accordance with the requirements specified in GG-I-526. There shall be no crevice or space at the joint between the shank and handle which may collect foreign material or be subject to corrosion.

3.5 Passivation. As a final finish operation the complete instrument shall be passivated.

3.6 Identification marking. Identification marking of finished instruments shall be in accordance with GG-I-526. In addition, instruments of other than United States origin shall also be marked "stainless".

3.7 Workmanship. Workmanship shall be first class throughout. The instrument shall be processed in such a manner as to be uniform in quality and shall be free from surface roughness, burrs, pits, scale, corrosion, or any other defect that will affect life, serviceability or appearance.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the metals may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number, (NSN) the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Inspection lot. The inspection lot shall be determined in accordance with MIL-STD-105.

4.2.2 Preparation for delivery. The inspection lot size shall be expressed in units of one fully prepared shipping container, containing complete instruments fully prepared for delivery and made from essentially the same materials and components. The sample unit shall be one fully prepared shipping container, containing instruments fully prepared for delivey, with the exception that it need not be sealed. The inspection shall be Inspection Level S-2 and the Acceptable Quality Level shall be 4.0 percent defective in accordance with MIL-STD-105.

4.2.3 Sampling for visual and dimensional examination. A random sample of instruments shall be selected from each lot offered to the Government in accordance with MIL-STD-105. The Acceptable Quality Levels (AQL's) shall be as indicated in table II. The unit of product shall be one instrument.

TABLE II. Sampling for examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor A	S-2	4.0
Minor B	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

4.2.4 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table III. Where feasible, the same sample shall be used for the determination of two or more test characteristics. Unless otherwise specified, the unit of product for tests shall be one instrument.

TABLE III. Sampling criteria for tests

Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Hardness	3.3.2	445.1	S-1	1.0
Corrosion resistance	3.3.3	4.5.2.1, 4.5.2.2, & 4.5.2.3	S-2	1.5

4.2.5 Raw materials. A sufficient amount from each lot of each metal used in the construction of the curette shall be selected for chemical analysis.

4.3 Examination for visual and dimensional defects. The instrument shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables II and IV. Examination, however, shall not be restricted to defects listed in table IV. Any instrument in the sample containing one or more defects shall be rejected and if the number of defective instruments in any sample exceeds the acceptance number for that sample, the lot represented by that sample shall be rejected.

TABLE IV. Classification of defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Instrument not constructed as specified.
103	Instrument not free of rough areas, burrs, cracks, marks or overlaps.
104	Operative end not sharp as specified.
Minor A	
201	Physical dimensions not as specified.
Minor B	
251	Identification marking not present, correct, complete or legible.
252	Finish not as specified.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:54Z
Check the source to verify that this is the currentversion before use.

4.4 Examination of preparation for delivery. Each of the fully prepared shipping containers, containing instruments, selected as a sample unit from the lot shall be visually examined to determine whether the packaging, packing and marking conform to this specification. The classification of defects, table IV, shall be used to classify the defects found.

TABLE IV. Examination for preparation for delivery.

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and packing materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper location, sequence, or method of application.

4.4.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-585, PPP-B-601, PPP-B-621, or PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5.1 Hardness. Unless otherwise specified in 3.3.2, hardness shall be determined in accordance with ASTM test method E-10, E-18 or E-92. Hardness values shall be converted to Rockwell scale using tables of ASTM E-140. A minimum of 5 hardness readings shall be made on test specimens representative of the material used in the fabrication of the instrument or on the finished instrument.

4.5.2 Corrosion tests.

4.5.2.1 Boil test. The instrument shall be subjected to the boil test as specified in GG-I-526.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:54Z
Check the source to verify that this is the currentversion before use.

4.5.2.2 Copper sulfate test. Instruments fabricated entirely of AISI Type 400 material shall be subjected to the copper sulfate test as specified in GG-I-526. Instruments having the handle fabricated of nonferrous metals and the remainder of the instrument of corrosion resistant steel shall subject only the blade and shank to the copper sulfate test.

4.5.2.3 Salt-spray test. Instruments having the handle fabricated of nonferrous metals and the remainder of the instrument of corrosion resistant steel shall subject only the handle to the salt-spray test as specified in GG-I-526. At the option of the contractor the entire instrument may be tested.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Unit package. Each curette shall be thoroughly clean, wrapped in neutral tissue or other suitable anti-corrosive material. Each curette shall be packaged in accordance with MIL-P-116, method IC-2 except that a preservative shall not be used.

5.1.1.2 Intermediate package. Six unit packages containing curettes of one size only shall be packaged in a snug fitting box constructed in accordance with PPP-B-566, PPP-B-676, or PPP-B-636, type CF, class domestic. Closure of the box shall be as specified in the appendix of the applicable box specification.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty eight intermediate packages (288 units), containing curettes of one size only, shall be packaged in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585 Class 3, style 3; PPP-B-601 overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraph of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof as specified in the appendix of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:54Z
Check the source to verify that this is the currentversion before use.

5.2.2 Level B. Forty eight intermediate packages (288 units), containing curettes of one size only, shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636; type CF, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. The packages and shipping containers shall be marked in accordance with Fed. Std.No. 123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Curettes of the Spratt design are to be used for removal of diseased cells of the mastoid.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Size (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) Applicable National Stock Number (NSN)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

6.3 National Stock Number (NSN) coverage. This specification covers the following items listed in the Federal Supply Catalog.

National Stock Number	Item Identification	Size
6515-00-322-5400	CURETTE, MASTOID, Spratt	00
6515-00-322-5500	CURETTE, MASTOID, Spratt	1
6515-00-322-5550	CURETTE, MASTOID, Spratt	2
6515-00-322-5600	CURETTE, MASTOID, Spratt	3
6515-00-322-5700	CURETTE, MASTOID, Spratt	5
6515-00-322-5750	CURETTE, MASTOID, Spratt	6

6.4 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

6.5 Military requirements. Military requirements shall apply to all instruments purchased by military agencies. Where applicable, military requirements shall be in addition to all other requirements.

Military Custodians:

Army - MD
Navy - MS
Air Force - 03

Review activity:

DOD - MB

Preparing activity:
DLA-DM

Civil Agency Coordinating Activities:
GSA-FSS
HEW-FDA
HEW-HSM

Project No. 6515-2046

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents reference herein. Price 90 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:54Z
Check the source to verify that this is the currentversion before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

GG-C-1969A - CURETTE, MASTOID, SPRATT

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

GPO 1974— 603-680/ 6126 2-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:54Z
Check the source to verify that this is the current version before use.