
FED. SUP CLASS
6640

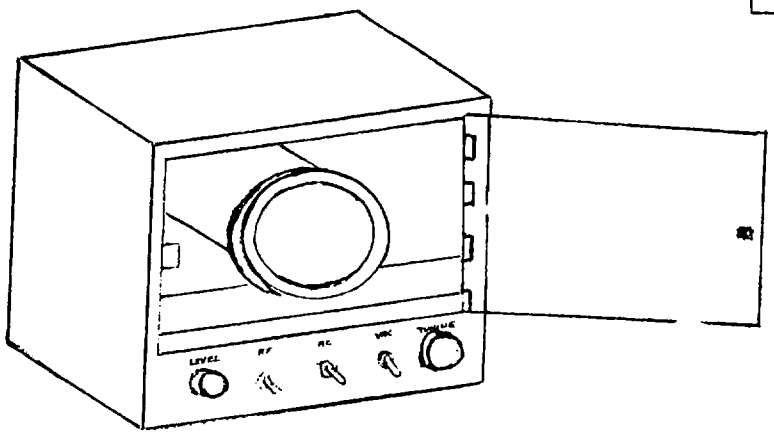

PART NUMBER	NUMBER OF CHAMBERS	OUTPUT WATTAGE
MS36283-1	1	0-100
MS36283-2	2	100-300
MS36283-3	4	100-500

MATERIAL: The chamber shall be borosilicate glass in accordance with Federal Specification, DD-G-541, type 1 class A. All other materials shall be suitable for construction that will enable proper function and strength.

DESIGN: The asher shall consist of the number of glass chambers as specified in the table. They shall be sealed by means of a silicone gasket when a vacuum of 0.8-1.5 mm Hg pressure is applied. Commercial grade oxygen at the rate of 150-200 cc/min shall be supplied to the chamber. A radio frequency of 13.56 mHz, crystal controlled as assigned by FCC regulations shall be provided by having electrodes or coils around the chamber. A R.F. tuning variable capacitor shall be provided to maintain minimum reflected power. Also, an interlocking RF power supply and AC cutoff switch shall be provided for safety when door is opened. The equipment shall conform to all the requirements of the Underwriters Laboratories, Code Number UL1262.

NOTE: Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

APPROVED 5 JAN 1983 REVISED

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 03

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
EA		ASHER, LOW TEMPERATURE, RADIO FREQUENCY	MS36283
Other Cust MS 99			
Procurement Specifications NONE	SUPERSEDES:		SHEET 1 OF 1

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1132

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:37Z
Check the source to verify that this is the current version before use.