MIL-B-37036A
30 December 1985
SUPERSEDING
MIL-B-37036
3 April 1974

MILITARY SPECIFICATION

BUR, DENTAL, FINISHING (Tungsten Carbide)

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers tungsten carbide finishing burs suitable for use with friction grip angle handpieces in finishing dental restorations.

1.2 Classification. Dental finishing tungsten carbide burs shall be of the following shapes and size numbers as specified (see 6.1):

Round
- Size No. 7002
- Size No. 7004
- Size No. 7008

Flame
- Size No. 7106

Cone
- Size No. 7204
- Size No. 7206

Inverted Cone
- Size No. 7304

Egg
- Size No. 7406

Tapered
- Size No. 7702

Bullet
- Size No. 7801
- Size No. 7803

Needle
- Size No. 7901
- Size No. 7902

Fine Ball
- Size No. 9004

AMSC N/A

FSC 6520

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue by the Department of Defense Index of Specifications and Standards (DoDISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-P-116	Preservation, Methods of

STANDARDS

Federal

FED-STD-151	Metal, Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.
MIL-STD-147	Palletized Unit Loads.
MIL-STD-794	Parts and Equipment, Procedures for Packaging of.

(Copies of specifications and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.)

2.2 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material.

3.1.1 Tungsten carbide. Bur shall be made of two-piece construction. The bur head shall be fabricated from a solid piece of cemented tungsten carbide with cobalt binder. Titanium or tantalum carbide, or both, may be added to achieve the required properties. The shank shall be made of steel as specified in 3.1.2.

3.1.2 Steel. The shank, neck and the base of the bur shall be fabricated from AISI-S5 tool steel or suitable stainless steel.

3.2 Figures. The figures forming a part of this specification are specification control figures. The supplier shall be responsible for preparing his own shop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide a product with dimensions within the tolerances prescribed on the drawing to insure proper design, and function, fit, assembly or operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.


3.3 Bur shape and dimensions.

3.3.1 Bur shank and overall length of bur. The bur shank shall be as shown in Figure 1. The bur shank and overall length of bur shall be in accordance with the dimensional requirements shown in Table I for the shape specified.

TABLE I. Length of shank and overall length of bur.

Shape	Length of shank (inch)	Overall length of bur (inch)
Round	0.433 - 0.536	0.755 ± 0.035
Flame	0.432 - 0.511	0.755 ± 0.035
Cone	0.433 - 0.511	0.787 ± 0.035
Inverted Taper	0.432 - 0.511	0.787 ± 0.035
Egg	0.432 - 0.511	0.755 ± 0.035
Tapered	0.433 - 0.511	0.787 ± 0.035
Bullet	0.433 - 0.511	0.755 ± 0.035
Needle	0.432 - 0.511	0.755 ± 0.035
Fine Ball	0.433 - 0.511	0.748 ± 0.020

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

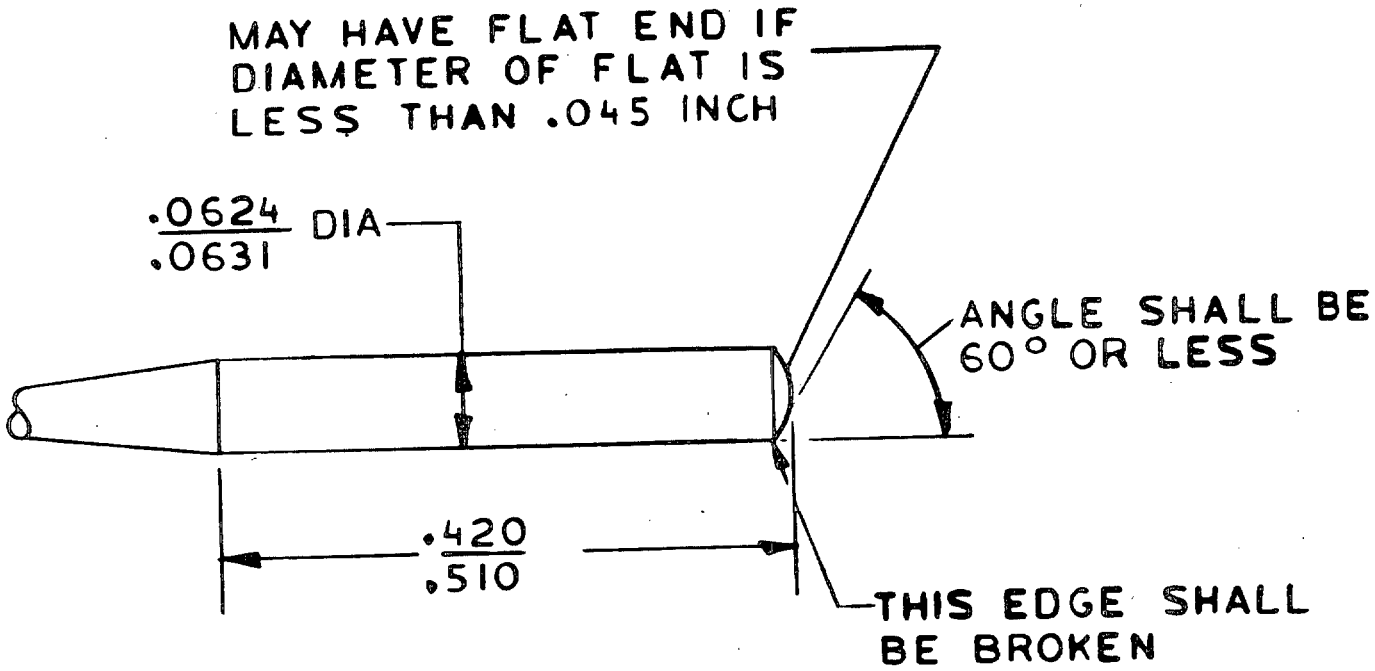

DIMENSIONS ARE IN INCHES.

FIGURE 1.

SHAPE AND DIMENSIONS OF BUR SHANK

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

3.3.2 Bur head and neck. The bur head shall be as shown in Figure 2 for the indicated shape. The bur head and neck shall be in accordance with the dimensional requirements shown in Table II for the shape specified.

TABLE II. Head and neck dimensions.


Shape	Size No.	Head diameter at largest place, ± 0.003 inch	Minimum length of head, inch	Maximum diameter of neck at head end, inch
Round	7002	0.039	0.026	0.030
Round	7004	0.055	0.032	0.036
Round	7008	0.091	0.063	0.052
Flame	7106	0.071	0.135	0.057
Cone	7204	0.055	0.335	SEE NOTE
Cone	7206	0.071	0.335	SEE NOTE
Inverted cone	7304	0.055	0.161	0.040
Egg	7406	0.071	0.130	0.057
Tapered	7702	0.040	0.193	0.040
Bullet	7801	0.035	0.100	0.035
Bullet	7803	0.048	0.110	0.048
Needle	7901	0.036	0.126	0.035
Needle	7902	0.040	0.130	0.040
Fine Ball	9004	0.055	0.032	0.035

NOTE: Shape C does not have a neck.

The number of blades shall be 12 for all burs, except size number 9004 shall be 30 blades. For burs 7204 and 7206, the taper or cone angle shall be 8-16, and for bur 7702, it shall be 4-11 (the total for both sides of the angle).


3.4 Design and construction. The burs shall be dental finishing burs, suitable for use in friction grip angle handpieces in trimming and finishing dental restorations. Burs shall consist of a shank, a neck (except for shape C which does not have a neck), and a head. The blades shall be uniformly cut and sharpened. The burs shall be of two-piece construction. The joint of burs shall be permanently welded to the shank as herein specified (see 3.6). The welded joint shall be milled so that the resultant shape has the appearance of an integral head unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.




12 BLADES

CUTTING END
(TYPICAL)

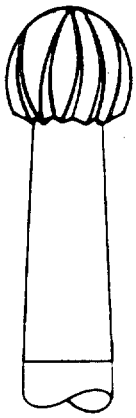


SHAPE A
ROUND



SHAPE B
FLAME




SHAPE C
CONE



SHAPE D
INVERTED TAPER




SHAPE E
EGG



SHAPE F
TAPERED



SHAPE G
BULLET



SHAPE H
NEEDLE

FIGURE 2 - SHAPE OF BUR HEADS

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

3.5 Runout . The total indicated runout of the bur shall not exceed 0.002 inch, when tested as specified in 4.4.2.

3.6 Strength of neck and joint . The neck shall not break on any of the burs, and the burs shall not fracture, when tested as specified in 4.4.3. The nondamaging test load shall be as specified in Table III for the applicable bur size number.

TABLE III. Strength requirements .

Bur size number	Nondamaging test load, pounds
7002	3.5
7004	6.5
7008	8.5
7106	6.5
7204	4.0
7206	6.0
7304	2.5
7406	6.5
7702	2.0
7801	3.0
7803	4.0
7901	2.0
7902	3.0
9004	6.5

3.6.1 Increase in runout. The increase in runout shall be no greater than 0.002 inch, when determined as specified in 4.4.3.3.

3.7 Finish. The bur head shall have a finely honed finish with sharpened blades. The neck and shank of the burs shall be smooth. The tool steel portion of two-piece burs shall be nickel or chromium plated. In addition, a flash of gold plate on shank shall be optional.

3.7.1 Autoclaving. The bur shall show no corrosion, after having been subjected to the autoclave test as specified in 4.4.4, except that corrosion present at the welded joint shall be disregarded, and shall not be cause for rejection.

3.7.2 Surface roughness. The surface roughness of the shanks of the burs shall be no more than the root-mean-square (RMS) average deviation of 20 microinches in the longitudinal direction of the shank, when determined as specified in 4.4.5.

3.8 Marking. Marking of the bur with the name or trademark shall be at the option of the supplier.

3.9 Workmanship. The burs shall be free from defects which may detract from their appearance or impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables IV and VI (see 4.2.1 and 4.3) and table V (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be as indicated in table IV. Unit of product for examination purposes shall be one package (10 burs).

Table IV. Sampling for Examination

Type defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified in Table V. The acceptance number shall be zero for all sample sizes. The unit of product for test purposes shall be one package (10 burs).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

Table V. Test criteria

Characteristic	Requirement	Test procedure	Inspection level
Chemical composition	3.1	4.4.1	(See 4.2.3)
Runout	3.5	4.4.2	S-3
Neck and joint strength	3.6	4.4.3	S-3
Increase in runout	3.6.1	4.4.3.3	S-3
Autoclaving	3.7.1	4.4.4	S-1
Surface roughness	3.7.2	4.4.5	S-1

4.2.3 Raw material. A sufficient quantity of each lot of raw material used in the manufacture of the burs shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same bur shall be used for the determination of two or more test characteristics.

4.3 Examination. The burs shall be examined for the possible defects listed in Table VI. The examination shall not be limited to those defects shown in the table. Unless otherwise indicated in the table, the defect listed shall apply to all shapes and size numbers of tungsten carbide, finishing burs covered by this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

Table VI. Classification of defects

Category	Defect
Major:	
101	Bur size number or head shape not as specified.
102	Bur shank not as specified.
103	Total indicated runout exceeds 0.002 inch.
104	Head diameter exceeds specification requirements at maximum cross-section.
105	Diameter of shank exceeds specification limits.
106	Length of head less than minimum requirement for applicable bur size number.
Minor:	
201	Cutoff end on shank not as shown in figure 1.
202	Burs not free from defects such as chipped blades, cracks, or pits.
203	Number of blades not as specified.
204	Finish on bur not as specified.
205	Overall length of bur not within specification limits.
206	Maximum neck diameter at head end exceeds specification limits.
207	Shank dimensions, other than those specified under major defects, not within specification limits.
208	Taper or cone angle of head (when applicable) not within specification limits.
209	Welded joint of two-piece bur does not give the appearance of an integral head unit.
210	Packaging and packing not as specified.
211	Marking on packaging or pack incorrect, illegible, incomplete, or missing altogether.

4.3.1 Dimensions. Examination of the dimensions, as listed in 3.3, shall be made with a toolmaker's microscope, or other instrument of equal accuracy. Manufacturer's gages may be used if properly calibrated checking standards are used in conjunction with them.

4.3.2 Microscopic examination. Examination of bur defects not readily perceptible to the naked eye shall be made using a microscope at 10 power (10X) magnification.

4.4 Test procedures.

4.4.1 Chemical composition. In the absence of certificates of quality for the raw material, the samples selected as specified in 4.2.3, shall be analyzed in accordance with Method 111 or 112 of FED-STD-151. In case of dispute, Method 111 shall be used for referee analysis. (Separate analyses shall be made on the carbide and the non-carbide portions of two-piece burs.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

4.4.2 Runout. The bur shall be placed and held in a "V" block or precision chuck, and rotated slowly. A dial indicator sensitive to 0.0002 inch and equipped with a knife-edge foot, or a shadow-graph or other suitable equipment of equal accuracy, shall be employed. If a dial indicator is used, the indicator shall be mounted with the shaft perpendicular to the axis of the bur, and so positioned that the foot contacts the bur neck at the point of smallest diameter. For shape C burs, the foot shall contact the shank at the point nearest the head. The maximum and minimum readings obtained during one complete 360-degree rotation of the bur shall be measured and recorded to the nearest 0.0005 inch. The difference between these two readings shall be taken as the total indicated runout.

4.4.3 Neck and joint strength.

4.4.3.1 Equipment for test. The equipment shall consist of a true-running chuck suitable for holding and rotating the test bur, and a loading device capable of applying the load indicated in Table III through an anvil with a flat surface at an angle of 22-1/2 ± 1/2 degrees to the bur axis. The chuck shall grip at least a 3/8 -inch portion of the bur shank starting at the intersection of the neck and shank.

4.4.3.2 Test procedure. Following an initial examination for total indicated runout as specified in 4.4.2, those burs which have been selected for the neck and joint strength test shall be rotated in the chuck to that position which shows the highest deflection reading on the dial indicator gage. A load of the magnitude specified in Table III shall be slowly applied at an angle to the bur axis of 22-1/2 ± 1/2 degrees, in the direction which tends to further increase the dial deflection reading. The neck and joint of the bur shall be observed for evidence of breakage. Should breakage not have occured at the point of maximum deflection, the load shall be removed and the examination for increase in runout determined as specified in 4.4.3.3.

4.4.3.3 Increase in runout. The increase in runout shall be determined only on those samples which have been subjected to the neck and joint strength, and shall be performed in the manner already specified in 4.4.2 for runout. The difference between the final and the initial indicated runout shall be taken as the increase in runout.

4.4.4 Autoclaving. The test burs shall be cleaned in accordance with the instructions supplied by the manufacturer. The burs shall then be autoclaved at 270 ± 5 degrees Fahrenheit (F.) and 27 ± 1 pounds per square inch pressure for a minimum of 20 minutes. After the burs are removed from the autoclave, the entire surface area of the non-carbide portion of the bur shall be examined for evidence of corrosion.

4.4.5 Surface roughness. The surface roughness of the bur shall be determined by using a Brush Surfindicator, or other equipment of equal accuracy. The RMS average shall be determined by squaring the height measurements of the peaks and valleys of the surface of the shank, obtaining the averages of the squared values, and then extracting the square root of this average square.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

4.5 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Cleaning. Burs shall be cleaned in accordance with MIL-P-116.

5.1.1.2 Drying. Burs shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative applications. Preservatives shall not be used.

5.1.1.4 Unit package. Ten burs of one shape and size only, shall be packaged in a plastic holder, so designed that each bur is contained in an individual cell. The plastic holder shall be designed with a clear plastic cover in order to prevent spilling of contents under normal handling. Each unit shall be further packaged in accordance with MIL-P-116, method IC-1. As an alternate, ten burs shall be packaged in one or more plastic holders and the holders sealed in a snug-fitting, polyethylene bag.

5.1.1.5 Intermediate package. Ten units containing burs of one shape and size only, shall be packed in a snug fitting box conforming to PPP-B-566, PPP-B-676 or a snug fitting plastic box having a partial telescope cover. Commercial colors are acceptable on intermediate containers. Closure shall be secured to prevent spilling of contents under normal handling. As an alternate, intermediate package shall be a snug-fitting, sealed, 3 mil, polyethylene bag.

5.1.2 Level C. The level C preservation for burs shall conform to MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.1).

5.2.1 Level A. One hundred intermediate packages containing burs of one shape and size only, shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure shall be as specified in the liner specification. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed as specified in PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

5.2.2 Level B. One hundred intermediate packages containing burs of one shape and size only, shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the box specification.

5.2.3 Level C. The level C packing for burs shall conform to MIL-STD-794 requirements for this level.

5.2.4 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Loads shall be unitized on pallets. Quantities less than 40 cubic feet need not be unitized. Unitized loads shall be uniform in size and quantities to the greatest extent practicable.

5.2.4.1 Levels A and B. Burs, packed as specified in 5.2.1 and 5.2.2, shall be unitized on pallets conforming to MIL-STD-147.

5.2.4.2 Level C. Burs, packed as specified in 5.2.3 shall be unitized as specified in MIL-STD-794.

5.3 Marking.

5.3.1 Levels A, B, and C. Each unit package, intermediate package, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.

6. NOTES

6.1 Ordering data.

6.1.1 Acquisition requirements. Acquisition documents should specify the following:

(a) Title, number, and date of this specification.
(b) Shape and size required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

6.2 Definitions.

(a) Shape. The shape of the bur shall indicate the geometric shape of the bur head.

(b) Size number. The size number of the bur shall indicate both the size and shape of the bur head. For any designated head shape an increase in the bur number shall indicate a larger head and a decrease shall indicate a smaller head.

6.3 National Stock Number coverage. The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification	Specification Shape	Designation Size No.
6520-01-098-5807	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7002, 10s	Round	7002
6520-01-098-5808	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten, Carbide, No. 7304, 10s	Inverted Cone	7304
6520-01-098-5809	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7406, 10s	Egg	7406
6520-01-098-5810	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7702, 10s	Tapered	7702
6520-01-098-5811	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7803, 10s	Bullet	7803
6520-01-098-5812	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7902, 10s	Needle	7902
6520-01-098-5813	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7106, 10s	Flame	7106

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

6520-01-098-5814	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7008, 10s	Round	7008
6520-01-098-5815	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7004, 10s	Round	7004
6520-01-098-5816	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7204, 10s	Cone	7204
6520-01-098-5817	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7206, 10s	Cone	7206
6520-01-099-0328	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7901, 10s	Needle	7901
6520-01-105-0429	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 7801, 10s	Bullet	7801
6520-01-105-0430	Bur, Dental, Finishing, Friction Grip Angle Handpiece, Tungsten Carbide, No. 9004, 10s	Fine Ball	9004

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:
VA-OSS

Project No. 6520-1800

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil/ - Downloaded: 2026-10-21T09:49Z
Check the source to verify that this is the current version before use.