MIL-C-37022A
30 September 1976
SUPERSEDING
MIL-C-37022 (DSA-DM)
10 December 1973

MILITARY SPECIFICATION

CENTRIFUGES, LABORATORY, FLOOR MODEL

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers two floor model centrifuges suitable for use in laboratory analysis.

1.2 Classification. Centrifuges shall be of the following sizes as specified:

Size 1 - 1/3 horsepower (hp.)
Size 2 - 3/4 hp.

2. APPLICABLE DOCUMENTS

2.1 Issue of documents. The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
CC-M-636	- Motors, Fractional Horsepower (Alternating Current).
PPP-B-636	- Boxes, Shipping Fiberboard.
PPP-B-1055	- Barrier Material, Waterproof, Flexible.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Hq, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document, or by letter.

FSC 6640

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-M-7298 - Manual, Technical: Commercial Equipment.

STANDARDS

FEDERAL

FED-STD-66 - Steel: Chemical Composition and Hardenability.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN NATIONAL STANDARDS INSTITUTE (ANSI)

ANSI C73-11 Dimensions of Plugs and Receptacles - General Purpose, 125 Volts, 15 Amperes, 2 Pole, 3-Wire, Grounding Type.

(Application for copies should be addressed to the American National Standards Institute, 1430 Broadway, New York, NY 10018.)

UNDERWRITERS' LABORATORIES, INC. (UL)

UL 73 Standards for Safety--Motor Operated Appliances.

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 1285 Walt Whitman Road, Melville, L.I., NY 11746; 207 East Ohio Street, Chicago, IL 60611; and 1655 Scott Boulevard, Santa Clara, CA 95050; 333 Pfingsten Road, Northbrook, IL 60062.)

OCCUPATIONAL SAFETY AND HEALTH ADMINISTRATION

Code of Federal Regulation, Title 29, part no. 1910, paragraph 1910.95, Occupational Noise Exposure.

(Application for copies should be addressed to the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.)

3. REQUIREMENTS

3.1 Fire and casualty hazards. The contractor must submit proof prior to delivery that the items to be delivered under the contract conform to the applicable requirements of UL 73. Proof shall consist of one of the following:

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:48Z
Check the source to verify that this is the currentversion before use.

a. UL label or UL listing of the product provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the contracting officer, upon the latter's request.

b. Laboratory report from a qualified independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with UL standards. The qualification of such laboratory shall be determined by the Government which reserves the right to require a facilities report and to conduct a facilities survey. Any laboratory report submitted shall include actual test methods, data taken, and results of tests. Detailed findings of examinations necessary to determine compliance shall also be included. The test report shall also have a section that describes the test sample in such a way that the report can be used to insure identity of production items with the test sample. This section shall be supplemented with construction information such as materials used, spacings between electrical components, types of bushings, photographs, wiring diagrams, sketches, and parts list, all appropriately identified.

3.1.1 Compliance with above paragraph does not excuse compliance with all other requirements of the contract and specifications.

3.2 Material. Material shall be as specified herein. When material is not specified, it shall be of a quality which meets the functional requirements of the centrifuge.

3.3 Construction. The centrifuge shall consist of a guard bowl, a cover, a motor, a speed control device, a tachometer and a timer. Size 1 shall be in accordance with Figure 1; Size 2 shall be in accordance with Figures 1 or 2. For centrifuge in Figure 1, guard bowl and motor shall be enclosed in a metal cabinet. For centrifuge in Figure 2, guard bowl shall be supported by a base. This base shall contain the motor. Cabinet and base shall be sufficiently strong to support the applicable centrifuge components without buckling or other deformation. Vibration dampeners shall be placed between the guard bowl and the motor, the guard bowl and the cabinet, and the guard bowl and the base.

3.3.1 Guard bowl. For purposes of this specification, the guard bowl is the chamber which houses the drive spindle and head, trunnions and shields. The walls of the guard bowl shall be constructed of sheet steel. For Figure 1, thickness of guard bowl walls shall be 1/16-inch thick. For Figure 2, thickness of guard bowl walls shall be 3/16-inch thick. Commercial tolerances shall apply to thickness of sheet steel. Top view of the guard bowl shall be circular. Inner circumferences of the lower portions of the bowl shall be such that they provide a chamber large enough for operation, in place, of the centrifuge with head, trunnions, and other accessories listed in 3.8.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

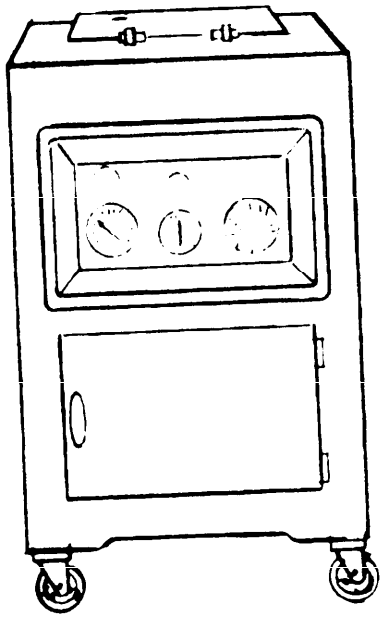


FIGURE 1

FOR REFERENCE PURPOSES

Variation in design is acceptable provided item meets detailed specification requirements.

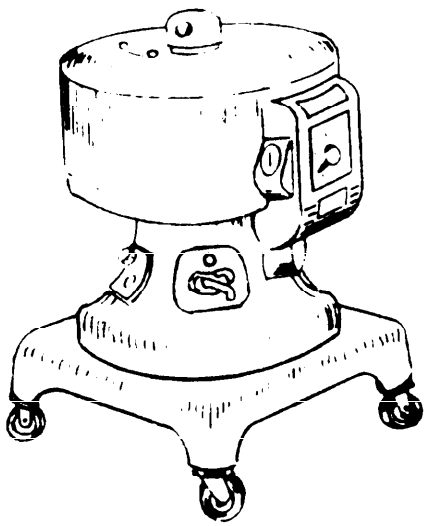


FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

3.3.1.1 Inner diameter of Size 1. Inner diameter at the top of the guard bowl for Size 1 shall be not less than 14-1/4 in.

3.3.1.2 Inner diameter of Size 2. Inner diameter at the top of the guard bowl for Size 1 shall be not less than 15-3/4 in.

3.3.2 Cover. Cover shall be located at the top of the guard bowl or at the top of the cabinet. Cover shall be fabricated of sheet steel which is 3/16 inch thick. Commercial tolerances shall apply to thickness of sheet steel. Cover shall be secured to the chamber or cabinet by means of a hinge and a positive and easy-operating lock. A rubber gasket shall be placed on the top of the cabinet or guard bowl so that the metal portion of the closure area does not touch the metal portion of the cabinet or chamber when the cover is closed.

3.3.3 Motor. Motor shall be a variable speed motor which operates on 115 volts, 50/60 Hz, AC. Motor shall be in balance when tested as specified in 4.4.1.

3.3.3.1 Size 1 hp. Rated power of Size 1 motor shall be not less than 1/3 hp.

3.3.3.2 Size 2 hp. Rated power of Size 2 motor shall be not less than 3/4 hp.

3.3.4 Drive spindle. The drive spindle shall be a vertically-mounted steel shaft. The top shall be designed so as to be capable of attaching the head. The drive spindle shall be of adequate size to support static and dynamic forces encountered in its operation. The drive spindle shall be an integral extension of the motor shaft, or a separate shaft mounted so that it is driven by the motor shaft.

3.3.5 Speed control device. The centrifuges shall be provided with a speed control device which shall be of the continuous auto-transformer type. Dial of the speed control device shall provide for not less than 50 steps of speed control and an "off" position. The device shall be legibly identified and located so as to be convenient to the operator.

3.3.6 Tachometer. Tachometer shall have a dial graduated in increments of 100 from 0 to 6000 revolutions per minute (r.p.m.). For centrifuge in accordance with Figure 1, tachometer shall be located on instrument panel; for centrifuge in accordance with Figure 2, tachometer shall be mounted on the cover.

3.3.7 Brake. The centrifuges shall be equipped with decelerator switch so that rapid deceleration may be accomplished as specified in 3.12.3.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:48Z
Check the source to verify that this is the currentversion before use.

3.3.8 Master switch. The centrifuges shall be provided with a conveniently located master (on-off) switch.

3.3.9 Safety cut-out relay. Centrifuges shall be provided with a low voltage cut-out relay which automatically shuts the motor off when the line voltage drops below 45 volts. Design of relay shall be such that the centrifuge will not reactivate until normal starting procedures are performed.

3.3.10 Timer. Shall be a two-hour timer with two-minute intervals. Timer shall be part of the electrical circuit of the centrifuge when timer switch is in the "on" position and shall automatically shut the centrifuge off when it is operated for any pre-set length of time within timer range. Centrifuge shall run for an indefinite rather than a pre-set time when timer switch is in the "off" position. Timer and switch shall be legibly identified and so located as to be convenient to the operator.

3.4 Dimensions. With the cover closed and the casters in place, overall dimensions shall be in inches as follows:

	Height	Width	Depth
Size 1	37 ± 3	20 ± 2	22 ± 3
Size 2	36 to 49	32 maximum	32 maximum

3.5 Cord and plug. The centrifuges shall have a three-wire electrical cord equipped with a grounding plug in accordance with ANSI C73-11. Cord shall be a flexible heavy-duty type and shall be at least five feet long externally.

3.6 Lubrication. If lubrication is required, oil cups and grease nipples shall be easily accessible; lubrication shall be accomplished without the use of special tools.

3.7 Casters. Centrifuge shall be equipped with four ball bearing swivel-type casters. Casters shall be located as shown in Figures 1 or 2. The total load-carrying capacity of the four casters shall be not less than double the net weight of the centrifuge. Caster wheel diameters shall be not less than 3 inches, and wheel tread widths shall be not less than 7/8-inch.

3.8 Accessories. Size 1 and Size 2 centrifuges shall be supplied with the following accessories which shall be interchangeable with all centrifuges procured under a specific contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

Quantity		Item
Size 1	Size 2	
1	-	8-place manganese bronze head
-	1	16-place manganese bronze head
24	48	10-ml. AISI 300 series 1/ corrosion-resisting steel or chromium-plated brass tubes with rubber cushions.
8	16	50-ml. AISI 300 series 1/ corrosion-resisting steel or chromium-plated brass tubes with rubber cushions.
8	16	Trunnion cups, aluminum, Babcock, with rubber pads.
8	16	Trunnion rings for 50-ml. tubes.
8	16	3-place manganese bronze trunnion carriers.
8	16	8-place multiple carriers, with rubber cushions and corrosion-resisting steel trunnions.
8	-	Aluminum reducing caps which hold 10-ml. glass tubes in 50-ml. tubes (shields).

1/ Conforming to FED-STD-66.

The heads shall be dynamically balanced. The trunnion rings, tubes, cups and carriers shall be weighed and matched to .5 gram with the gram weight stamped on each piece.

3.9 Finish. Outside finish shall be smooth or hammertone baked-on enamel. Color of enamel shall be gray or beige. Inside of guard bowl shall be finished with baked-on white epoxy enamel or shall be corrosion-resisting steel.

3.10 Service data. The contractor shall furnish with each unit three copies of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract, the contractor shall furnish to the contracting officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual, for review and comment by the Directorate of Medical Materiel (based on a maximum period of 30 days for such review) and allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract. In addition, the contractor shall furnish 15 copies of the approved technical manual to the contracting officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of contract and propose to furnish manuals identical with those previously accepted, the requirements for review of drafts and submission of 15 additional copies may be waived upon request by the contracting officer. Waiver of submission of 15 additional copies shall be at the option of the Government.

3.10.1 The data supplied shall include nomagraph or similar data for rapid conversions of revolutions per minute and known radii into relative centrifugal force (RCF).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

3.11 Center of gravity and net weight information. The contractor shall prepare a drawing, figure or illustration, indicating the position of the vertical center of gravity of the unit with reference to its base. The net weight of the unit shall also be indicated. Four copies shall be submitted by the contractor directly to the Chief, Technical Services Branch, Technical & Quality Assurance Division, Directorate of Medical Materiel, Attention. DPSC-ATTP, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, PA 19101. Drawings shall be submitted only on the initial contract. Drawings shall not be required on subsequent procurements unless the unit has been redesigned.

3.12 Performance.

3.12.1 Speed measurement. Tachometer reading shall be identical to stroboscope reading ± 120 revolutions per minute (r.p.m.) when tested as specified in 4.4.2.

3.12.2 Relative centrifugal force. Size 1 shall attain a force of at least 2100 gravities and a speed of 3100 r.p.m.; Size 2 shall attain a force of at least 1300 gravities when tested as specified in 4.4.3.

3.12.3 Braking time. Braking time from top speed to a complete stop shall be 15-30 seconds for Size 1, and 70-90 seconds for Size 2 when tested as specified in 4.4.4.

3.12.4 Temperature rise. The temperature of the water in the centrifuge tube shall not increase more than 17° Centigrade (C.) when tested as specified in 4.4.5.

3.12.5 Timer accuracy. Timer reading shall be identical to reading on test timer ± six minutes when tested as specified in 4.4.6.

3.12.6 Dielectric test. There shall be no electrical breakdown when the centrifuge is subjected to the test specified in 4.4.7.

3.12.7 Operations test. Centrifuge shall perform all functions specified herein and all functions indicated in service data when tested as specified in 4.4.8.

3.12.8 Sound level. At a distance of two feet from the centrifuge, sound level shall not exceed 90 dBA when tested as specified in 4.4.9.

3.12.9 Dynamic balance. Centrifuge shall not move or vibrate excessively when tested as specified in 4.4.3.

3.13 Nameplate. Centrifuge shall have a nameplate which is permanently attached and which is marked with the manufacturer's name, model or catalog number, voltage, type of current and watts input or amperage and operational speeds for which it is designed. The nameplate shall be of corrosion-resisting metal and shall include the national stock number, item identification, contract or purchase order number and serial number.

3.14 Workmanship. Workmanship shall be first class throughout. Centrifuges and accessories shall be free of defects indicated in Table III or other defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for insnection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificate of quality. Certificate of quality, supplied by the manufacturer of the corrosion-resisting steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and Table I.

Table I. For examination

	Inspection level	AQL (precent defective)
For visual examination Major defects	II	1.0
For dimensional and weight examination	S-1	2.5

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:48Z
Check the source to verify that this is the currentversion before use.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with Table II and MIL-STD-105. Acceptance number shall be zero, and inspection level shall be S-1, except for dielectric strength and operational tests. For dielectric strength and operational tests, each centrifuge shall be tested.

Table II. Sampling for tests.

Component	Characteristic	Requirement	Test procedure
Motor	Balance	3.3.3	4.4.1
Tachometer	Speed measurement	3.12.1	4.4.2
Centrifuge	Relative centrifugal force	3.12.2	4.4.3
Centrifuge	Braking time	3.12.3	4.4.4
Centrifuge	Temperature rise	3.12.4	4.4.5
Timer	Accuracy	3.12.5	4.4.6
Centrifuge	Dielectric strength	3.12.6	4.4.7
Centrifuge	Operations test	3.12.7	4.4.8

4.3 Examination. Centrifuge shall be examined to determine compliance with all requirements listed in this specification.

Table III. Classification of defects

Category	Defect
Major	
101	Component or accessory missing.
102	Component not secured.
103	Centrifuge or accessories not free of sharp edges and burrs.
104	Finish not free of chipping, cracking and peeling.
105	Centrifuge or accessories not free of rust spots.
106	Service data missing.
107	Numerals or other markings on components not complete, correct, legible and permanent.
108	Markings on nameplate not complete, correct, legible and permanent.
109	Nameplate not attached permanently.
110	Cover cannot be securely closed.

4.3.1 Dimensional examination. The centrifuge and accessories shall be examined for defects in dimensions and weight. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements. If appropriate, tests may be combined.

4.4.1 Balance. Motor shall be tested for balance in accordance with applicable portions of CC-M-636 (see 3.3.3).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

4.4.2 Speed measurement. Revolutions per minute of head shall be measured by a stroboscope of known accuracy. Tachometer shall be set at 2000 and 3000 r.p.m.

4.4.3 Relative centrifugal force. Head shall be filled with 50-ml. centrifuge tubes, 8 for Size 1 and 16 for Size 2. Centrifuge tubes shall be filled with water and shall be in shields; water and centrifuge shall be allowed to come to ambient temperature, and the temperature of the water shall be recorded (4.4.5). Speed shall be set at maximum, and centrifuge shall be activated in accordance with service date. Centrifuge shall be allowed to run at maximum speed for one half hour. Speed shall be measured by stroboscope of known accuracy, and relative centrifugal force at the tip of the 50-ml. tube shall be calculated in accordance with procedures in service data. Test should be run at 115 volts.

4.4.4 Braking time. With centrifuges running as indicated in 4.4.2, brake shall be applied in accordance with directions in service data. Time of braking, time that centrifuge head comes to a complete stop, and temperature of water (4.4.5) shall be recorded.

4.4.5 Temperature rise. Temperature of water shall be recorded as indicated in 4.4.3 and 4.4.4.

4.4.6 Timer reading. Accuracy of centrifuge timer shall be measured by a testing timer of known accuracy. Centrifuge timer shall be set at two hours.

4.4.7 Dielectric strength. Immediately after operation, a 60-cycle alternating potential of 1000 plus twice the rated voltage shall be applied for a period of one minute between the current-carrying parts and dead metal parts. Tests shall be conducted with a transformer which regulates the output voltage. Starting at zero voltage, the applied potential shall be increased gradually until the required test value is reached or breakdown occurs.

4.4.8 Operations test. Centrifuges shall be activated and run until all specified functions and all functions indicated in service data are performed.

4.4.9 Sound level. Sound level shall be determined as specified in CFR Title 29, paragraph 1910.95, Occupational Noise Exposure.

* 4.5 Packaging inspection. The inspection of the unit, intermediate package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

* 5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be Level A or C, as specified (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

5.1.1 Level A.

5.1.1.1 Unit preparation. Accessories shall be wrapped in kraft or tissue paper and packaged in boxes conforming to PPP-B-636, class domestic. The accessories shall be cushioned within the boxes in such a manner as to prevent shifting or damage. The finished exterior surfaces of the centrifuges shall be protected by wrapping with kraft paper or other suitable material.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.1).

5.2.1 Level A. Each unit, with accessories, shall be overboxed in an exterior container designed for a type 3 load and constructed in accordance with PPP-B-601, overseas type, or PPP-B-621, class 2. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, or other interior fittings to insure against shifting or breakage. The work shall be accomplished in such a manner that the weight of the unit shall not be carried directly by the casters. Each unit shall be protected by a shroud fabricated of waterproof barrier material conforming to PPP-B-1055, class H-1, H-5 or M-1. The exterior container design shall include three skids of not less than 1-1/2 inches in thickness, applied crosswise to the base, so positioned as to facilitate handling with a forklift truck and to maintain unit in an upright position. Closure and strapping shall comply with appendix of applicable specification.

5.2.2 Level B. Each unit shall be packed as specified in 5.2.1, except that the exterior containers shall conform to PPP-B-601 or PPP-B-621, class 1. In addition, waterproof shroud and strapping shall not be required.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract.

5.3 Marking.

5.3.1 Interior packages. Interior packages shall be marked to identify contents and quantity contained.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior containers. Exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

a. Title, number and date of this specification.
b. National Stock Number (NSN).
c. Size of centrifuge required (see 1.2).
d. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not cover all types, classes, grades or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types normally procured to meet requirements.

6.3 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6640- 0989

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS. The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-C-37022A CENTRIFUGES, LABORATORY, FLOOR MODEL

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:48Z
Check the source to verify that this is the current version before use.