MILITARY SPECIFICATION

DILATOR SET, LACHRYMAL, NETTLESHIP-WILDER, SET OF 3

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a set of three lachrymal dilators, Nettleship-Wilder design, suitable for progressive dilation of the lachrymal duct.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical, General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case and Sheet, Overwrap; Watervaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The dilator set shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The dilators shall be fabricated from Class 3, type 304 material.

3.3 Hardness. After proper stress relieving, the Rockwell hardness of the dilators shall be B-75 to B-85.

3.4 Style, design and dimensions. The style, design, and dimensions of the dilator set shall be in accordance with Figure 1.

3.5 Finish. Operative end shall be mirror, remainder mirror or satin.


3.6 Identification marking. In addition to GG-I-526 requirements, dilator sets of foreign manufacture shall also be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

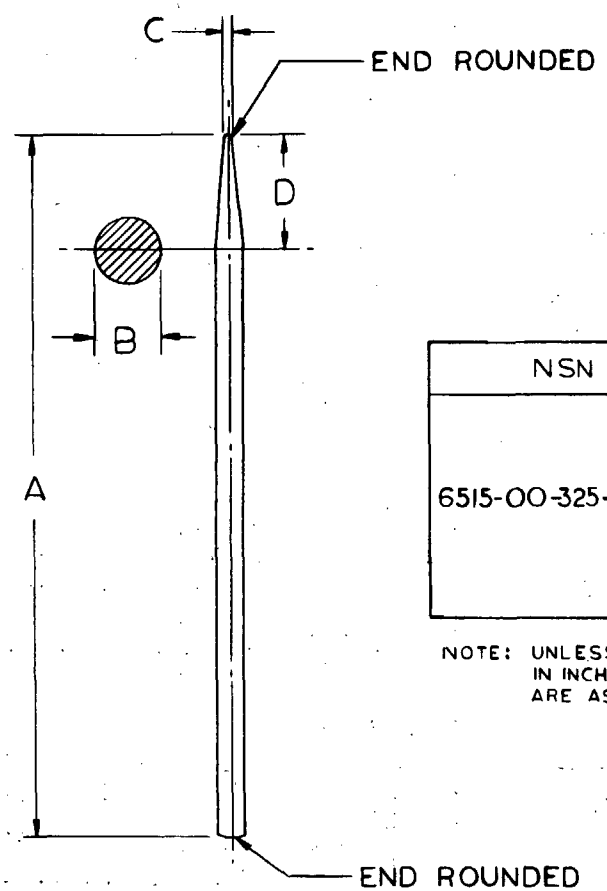

NSN	SIZE	A	B	C	D
6515-00-325-3400	1	$3\frac{7}{8}$	$\frac{1}{8}$	.046	$\frac{11}{16}$
	2			.032	$\frac{15}{16}$
	3			.015	$1\frac{1}{4}$
	TOL.	$\pm\frac{1}{4}$	$\pm\frac{1}{64}$	$\pm$.005	$\pm\frac{1}{16}$

NOTE: UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES AND TOLERANCES ON DIMENSIONS ARE AS SHOWN

DILATOR SET

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Shall be in accordance with GG-I-526.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one dilator set.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics. Unit of product shall be one dilator set.

Table II. Sampling for Tests

Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Composition analysis	3.2 and GG-I-526	GG-I-526	*	*
Hardness	3.3 and GG-I-526	GG-I-526	S-2	*
Dimensions	3.4	----	S-2	*
Boil test	GG-I-526	GG-I-526	S-2	*

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

* Acceptance number shall be zero for all sample sizes.
** Sufficient amount from each lot of metal used in the construction of the dilator sets shall be selected for composition analysis.

4.3 Examination. The dilator sets shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but shall not be limited to the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Instrument not free from sharp edges, rough areas, burrs, cracks, grind marks, or overlaps.
Minor	
201	Finish not as specified.
202	Instrument not permanently and legibly marked with either the name or trademark of the contractor.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One Dilator Set, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	144 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be applied.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IC-1.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566, PPP-B-676 or PPP-B-636, class domestic. Commercial colors are acceptable on intermediate cartons and closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Special requirements as specified in Table II of PPP-B-636 shall apply for fiberboard boxes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage or distribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The dilator sets are intended for use as a punctum dilator.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement document should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6515-00-325-3400	DILATOR SET, LACHRYMAL, Nettleship-Wilder, Set of 3

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

6.4 Supercession data. This specification includes requirements of Purchase Description No. 3, dated 27 March 1963 for FSN 6515-325-3400 DILATOR, SET, LACHRYMAL, Nettleship-Wilder, Set of 3.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing Activity:
Defense Supply Agency - DM

Project No. 6515-1807

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-D-37041

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:50Z
Check the source to verify that this is the current version before use.